
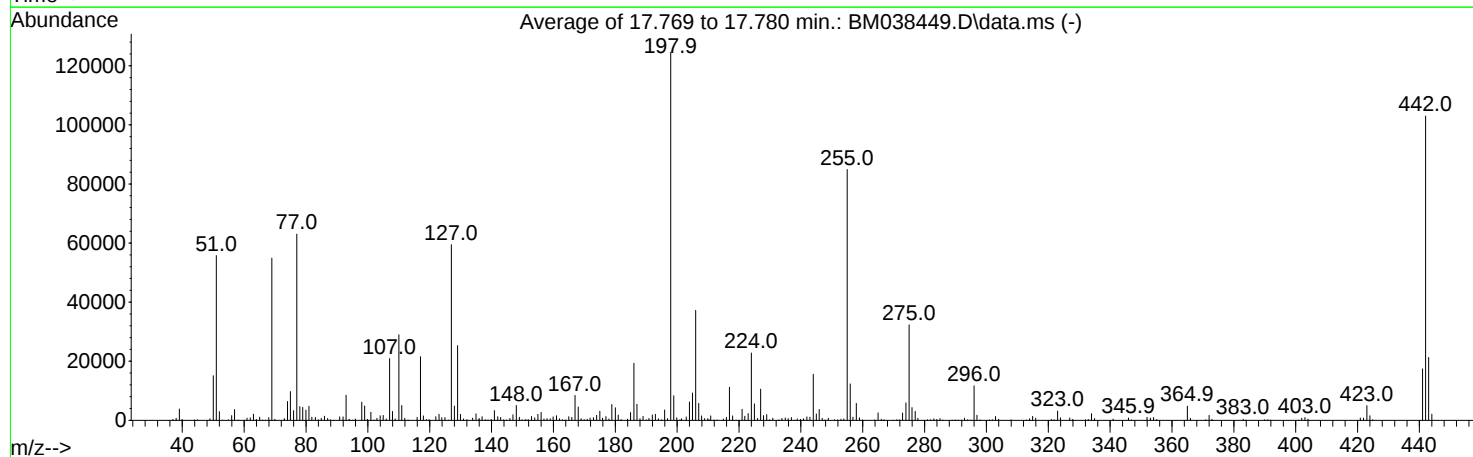


Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM011623\  
Data File : BM038449.D  
Acq On : 16 Jan 2023 12:34  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM011623.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Tue Jan 17 03:06:05 2023

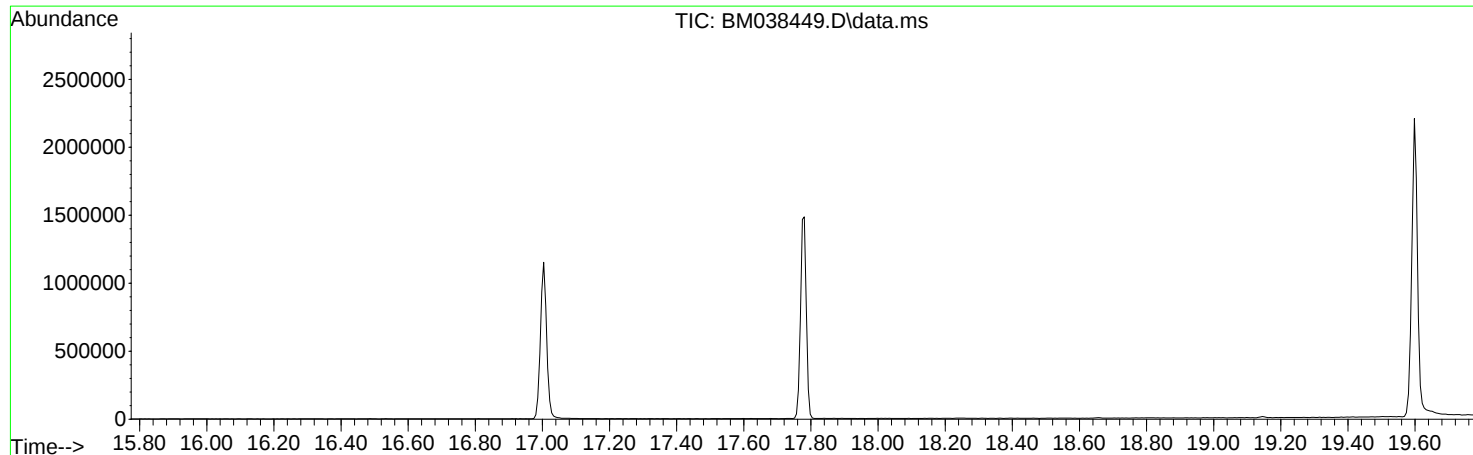




AutoFind: Scans 2479, 2480, 2481; Background Corrected with Scan 2473

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 44.8         | 55781      | PASS                |
| 68             | 69              | 0.00            | 2               | 1.6          | 904        | PASS                |
| 69             | 198             | 0.00            | 100             | 44.1         | 54927      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.6          | 353        | PASS                |
| 127            | 198             | 10              | 80              | 47.7         | 59448      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.4          | 557        | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 124536     | PASS                |
| 199            | 198             | 5               | 9               | 6.7          | 8328       | PASS                |
| 275            | 198             | 10              | 60              | 26.0         | 32322      | PASS                |
| 365            | 198             | 1               | 100             | 3.9          | 4806       | PASS                |
| 441            | 198             | 0.01            | 100             | 14.0         | 17437      | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 102987     | PASS                |
| 443            | 442             | 15              | 24              | 20.7         | 21268      | PASS                |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM011623\  
Data File : BM038449.D  
Acq On : 16 Jan 2023 12:34  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP

Quant Time: Jan 17 07:30:52 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM011623.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Jan 17 03:06:05 2023  
Response via : Initial Calibration

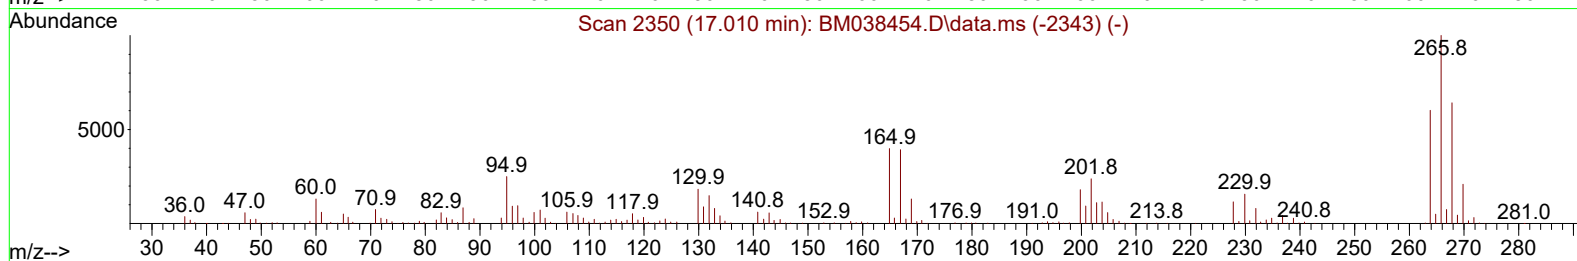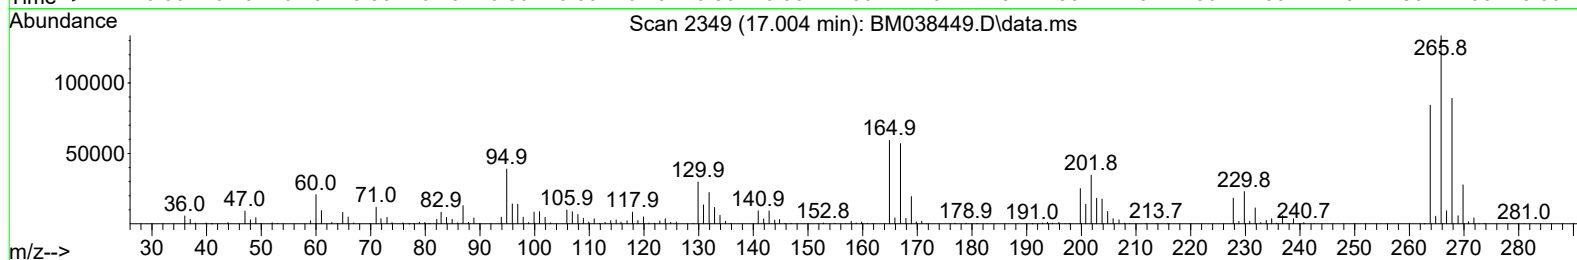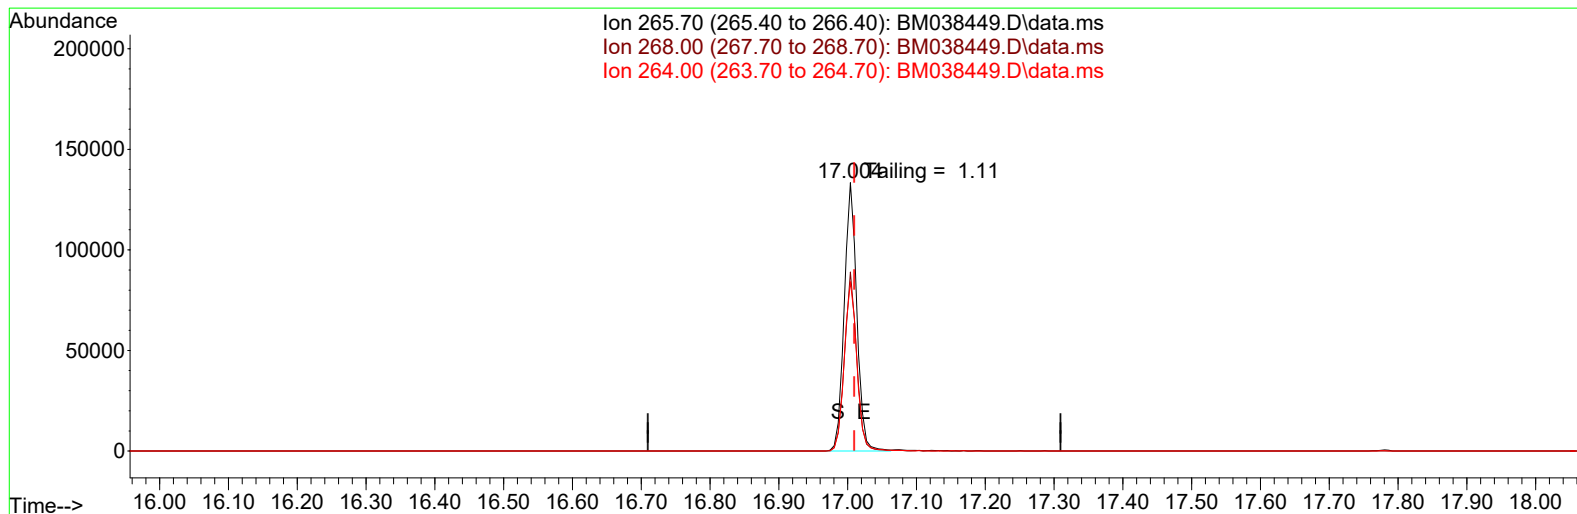

TIC: BM038449.D\data.ms

**(70) Pentachlorophenol (C)**

17.004min (-0.006) 0.00 ng




response 168979

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 64.20  | 66.73  |
| 264.00 | 60.20  | 63.10  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM011623\  
 Data File : BM038449.D  
 Acq On : 16 Jan 2023 12:34  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 DFTPP

Quant Time: Jan 17 07:30:52 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM011623.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Tue Jan 17 03:06:05 2023  
 Response via : Initial Calibration

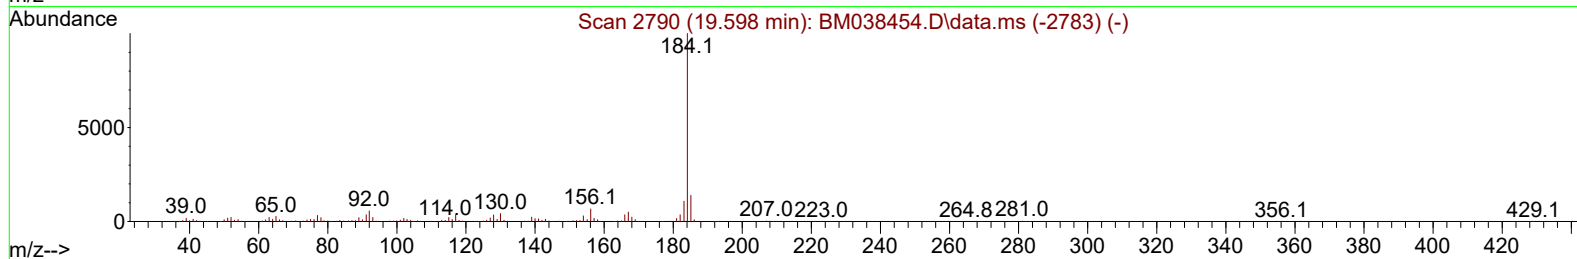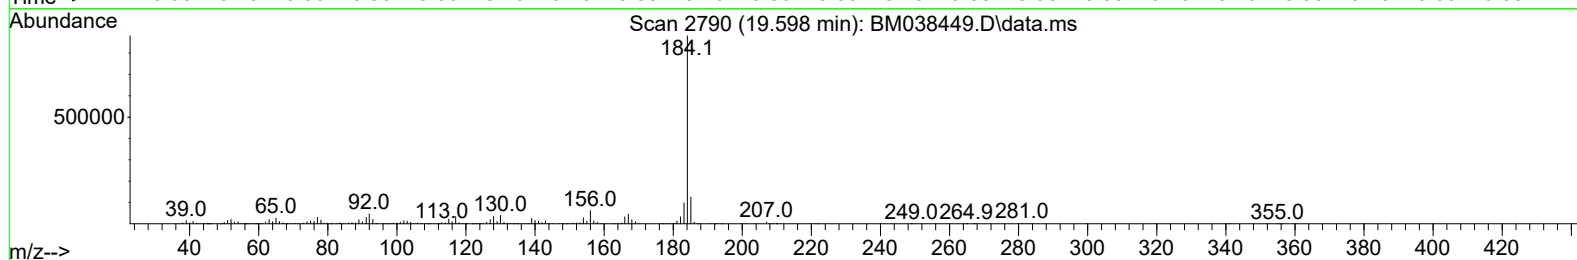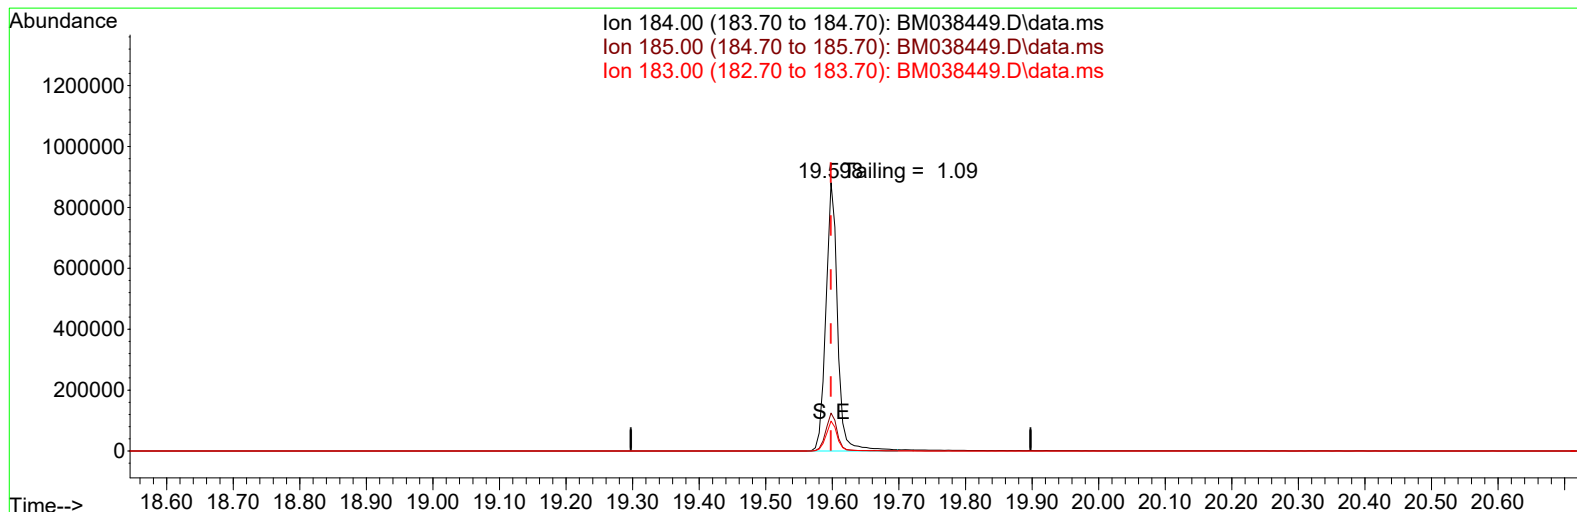

TIC: BM038449.D\data.ms

**(77) Benzidine**

**19.598min (+ 0.000) 0.00 ng**

**response 1081435**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 13.90  | 14.13  |
| 183.00 | 10.80  | 11.17  |
| 0.00   | 0.00   | 0.00   |

### DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 1/16/2023     | BNA_M            | <u>BM038449.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 573734           | 20.815             |
| DDD           | 4433             | 20.427             |
| DDE           | 0                | 19.9               |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 4433          | 578167           | 0.77               |
|               |                  |                    |

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP