

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011624\
 Data File : BM043845.D
 Acq On : 15 Jan 2024 17:59
 Operator : MA/JU
 Sample : PB158384BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK384

Quant Time: Jan 16 00:41:48 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM011024.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jan 10 15:40:11 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.950	152	7313	0.400	ng/ul	0.00
4) Naphthalene-d8	10.757	136	22975	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.592	164	13400	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.443	188	1875945	0.400	ng/ul	# 0.09
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.54
23) Perylene-d12	23.962	264	25150	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.355	96	47295	5.348	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.374	152	8982	0.270	ng/ul	0.00
18) Fluoranthene-d10	19.375	212	17164	0.000	ng/ul	0.00
Target Compounds						
						Qvalue
12) Fluorene	15.587	166	3935	0.066	ng/ul#	14
26) Benzo(a)pyrene	23.798	252	6699	0.070	ng/ul#	62


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011624\
Data File : BM043845.D
Acq On : 15 Jan 2024 17:59
Operator : MA/JU
Sample : PB158384BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK384

Quant Time: Jan 16 00:41:48 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM011024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 10 15:40:11 2024
Response via : Initial Calibration




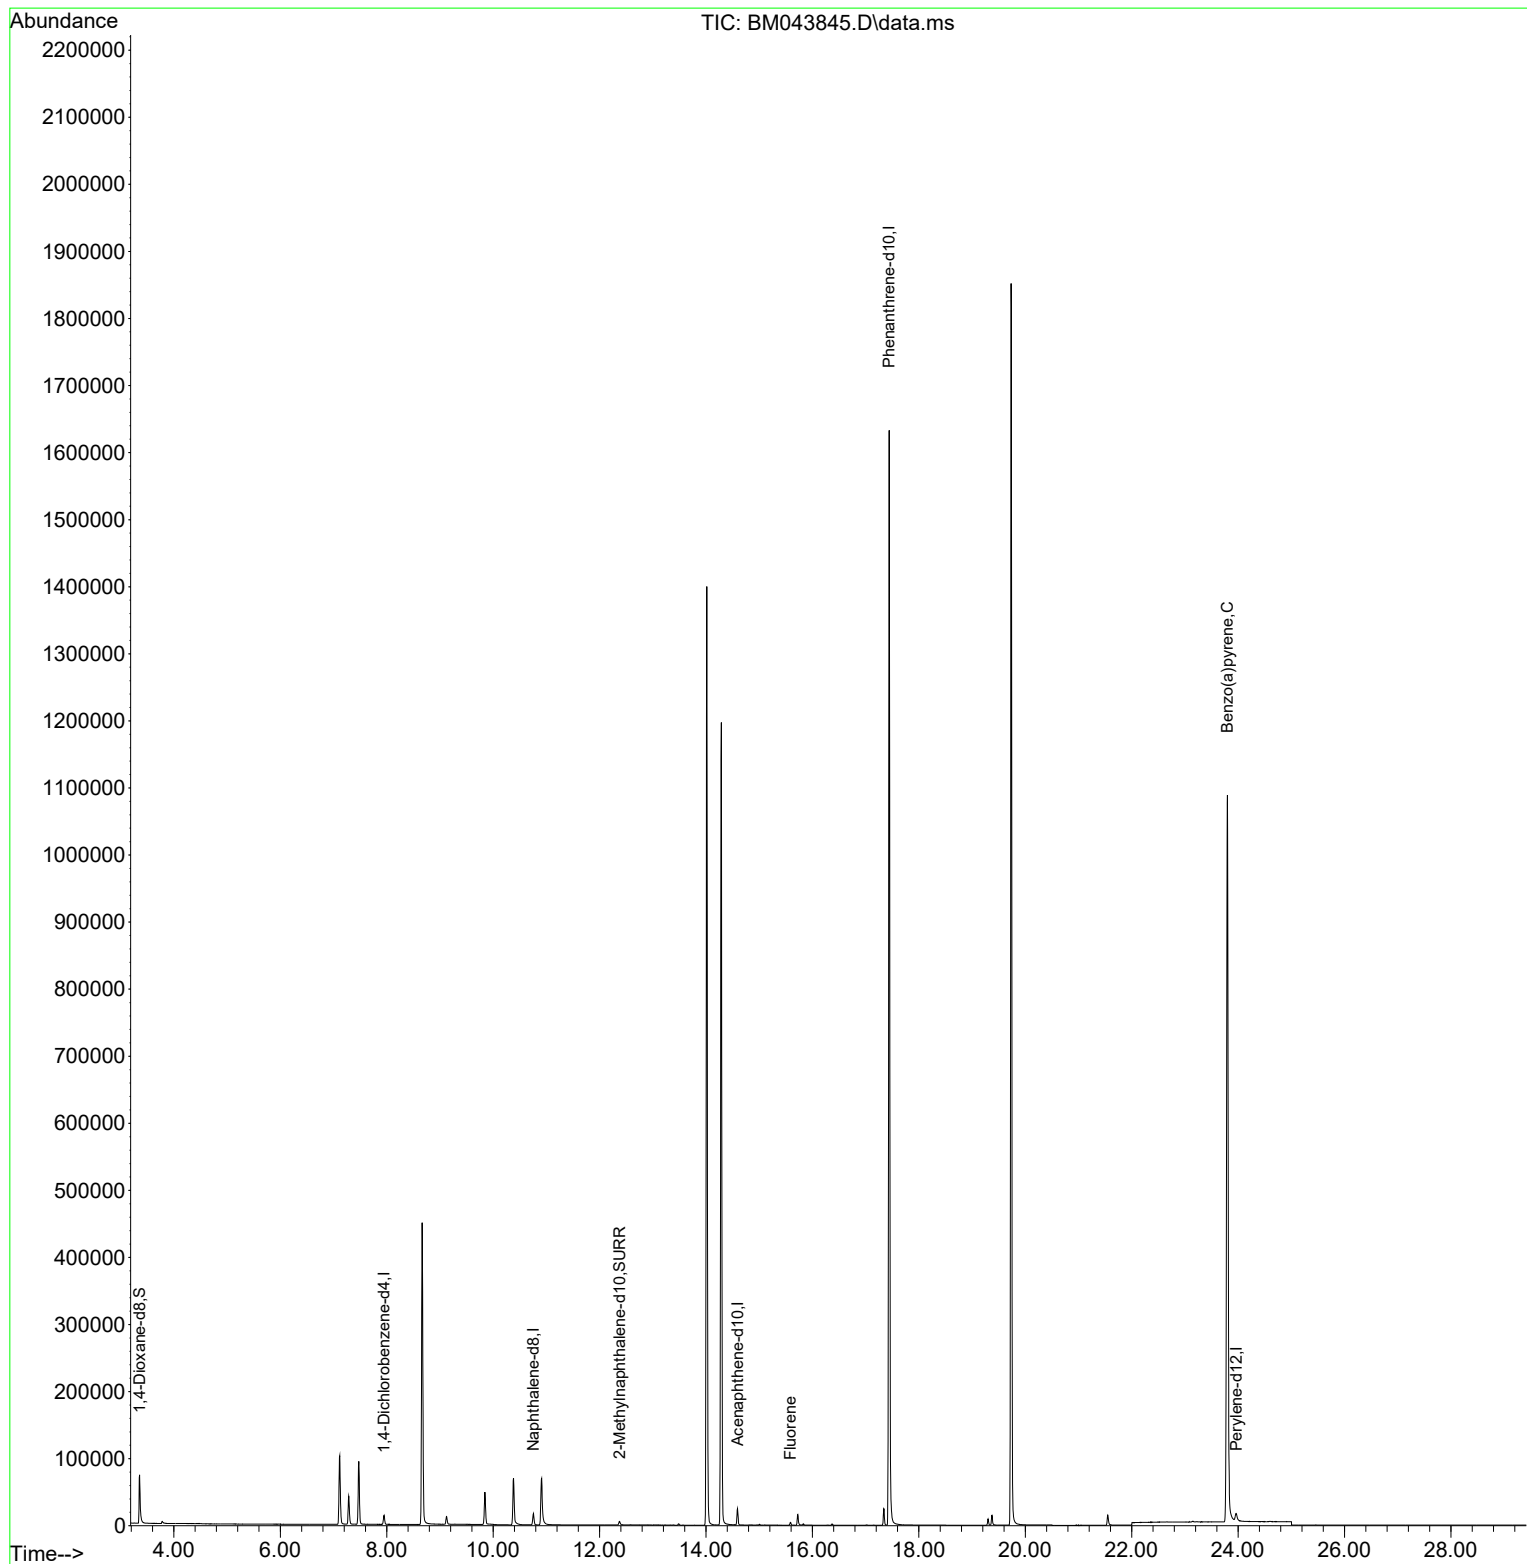


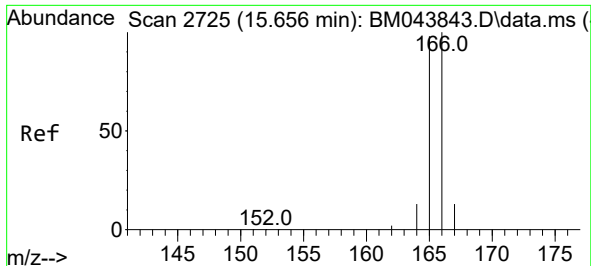

#12
Fluorene
Concen: 0.066 ng/ul
RT: 15.587 min Scan# 21
Delta R.T. -0.069 min
Lab File: BM043845.D
Acq: 15 Jan 2024 17:59

Instrument :
BNA_M
ClientSampleId :
SBLK384

Tgt Ion:166 Resp: 3935
Ion Ratio Lower Upper
166 100
165 7.9 79.4 119.2#
167 31.5 11.1 16.7#

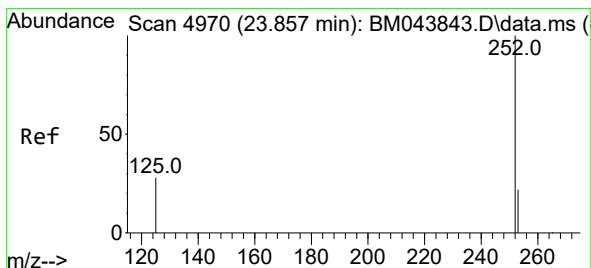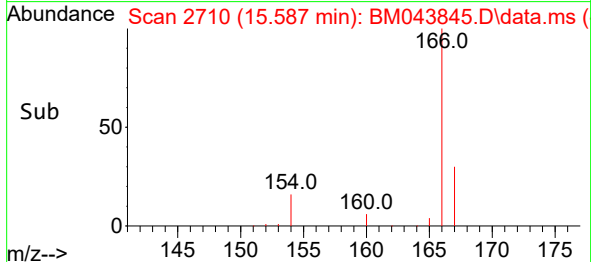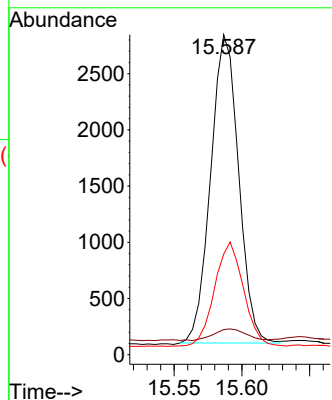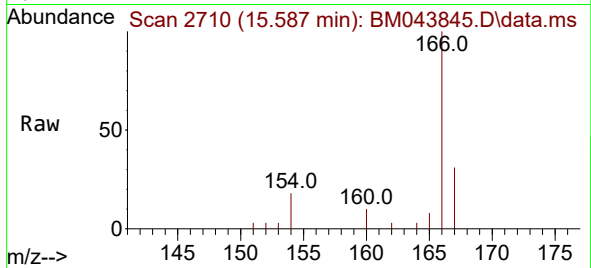

#26
Benzo(a)pyrene
Concen: 0.070 ng/ul
RT: 23.798 min Scan# 4950
Delta R.T. -0.067 min
Lab File: BM043845.D
Acq: 15 Jan 2024 17:59

Tgt Ion:252 Resp: 6699
Ion Ratio Lower Upper
252 100
253 47.7 20.8 31.2#
125 42.4 20.2 30.2#

