

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011624\
 Data File : BM043846.D
 Acq On : 15 Jan 2024 18:35
 Operator : MA/JU
 Sample : P1130-07
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AZ8

Quant Time: Jan 16 00:41:54 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM011024.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jan 10 15:40:11 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.950	152	6419	0.400	ng/ul	0.00
4) Naphthalene-d8	10.757	136	20451	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.592	164	12130	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.443	188	2253526	0.400	ng/ul	# 0.09
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.54
23) Perylene-d12	23.959	264	25153	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.355	96	32851	4.232	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.363	152	10136	0.343	ng/ul	0.00
18) Fluoranthene-d10	19.375	212	21093	0.000	ng/ul	0.00
Target Compounds						
						Qvalue
12) Fluorene	15.587	166	4633	0.086	ng/ul#	13
26) Benzo(a)pyrene	23.795	252	8586	0.089	ng/ul#	70


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011624\
Data File : BM043846.D
Acq On : 15 Jan 2024 18:35
Operator : MA/JU
Sample : P1130-07
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AZ8

Quant Time: Jan 16 00:41:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM011024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 10 15:40:11 2024
Response via : Initial Calibration

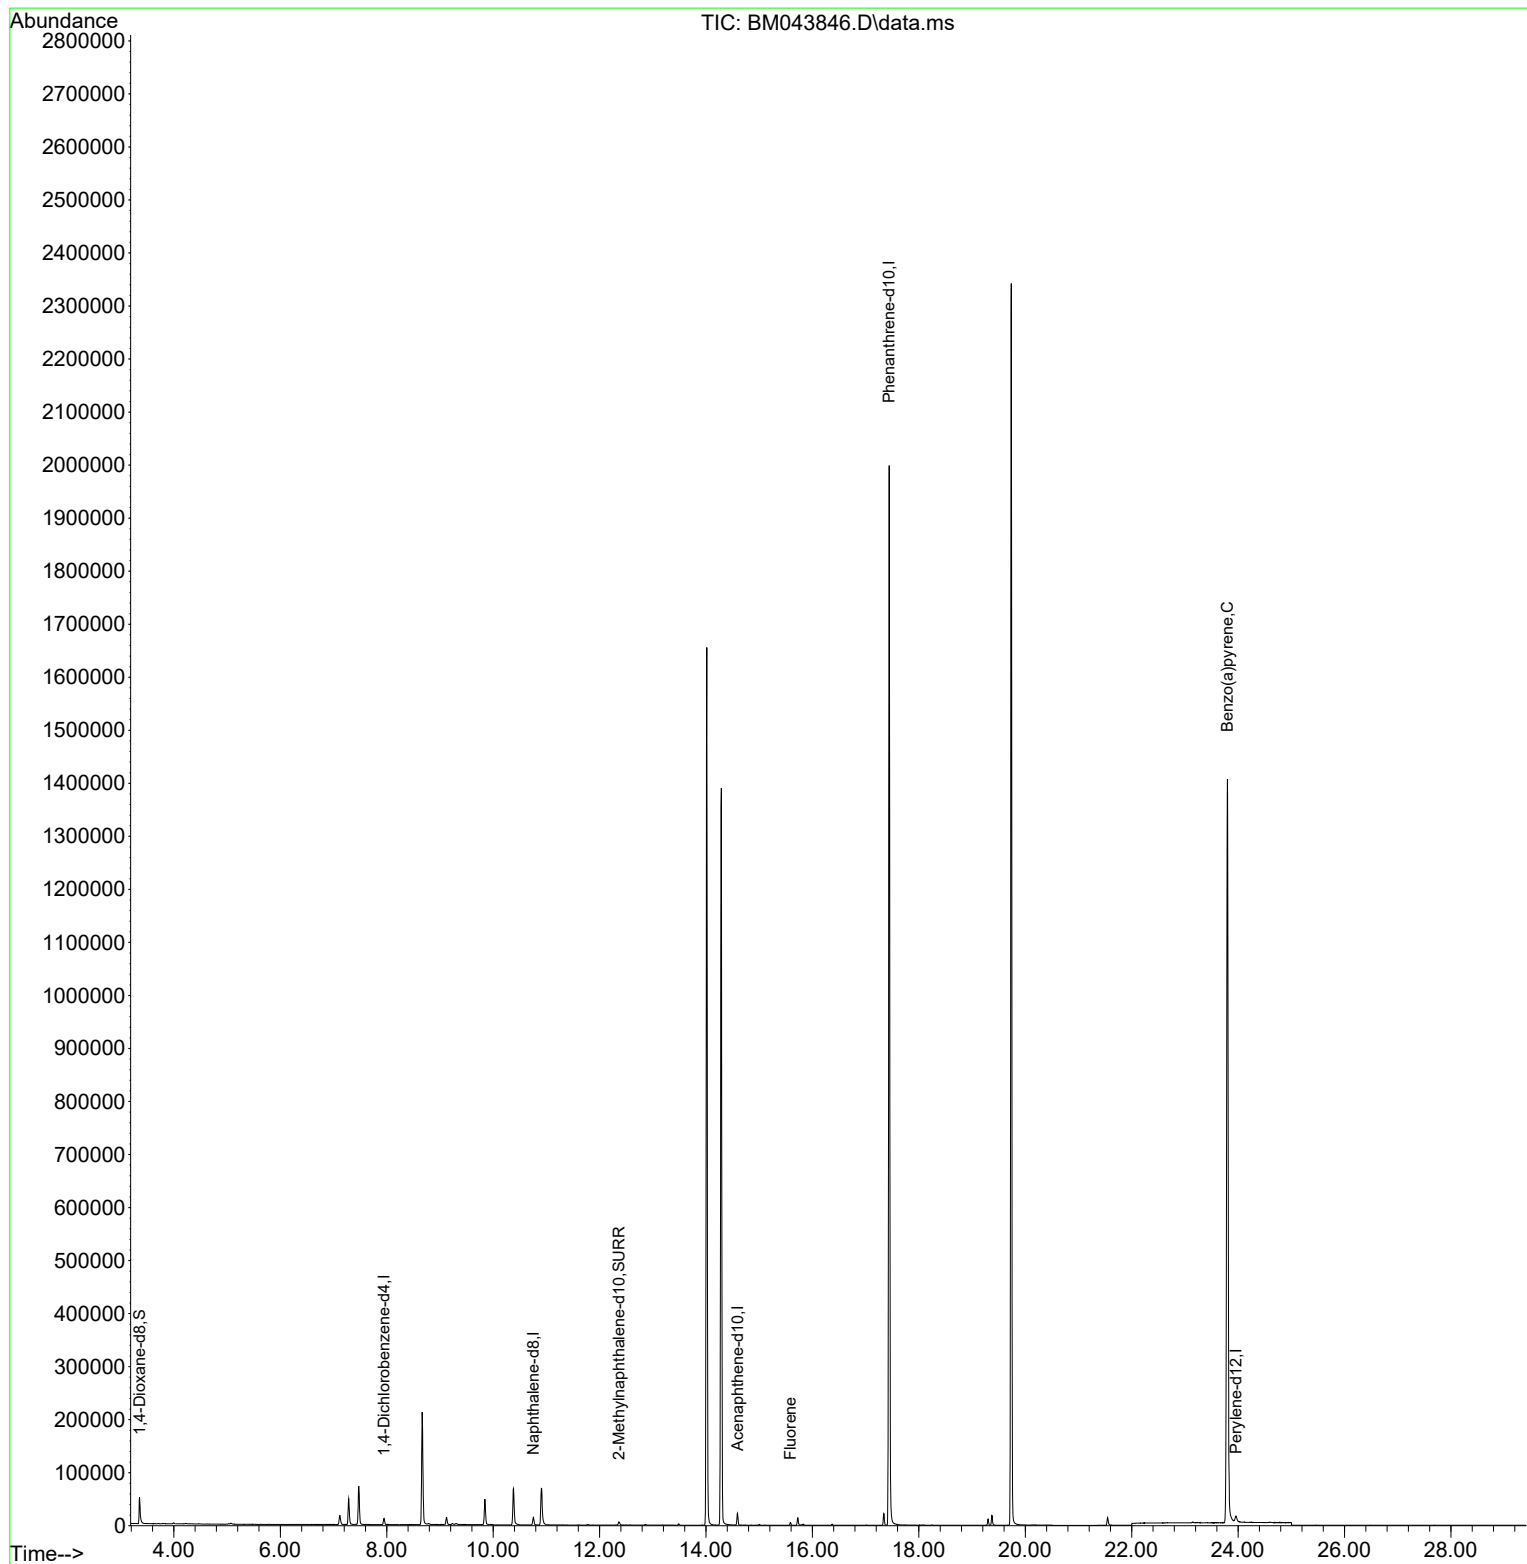

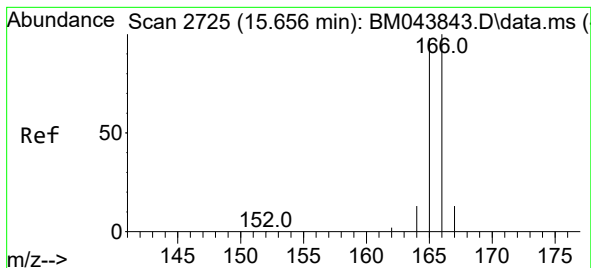

#12

Fluorene

Concen: 0.086 ng/ul

RT: 15.587 min Scan# 21

Delta R.T. -0.069 min

Lab File: BM043846.D

Acq: 15 Jan 2024 18:35

Instrument :

BNA_M

ClientSampleId :

C0AZ8





Tgt Ion:166 Resp: 4633

Ion Ratio Lower Upper

166 100

165 7.2 79.4 119.2#

167 32.0 11.1 16.7#

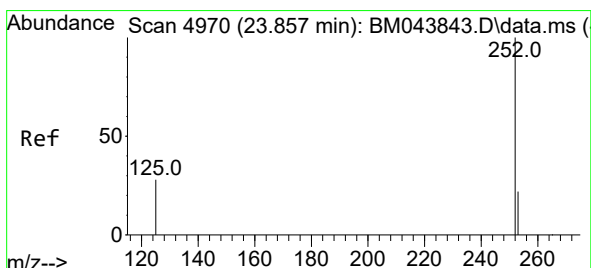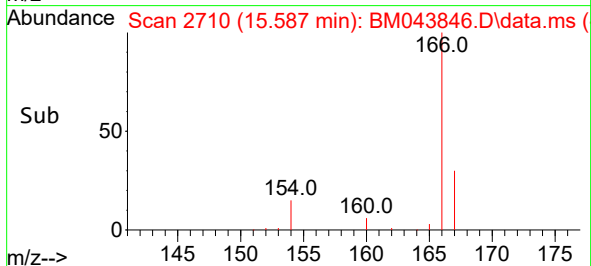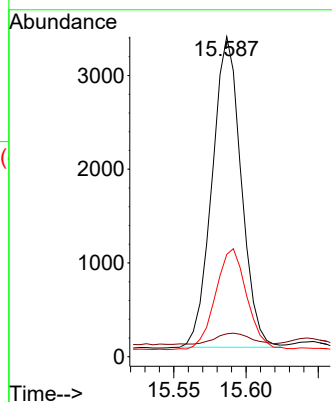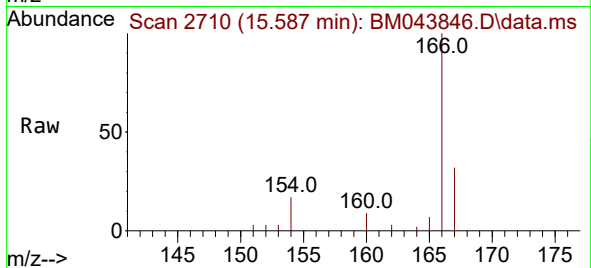

#26

Benzo(a)pyrene

Concen: 0.089 ng/ul

RT: 23.795 min Scan# 4949

Delta R.T. -0.070 min

Lab File: BM043846.D

Acq: 15 Jan 2024 18:35

Tgt Ion:252 Resp: 8586

Ion Ratio Lower Upper

252 100

253 43.3 20.8 31.2#

125 38.6 20.2 30.2#

