

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011624\
 Data File : BM043847.D
 Acq On : 15 Jan 2024 19:12
 Operator : MA/JU
 Sample : P1091-14
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0B45

Quant Time: Jan 16 00:42:00 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM011024.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jan 10 15:40:11 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.950	152	5343	0.400	ng/ul	0.00
4) Naphthalene-d8	10.757	136	16881	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.592	164	9878	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.443	188	2270805	0.400	ng/ul	# 0.09
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.54
23) Perylene-d12	23.959	264	21086	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.355	96	31583	4.888	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.368	152	8420	0.345	ng/ul	0.00
18) Fluoranthene-d10	19.371	212	22015	0.000	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.587	166	4081	0.093	ng/ul#	14
26) Benzo(a)pyrene	23.798	252	8514	0.106	ng/ul#	62


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011624\
Data File : BM043847.D
Acq On : 15 Jan 2024 19:12
Operator : MA/JU
Sample : P1091-14
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0B45

Quant Time: Jan 16 00:42:00 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM011024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 10 15:40:11 2024
Response via : Initial Calibration




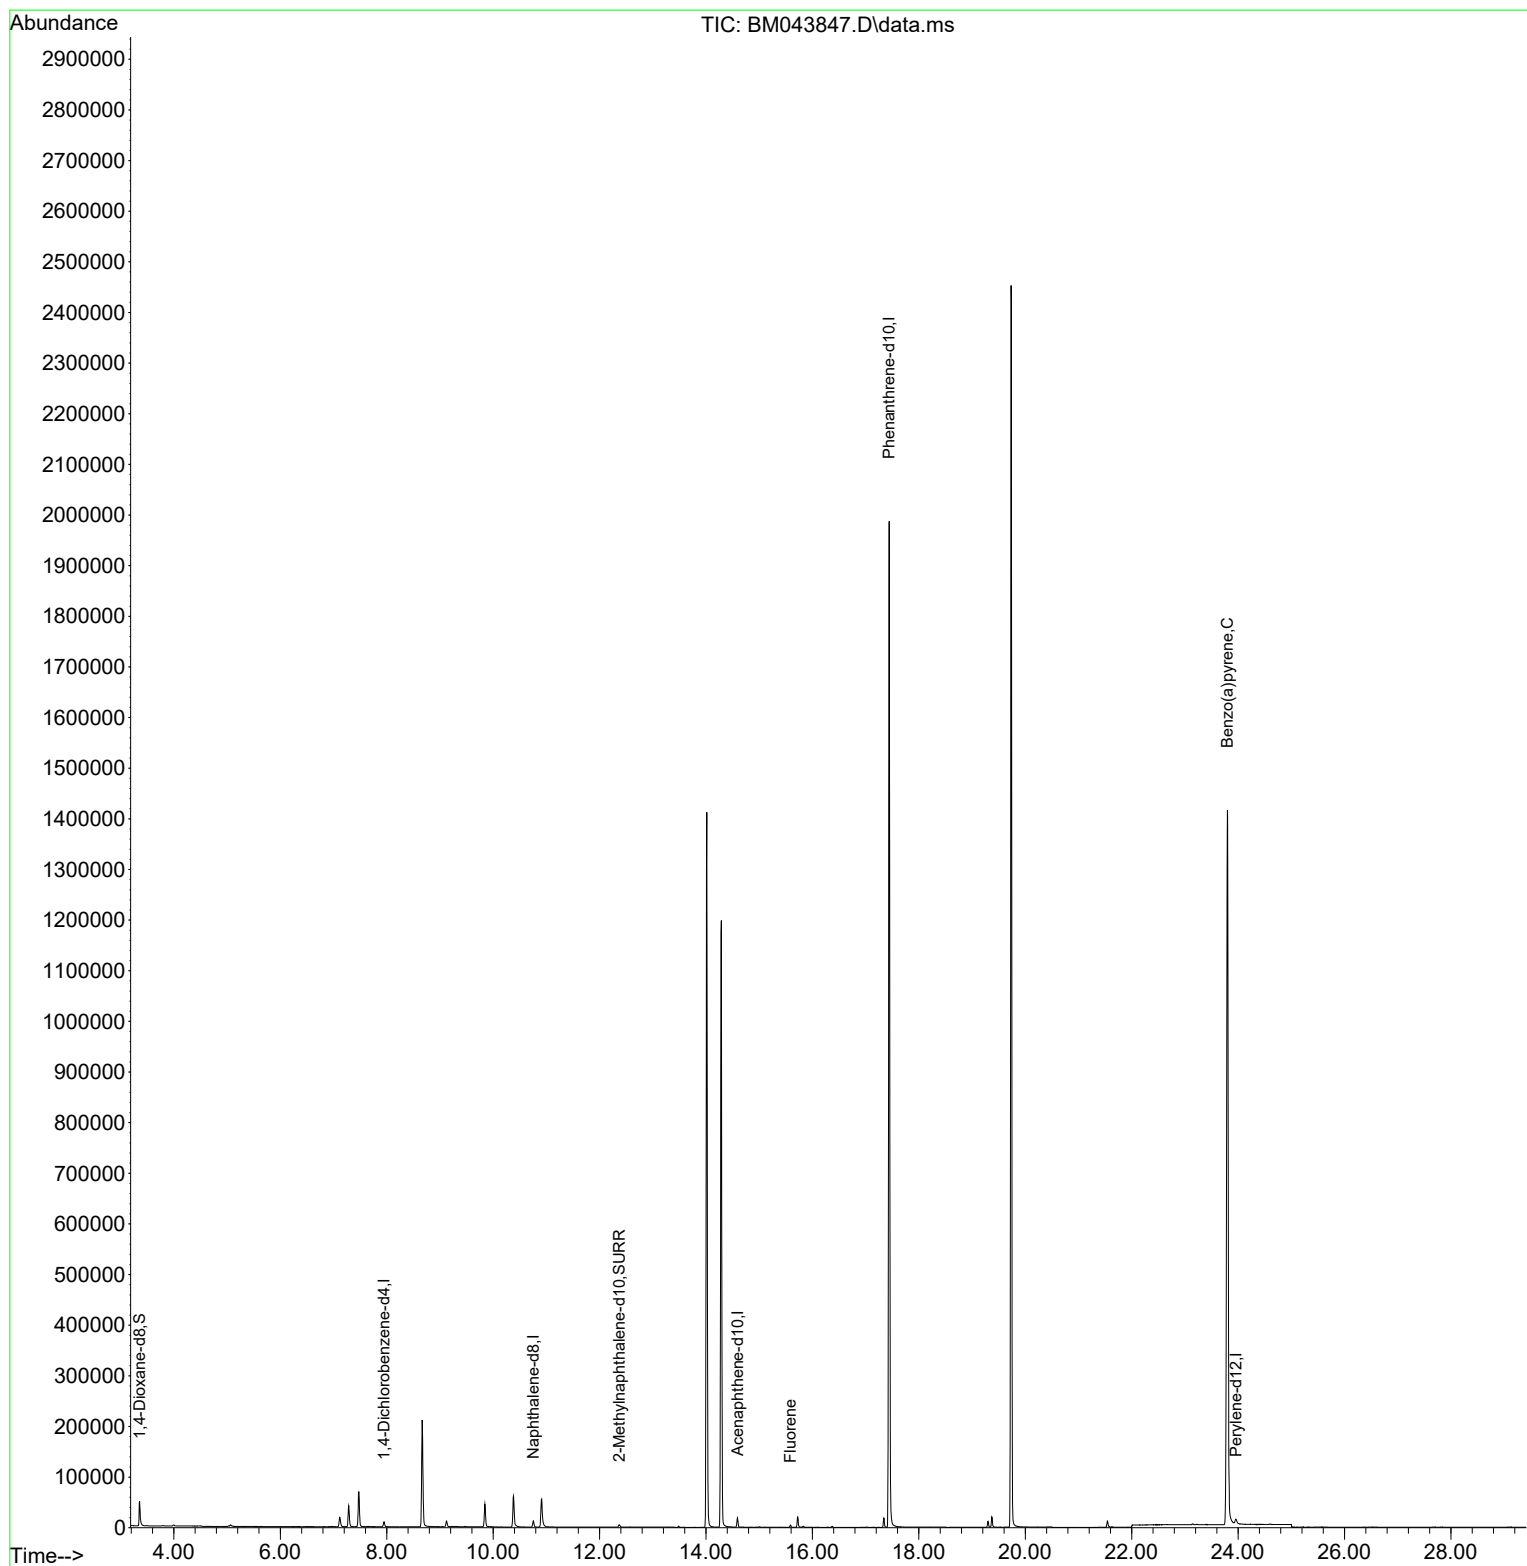


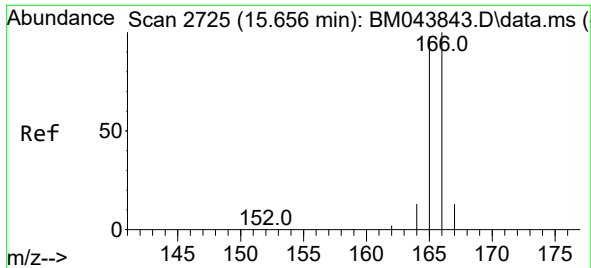

#12
Fluorene
Concen: 0.093 ng/ul
RT: 15.587 min Scan# 21
Delta R.T. -0.069 min
Lab File: BM043847.D
Acq: 15 Jan 2024 19:12

Instrument :
BNA_M
ClientSampleId :
C0B45

Tgt Ion:166 Resp: 4081
Ion Ratio Lower Upper
166 100
165 7.8 79.4 119.2#
167 32.6 11.1 16.7#

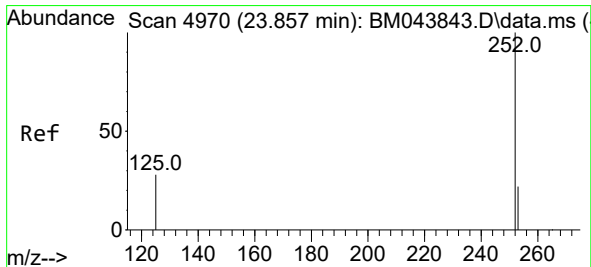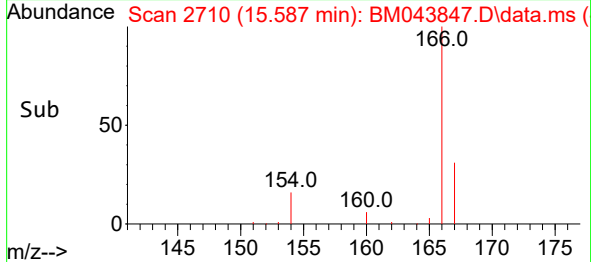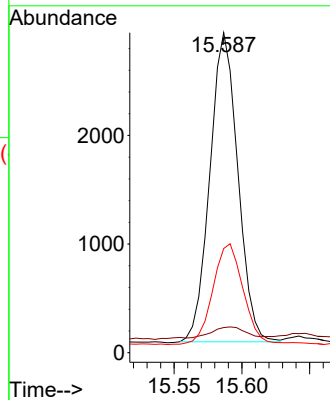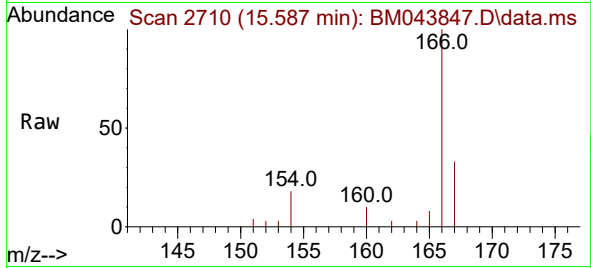

#26
Benzo(a)pyrene
Concen: 0.106 ng/ul
RT: 23.798 min Scan# 4950
Delta R.T. -0.067 min
Lab File: BM043847.D
Acq: 15 Jan 2024 19:12

Tgt Ion:252 Resp: 8514
Ion Ratio Lower Upper
252 100
253 43.5 20.8 31.2#
125 45.8 20.2 30.2#

