

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011624\
 Data File : BM043849.D
 Acq On : 15 Jan 2024 20:24
 Operator : MA/JU
 Sample : P1091-16
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0B38

Quant Time: Jan 16 00:42:12 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM011024.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jan 10 15:40:11 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.950	152	6423	0.400	ng/ul	0.00
4) Naphthalene-d8	10.757	136	20000	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.592	164	12182	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.443	188	2115371	0.400	ng/ul	# 0.09
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.54
23) Perylene-d12	23.959	264	22748	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.355	96	33658	4.334	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.352	152	9458	0.327	ng/ul	-0.02
18) Fluoranthene-d10	19.371	212	20752	0.000	ng/ul	0.00
Target Compounds						
						Qvalue
12) Fluorene	15.587	166	4111	0.076	ng/ul#	14
26) Benzo(a)pyrene	23.793	252	7761	0.089	ng/ul#	66


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011624\
Data File : BM043849.D
Acq On : 15 Jan 2024 20:24
Operator : MA/JU
Sample : P1091-16
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0B38

Quant Time: Jan 16 00:42:12 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM011024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 10 15:40:11 2024
Response via : Initial Calibration

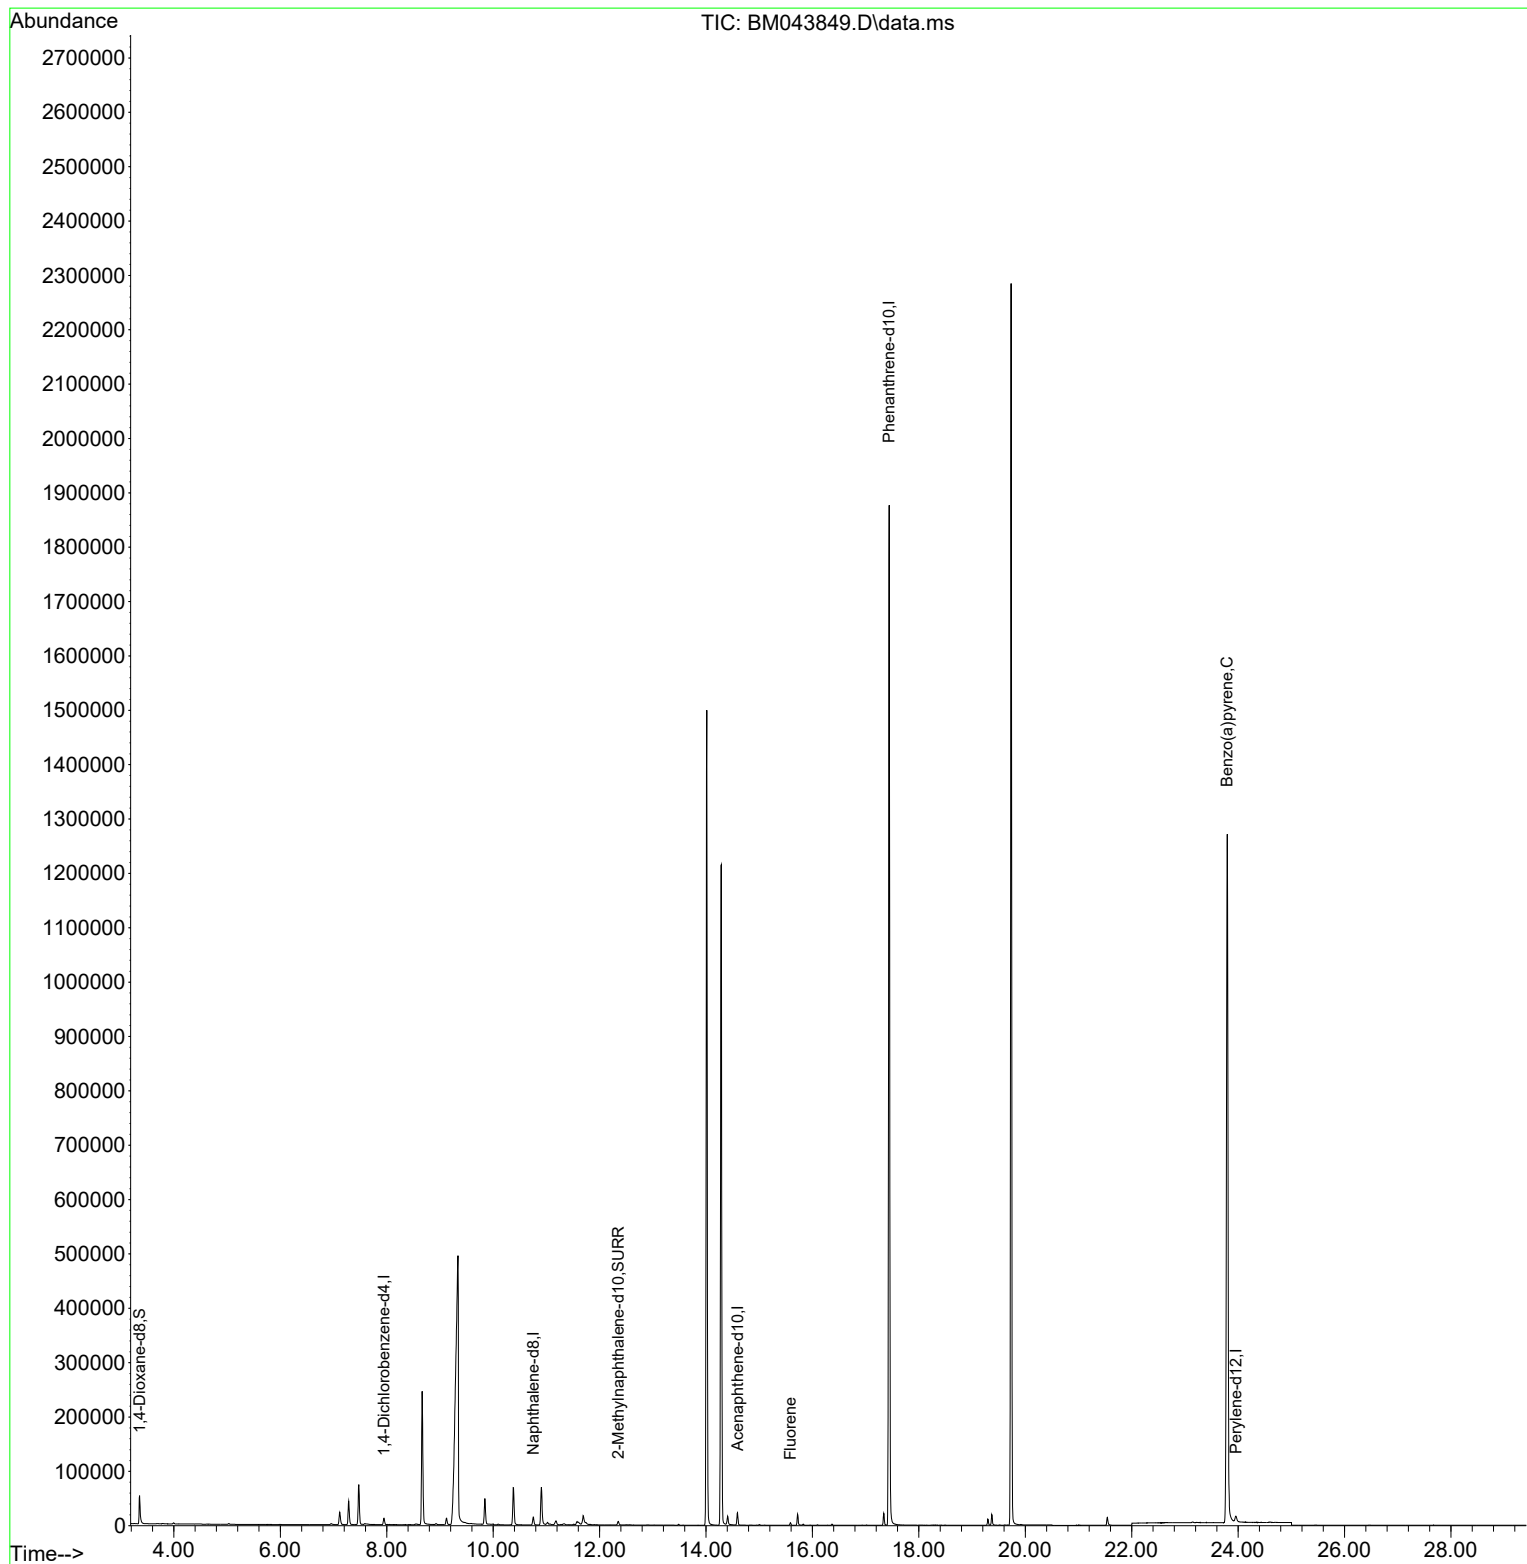

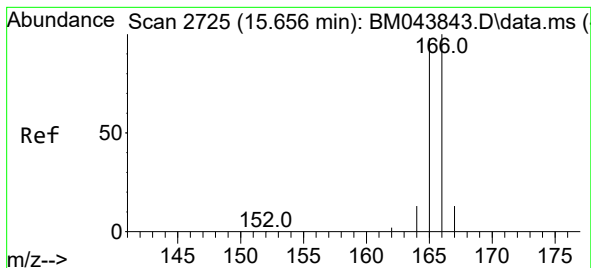

#12

Fluorene

Concen: 0.076 ng/ul

RT: 15.587 min Scan# 21

Delta R.T. -0.069 min

Lab File: BM043849.D

Acq: 15 Jan 2024 20:24

Instrument :

BNA_M

ClientSampleId :

C0B38





Tgt Ion:166 Resp: 4111

Ion Ratio Lower Upper

166 100

165 8.1 79.4 119.2#

167 32.4 11.1 16.7#

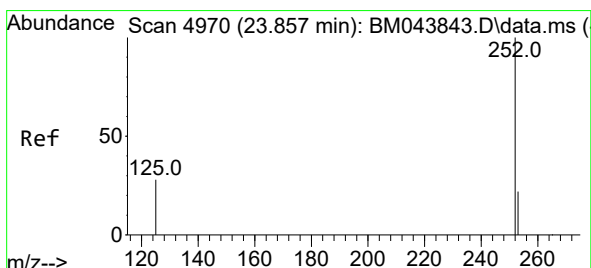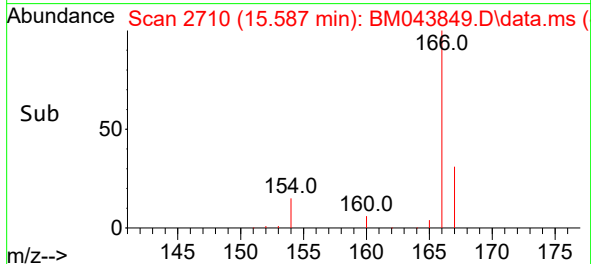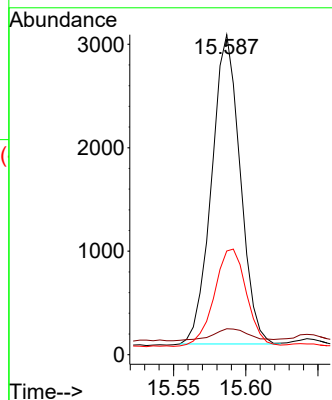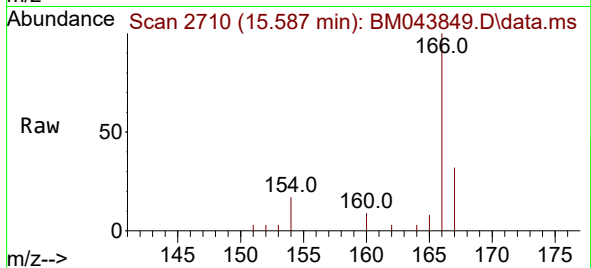

#26

Benzo(a)pyrene

Concen: 0.089 ng/ul

RT: 23.793 min Scan# 4948

Delta R.T. -0.073 min

Lab File: BM043849.D

Acq: 15 Jan 2024 20:24

Tgt Ion:252 Resp: 7761

Ion Ratio Lower Upper

252 100

253 43.5 20.8 31.2#

125 42.0 20.2 30.2#

