

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011624\
 Data File : BM043851.D
 Acq On : 15 Jan 2024 21:36
 Operator : MA/JU
 Sample : PB158427BS
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SLCS427

Quant Time: Jan 16 00:42:24 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM011024.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jan 10 15:40:11 2024
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.954	152	3	0.400	ng/ul	# 0.00
4) Naphthalene-d8	10.752	136	11	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.574	164	4	0.400	ng/ul	#-0.03
13) Phenanthrene-d10	17.358	188	39	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.542	240	313	0.400	ng/ul	# 0.00
23) Perylene-d12	23.991	264	122	0.400	ng/ul	# 0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.360	96	4625	1274.950	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.374	152	8268	520.046	ng/ul	0.00
18) Fluoranthene-d10	19.380	212	17126	16.923	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.393	88	14584	3780.686	ng/ul#	83
5) Naphthalene	10.834	128	16964	537.123	ng/ul	99
7) 2-Methylnaphthalene	12.445	142	10964	528.322	ng/ul	100
8) 1-Methylnaphthalene	12.654	142	10922	518.373	ng/ul	99
10) Acenaphthylene	14.328	152	18811	877.448	ng/ul	99
11) Acenaphthene	14.661	153	13693	878.524	ng/ul	99
12) Fluorene	15.661	166	15584	872.627	ng/ul	99
14) Pentachlorophenol	17.016	266	3925	317.538	ng/ul	100
15) Phenanthrene	17.400	178	23981	193.602	ng/ul	98
16) Anthracene	17.498	178	23334	197.862	ng/ul	99
19) Fluoranthene	19.413	202	27322	17.631	ng/ul	98
20) Pyrene	19.775	202	28265	17.510	ng/ul	98
21) Benzo(a)anthracene	21.533	228	20659	15.210	ng/ul	100
22) Chrysene	21.583	228	25097	17.156	ng/ul	99
24) Benzo(b)fluoranthene	23.231	252	18067	36.334	ng/ul	97
25) Benzo(k)fluoranthene	23.281	252	24763	45.150	ng/ul#	95
26) Benzo(a)pyrene	23.874	252	21786	46.755	ng/ul	97
27) Indeno(1,2,3-cd)pyrene	26.502	276	26920	45.678	ng/ul#	99
28) Dibenzo(a,h)anthracene	26.522	278	20583	45.082	ng/ul	97
29) Benzo(g,h,i)perylene	27.273	276	22563	45.781	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011624\
 Data File : BM043851.D
 Acq On : 15 Jan 2024 21:36
 Operator : MA/JU
 Sample : PB158427BS
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampleId :
 SLCS427


Quant Time: Jan 16 00:42:24 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM011024.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jan 10 15:40:11 2024
 Response via : Initial Calibration

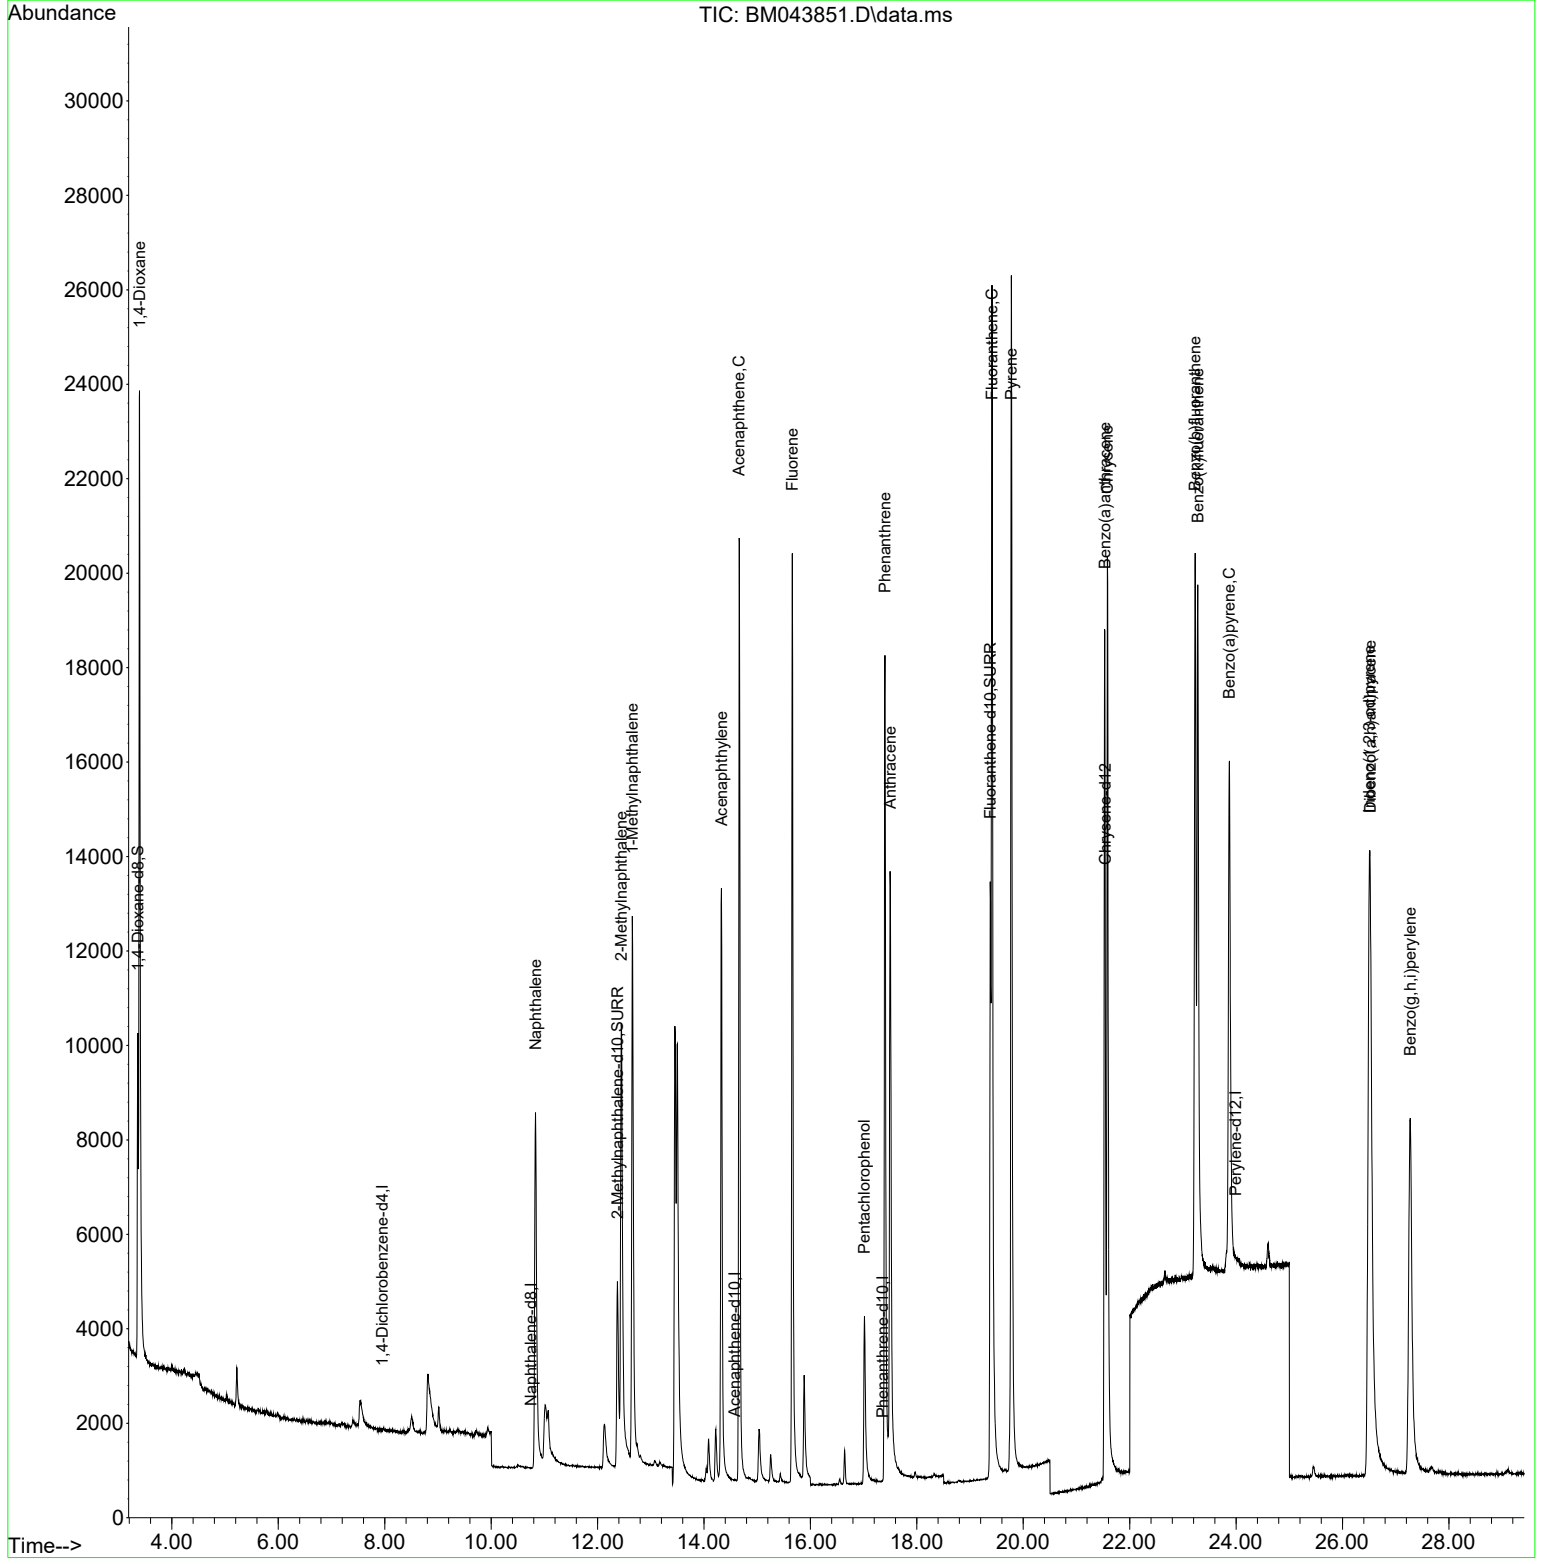






#2
 1,4-Dioxane
 Concen: 3780.686 ng/ul
 RT: 3.393 min Scan# 50
 Delta R.T. -0.004 min
 Lab File: BM043851.D
 Acq: 15 Jan 2024 21:36

Instrument :
 BNA_M
 ClientSampleId :
 SLCS427



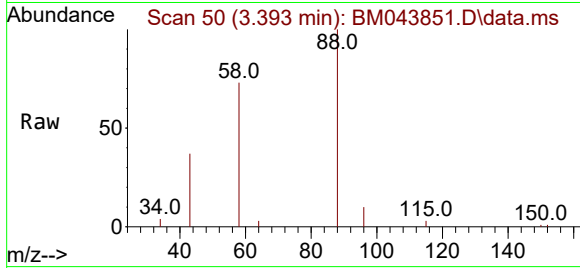



Tgt Ion: 88 Resp: 14584
 Ion Ratio Lower Upper
 88 100
 43 37.4 42.1 63.1#
 58 72.9 50.2 75.2

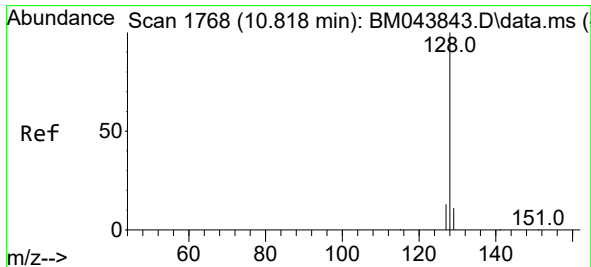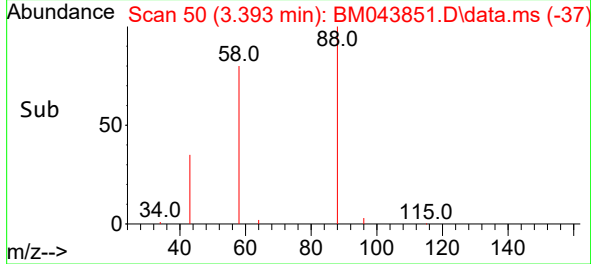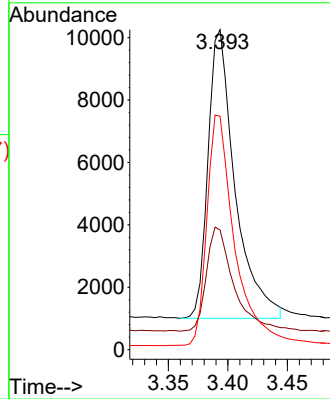

#5
 Naphthalene
 Concen: 537.123 ng/ul
 RT: 10.834 min Scan# 1771
 Delta R.T. 0.011 min
 Lab File: BM043851.D
 Acq: 15 Jan 2024 21:36

Tgt Ion: 128 Resp: 16964
 Ion Ratio Lower Upper
 128 100
 129 12.0 9.4 14.0
 127 13.8 10.6 15.8


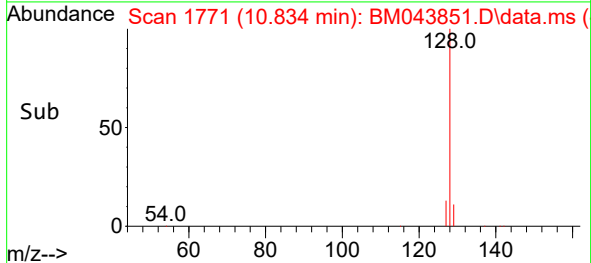
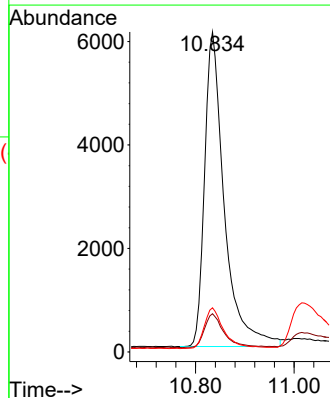
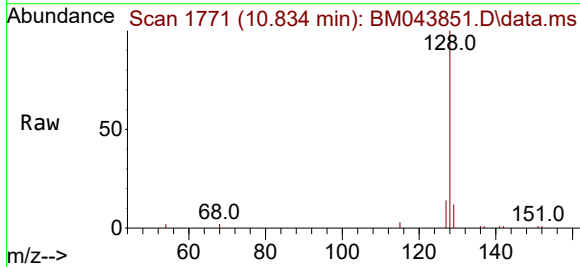




#7
 2-Methylnaphthalene
 Concen: 528.322 ng/ul
 RT: 12.445 min Scan# 2064
 Delta R.T. 0.006 min
 Lab File: BM043851.D
 Acq: 15 Jan 2024 21:36




Instrument : BNA_M
 ClientSampleId : SLCS427


Tgt Ion:142 Resp: 10964
 Ion Ratio Lower Upper
 142 100
 141 91.1 72.7 109.1

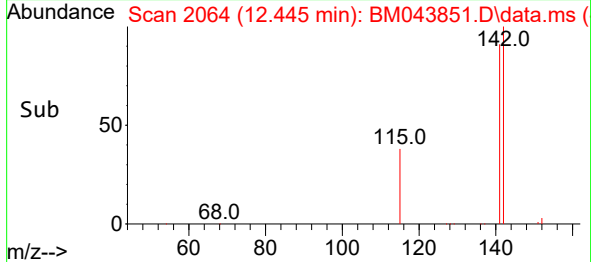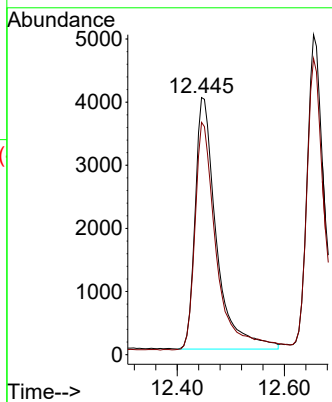

#8
 1-Methylnaphthalene
 Concen: 518.373 ng/ul
 RT: 12.654 min Scan# 2102
 Delta R.T. 0.000 min
 Lab File: BM043851.D
 Acq: 15 Jan 2024 21:36


Tgt Ion:142 Resp: 10922
 Ion Ratio Lower Upper
 142 100
 141 92.6 73.0 109.6

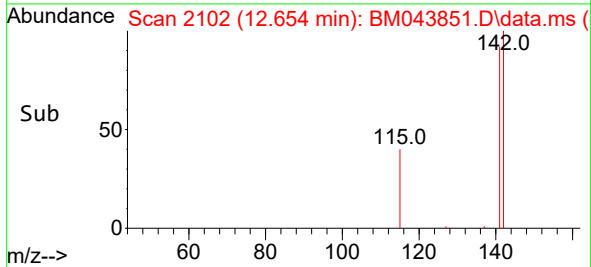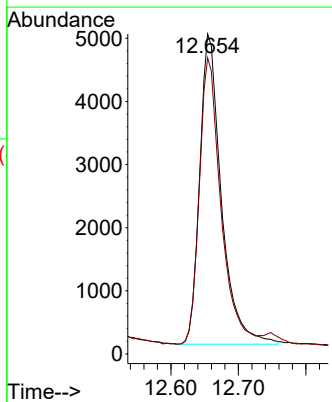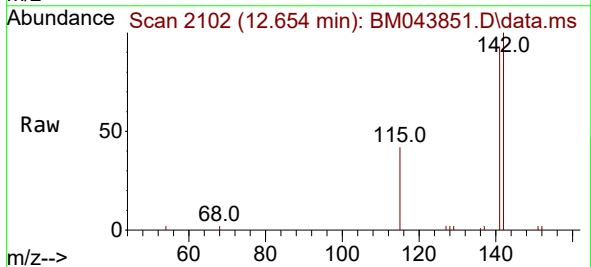

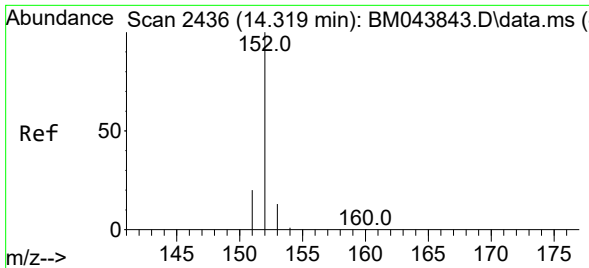




#10
 Acenaphthylene
 Concen: 877.448 ng/ul
 RT: 14.328 min Scan# 2438
 Delta R.T. 0.005 min
 Lab File: BM043851.D
 Acq: 15 Jan 2024 21:36

Instrument :
 BNA_M
 ClientSampleId :
 SLCS427

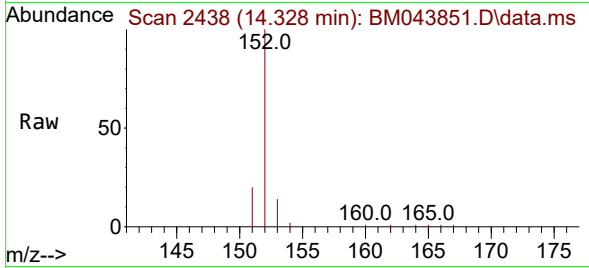

Tgt Ion:152 Resp: 18811




Ion	Ratio	Lower	Upper
152	100		
151	20.3	16.0	24.0
153	14.0	10.6	16.0

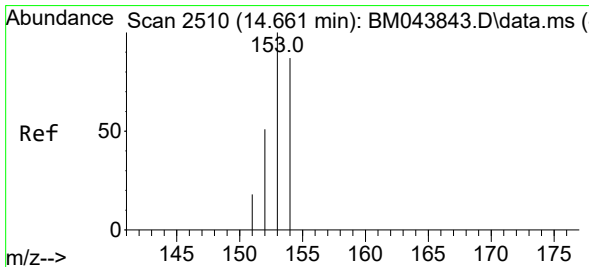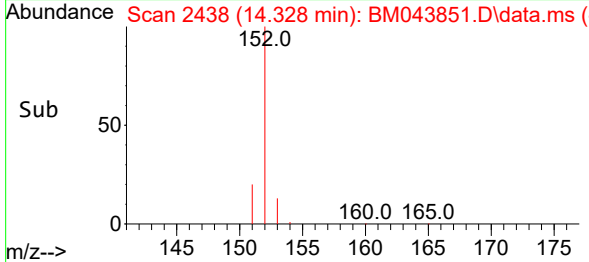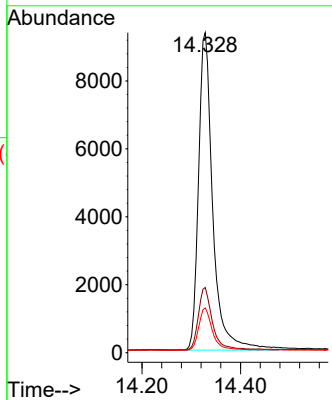


#11
 Acenaphthene
 Concen: 878.524 ng/ul
 RT: 14.661 min Scan# 2510
 Delta R.T. 0.000 min
 Lab File: BM043851.D
 Acq: 15 Jan 2024 21:36

Tgt Ion:153 Resp: 13693


Ion	Ratio	Lower	Upper
153	100		
152	52.6	40.6	61.0
154	87.5	69.4	104.2

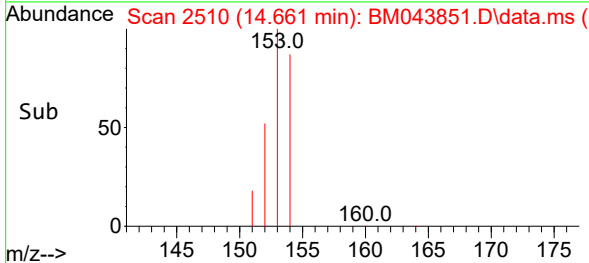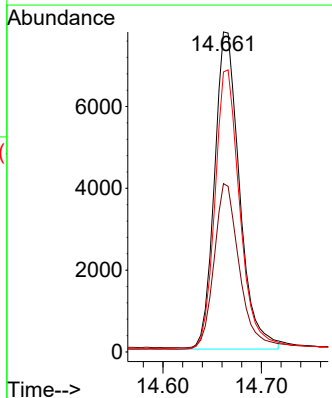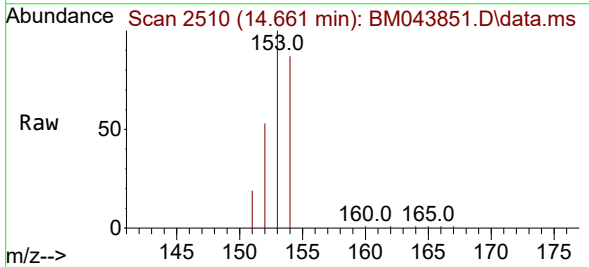



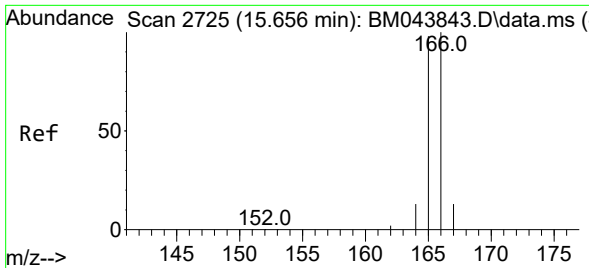


#12
 Fluorene
 Concen: 872.627 ng/ul
 RT: 15.661 min Scan# 21
 Delta R.T. 0.005 min
 Lab File: BM043851.D
 Acq: 15 Jan 2024 21:36

Instrument :
 BNA_M
 ClientSampleId :
 SLCS427



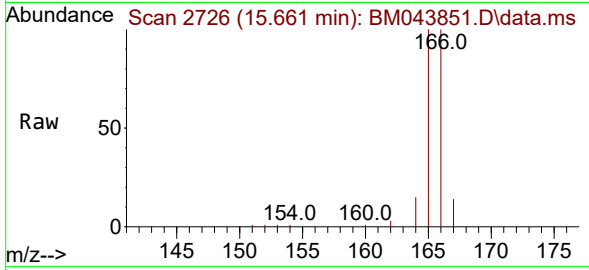



Tgt Ion:166 Resp: 15584
 Ion Ratio Lower Upper
 166 100
 165 100.0 79.4 119.2
 167 13.8 11.1 16.7

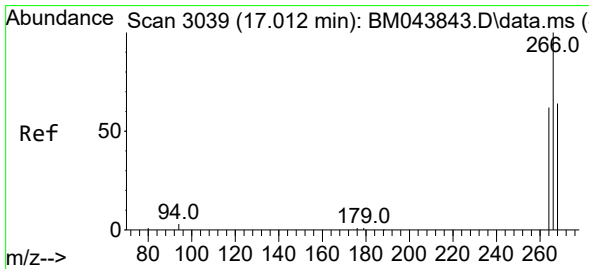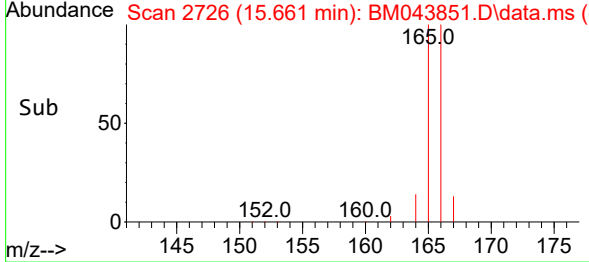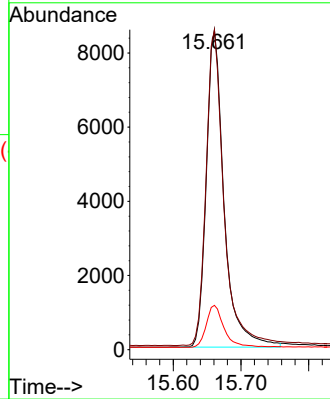

#14
 Pentachlorophenol
 Concen: 317.538 ng/ul
 RT: 17.016 min Scan# 3040
 Delta R.T. 0.000 min
 Lab File: BM043851.D
 Acq: 15 Jan 2024 21:36

Tgt Ion:266 Resp: 3925
 Ion Ratio Lower Upper
 266 100
 264 62.5 50.4 75.6
 268 65.3 52.2 78.2


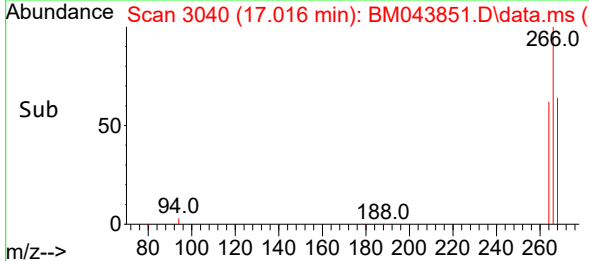
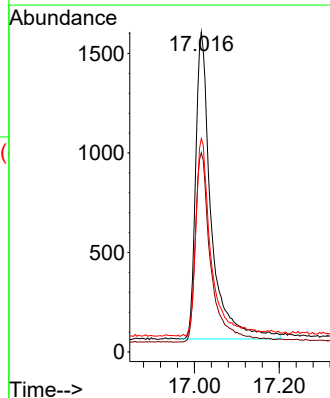
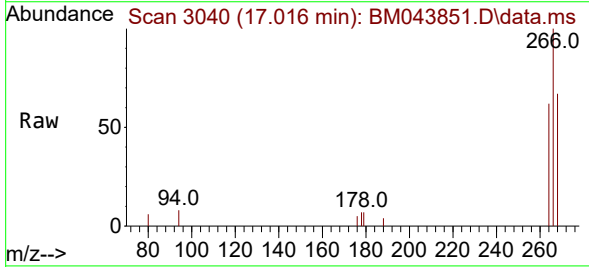




#15
 Phenanthrene
 Concen: 193.602 ng/u1
 RT: 17.400 min Scan# 3129
 Delta R.T. 0.004 min
 Lab File: BM043851.D
 Acq: 15 Jan 2024 21:36




Instrument :
 BNA_M
 ClientSampleId :
 SLCS427


Tgt Ion	Resp	Lower	Upper
178	100		
179	16.1	12.5	18.7
176	20.7	15.9	23.9

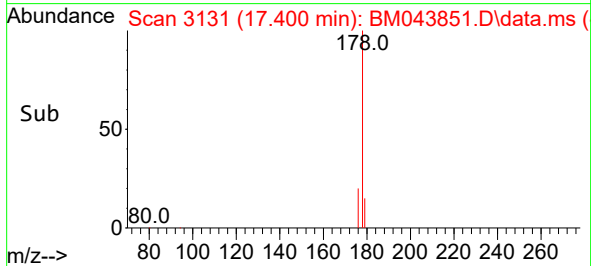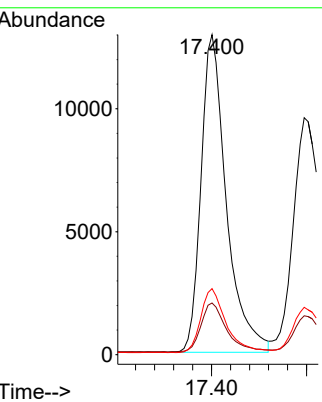

#16
 Anthracene
 Concen: 197.862 ng/u1
 RT: 17.498 min Scan# 3154
 Delta R.T. 0.004 min
 Lab File: BM043851.D
 Acq: 15 Jan 2024 21:36


Tgt Ion	Resp	Lower	Upper
178	100		
179	16.4	12.7	19.1
176	20.0	15.6	23.4

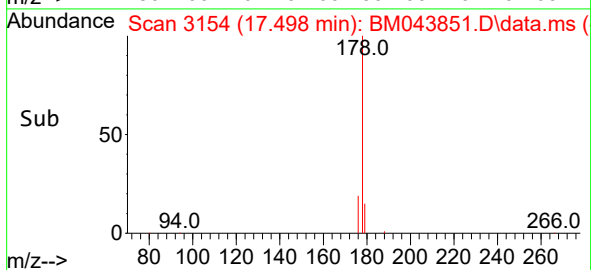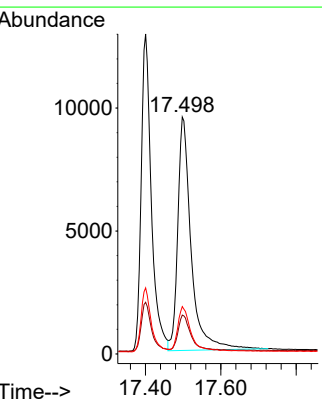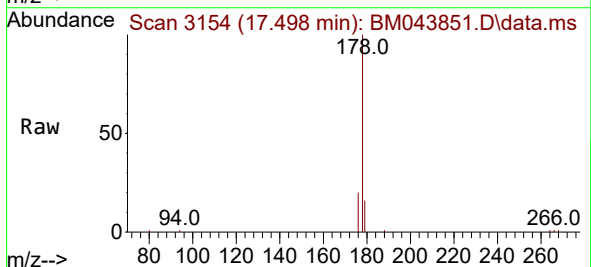



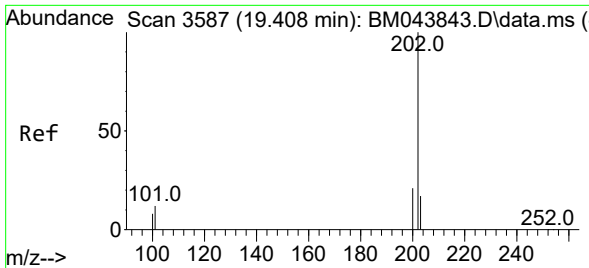


#19
 Fluoranthene
 Concen: 17.631 ng/u1
 RT: 19.413 min Scan# 31
 Delta R.T. 0.000 min
 Lab File: BM043851.D
 Acq: 15 Jan 2024 21:36


Instrument :
 BNA_M
 ClientSampleId :
 SLCS427

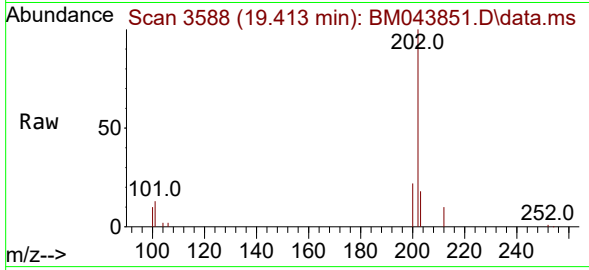



Tgt Ion:202 Resp: 27322
 Ion Ratio Lower Upper
 202 100
 101 12.7 9.6 14.4
 100 9.8 7.1 10.7

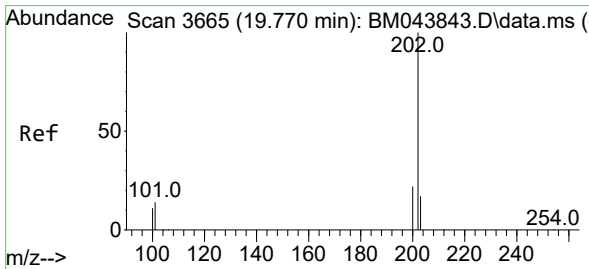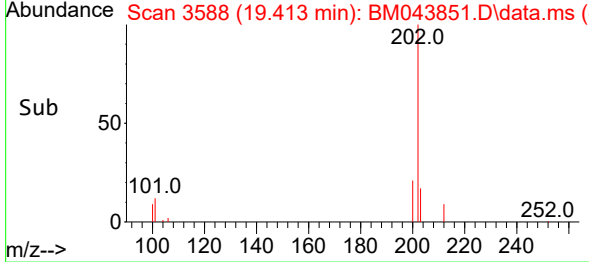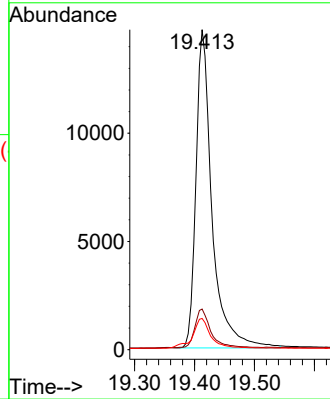


#20
 Pyrene
 Concen: 17.510 ng/u1
 RT: 19.775 min Scan# 3666
 Delta R.T. 0.000 min
 Lab File: BM043851.D
 Acq: 15 Jan 2024 21:36

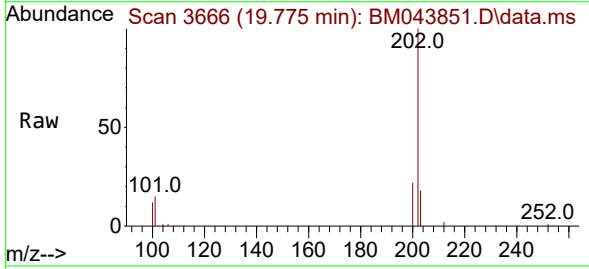


Tgt Ion:202 Resp: 28265
 Ion Ratio Lower Upper
 202 100
 101 15.1 11.3 16.9
 100 12.0 9.0 13.6

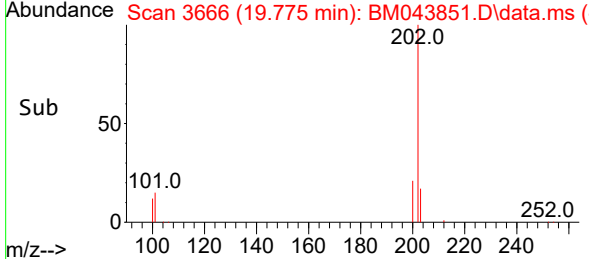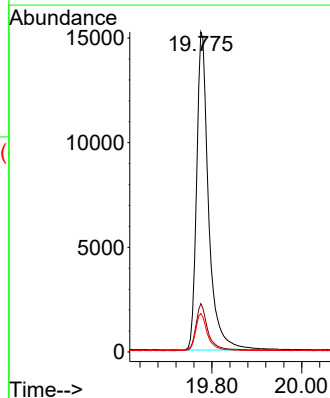






#21
 Benzo(a)anthracene
 Concen: 15.210 ng/uI
 RT: 21.533 min Scan# 4175
 Delta R.T. 0.003 min
 Lab File: BM043851.D
 Acq: 15 Jan 2024 21:36

Instrument :
 BNA_M
 ClientSampleId :
 SLCS427



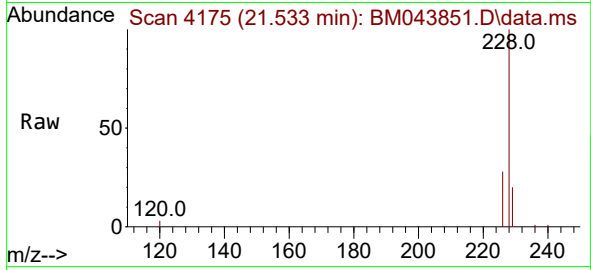



Tgt Ion:228 Resp: 20659
 Ion Ratio Lower Upper
 228 100
 229 19.7 15.7 23.5
 226 28.2 22.5 33.7

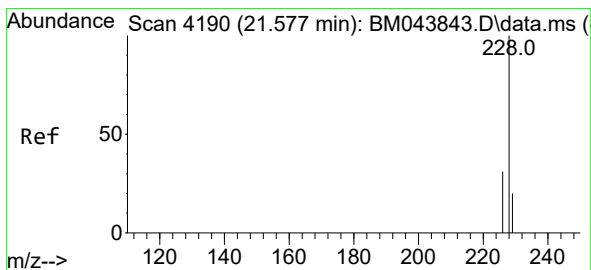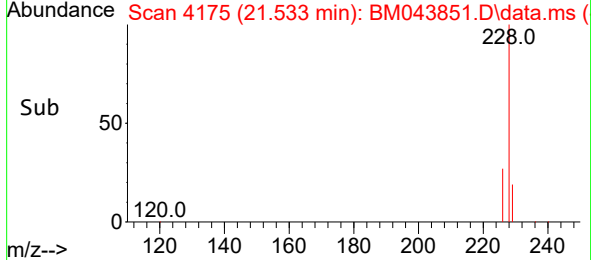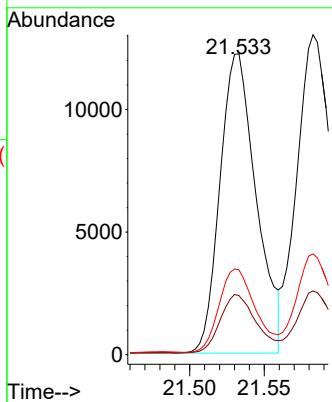

#22
 Chrysene
 Concen: 17.156 ng/uI
 RT: 21.583 min Scan# 4192
 Delta R.T. 0.003 min
 Lab File: BM043851.D
 Acq: 15 Jan 2024 21:36


Tgt Ion:228 Resp: 25097
 Ion Ratio Lower Upper
 228 100
 226 31.5 24.9 37.3
 229 19.9 15.7 23.5

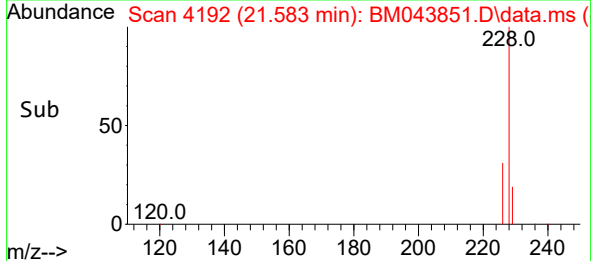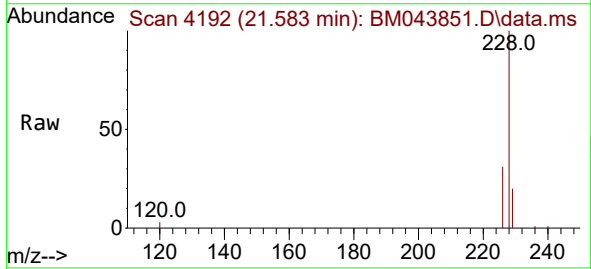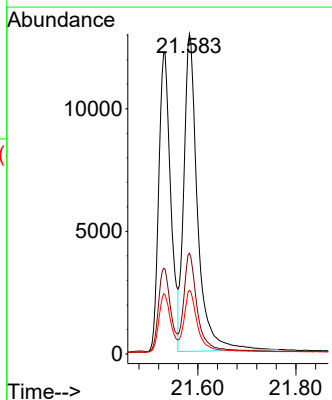






#24
 Benzo(b)fluoranthene
 Concen: 36.334 ng/uI
 RT: 23.231 min Scan# 4756
 Delta R.T. 0.000 min
 Lab File: BM043851.D
 Acq: 15 Jan 2024 21:36


Instrument :
 BNA_M
 ClientSampleId :
 SLCS427





Tgt Ion:252 Resp: 18067
 Ion Ratio Lower Upper
 252 100
 253 27.2 0.0 49.8
 125 20.6 0.0 40.4

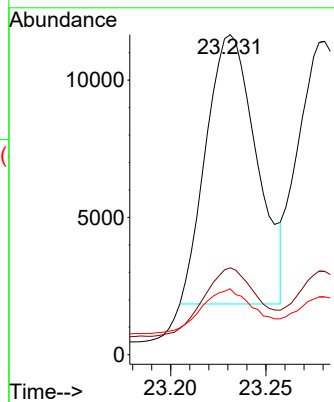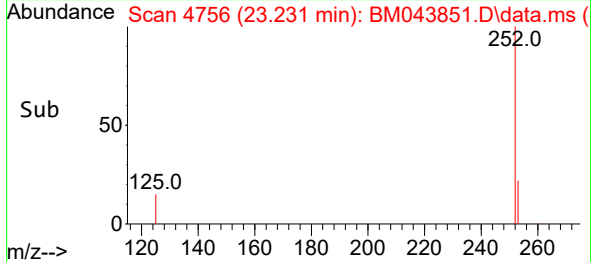


#25
 Benzo(k)fluoranthene
 Concen: 45.150 ng/uI
 RT: 23.281 min Scan# 4773
 Delta R.T. 0.003 min
 Lab File: BM043851.D
 Acq: 15 Jan 2024 21:36

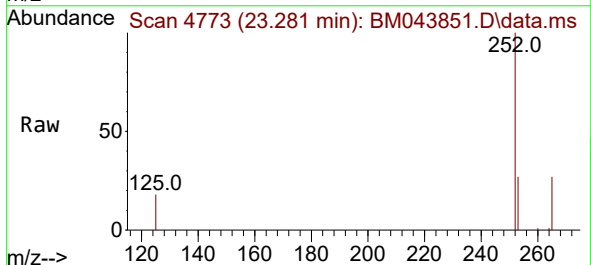


Tgt Ion:252 Resp: 24763
 Ion Ratio Lower Upper
 252 100
 253 26.6 19.9 29.9
 125 18.4 12.1 18.1#

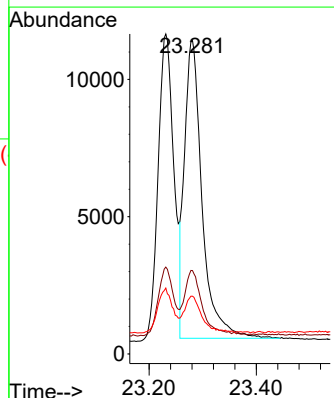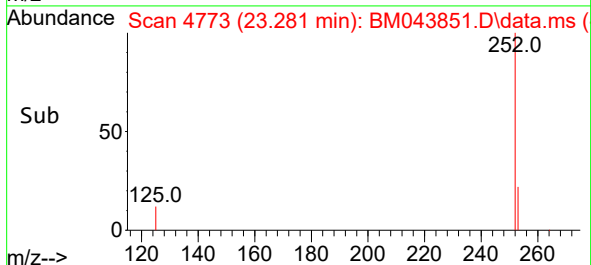



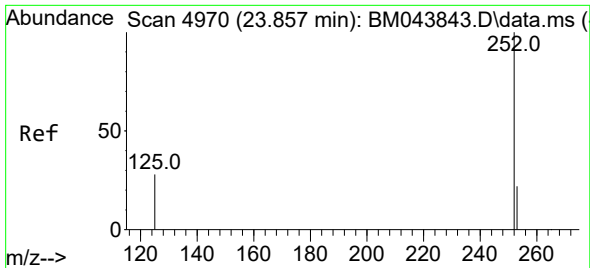


#26
 Benzo(a)pyrene
 Concen: 46.755 ng/u1
 RT: 23.874 min Scan# 4970
 Delta R.T. 0.009 min
 Lab File: BM043851.D
 Acq: 15 Jan 2024 21:36


Instrument :
 BNA_M
 ClientSampleId :
 SLCS427

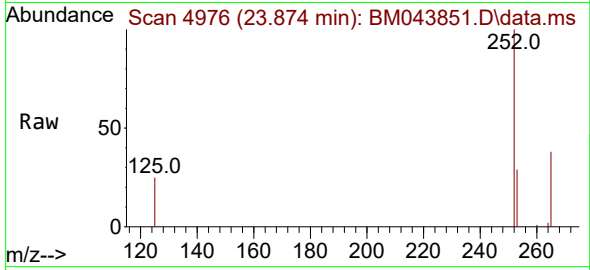



Tgt Ion:252 Resp: 21786
 Ion Ratio Lower Upper
 252 100
 253 29.0 20.8 31.2
 125 25.0 20.2 30.2

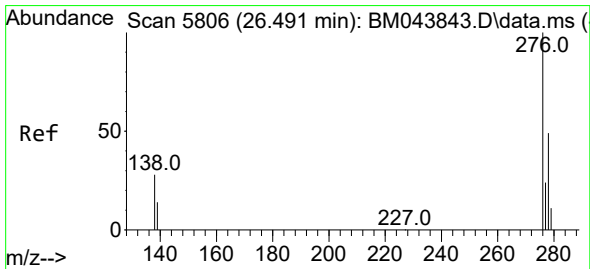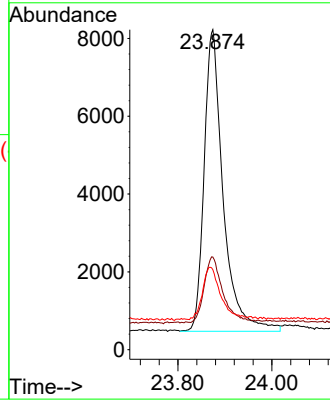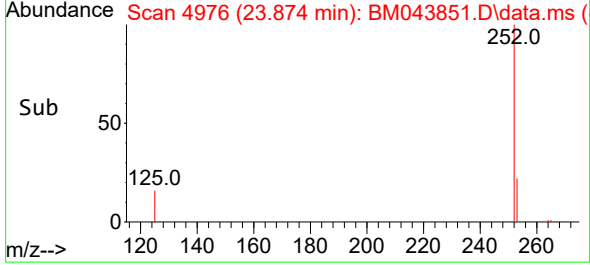


#27
 Indeno(1,2,3-cd)pyrene
 Concen: 45.678 ng/u1
 RT: 26.502 min Scan# 5809
 Delta R.T. 0.000 min
 Lab File: BM043851.D
 Acq: 15 Jan 2024 21:36

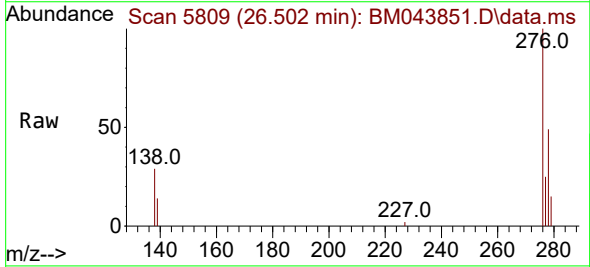


Tgt Ion:276 Resp: 26920
 Ion Ratio Lower Upper
 276 100
 138 29.7 23.5 35.3
 227 0.0 0.2 0.2#

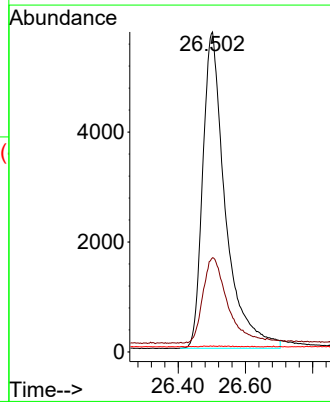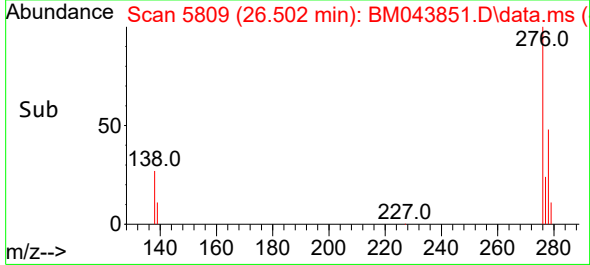



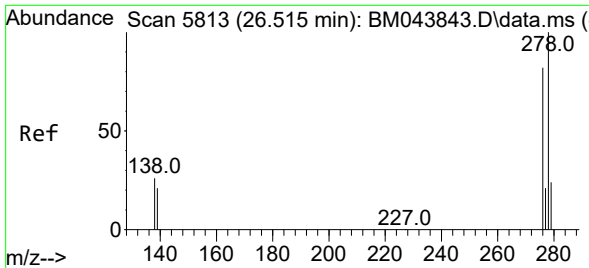


#28
 Dibenzo(a,h)anthracene
 Concen: 45.082 ng/ul
 RT: 26.522 min Scan# 5815
 Delta R.T. -0.003 min
 Lab File: BM043851.D
 Acq: 15 Jan 2024 21:36

Instrument :
 BNA_M
 ClientSampleId :
 SLCS427

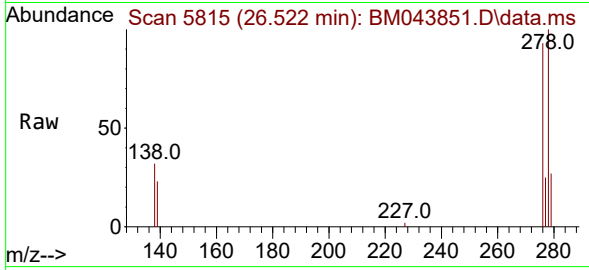

Tgt Ion:278 Resp: 20583
 Ion Ratio Lower Upper
 278 100
 139 23.3 18.1 27.1
 279 27.4 20.6 30.8

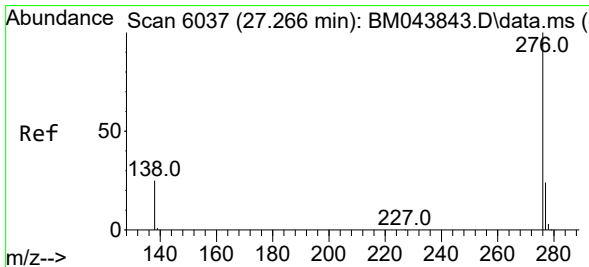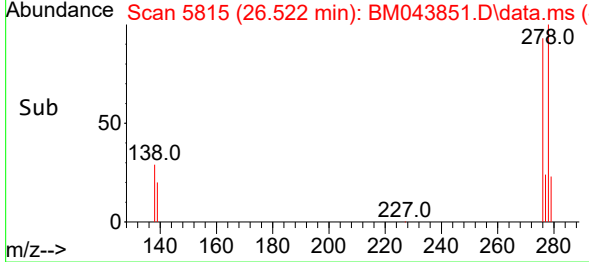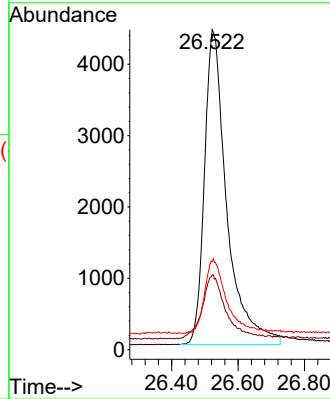

#29
 Benzo(g,h,i)perylene
 Concen: 45.781 ng/ul
 RT: 27.273 min Scan# 6039
 Delta R.T. -0.006 min
 Lab File: BM043851.D
 Acq: 15 Jan 2024 21:36

Tgt Ion:276 Resp: 22563
 Ion Ratio Lower Upper
 276 100
 138 28.4 21.0 31.4
 277 25.6 19.8 29.6

