
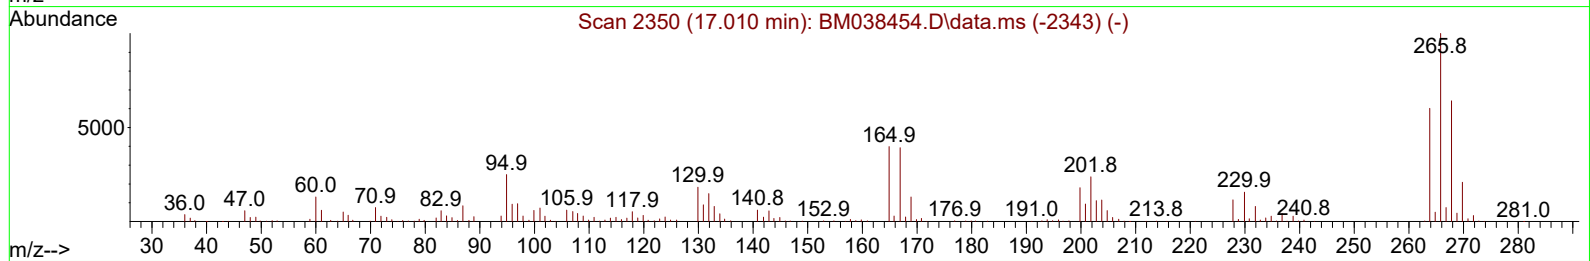
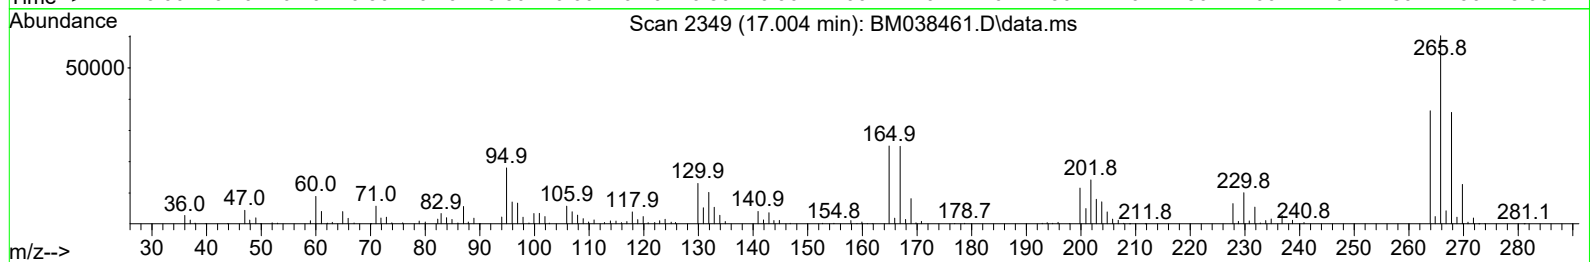


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011723\
Data File : BM038461.D
Acq On : 17 Jan 2023 09:50
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 18 07:04:26 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM011623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 17 03:06:05 2023
Response via : Initial Calibration

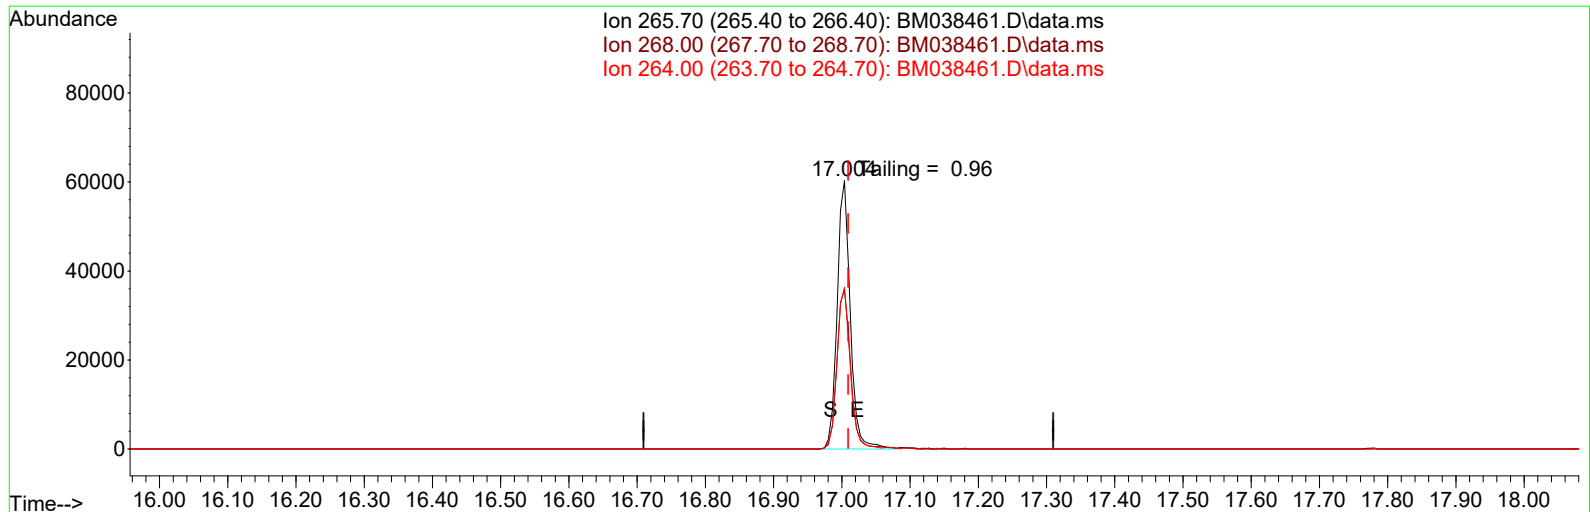

TIC: BM038461.D\data.ms

(70) Pentachlorophenol (C)




17.004min (-0.006) 0.00 ng

response 80790

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.20	59.38
264.00	60.20	60.20
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011723\
Data File : BM038461.D
Acq On : 17 Jan 2023 09:50
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 18 07:04:26 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM011623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 17 03:06:05 2023
Response via : Initial Calibration

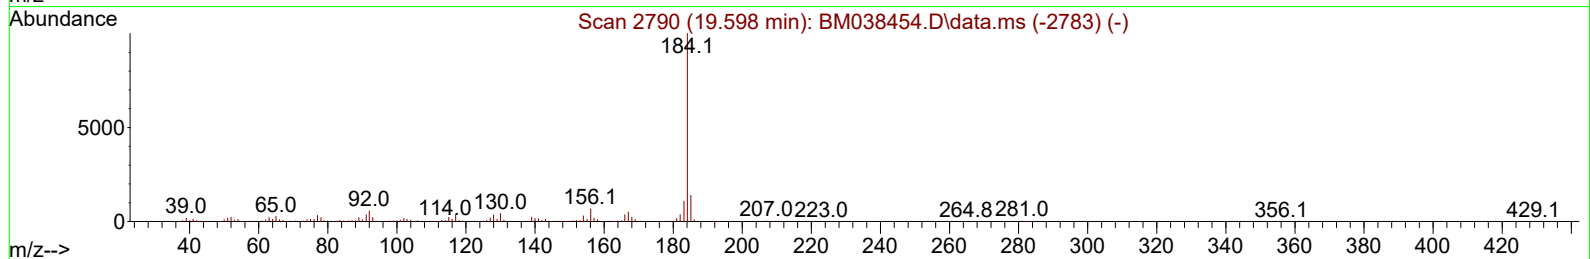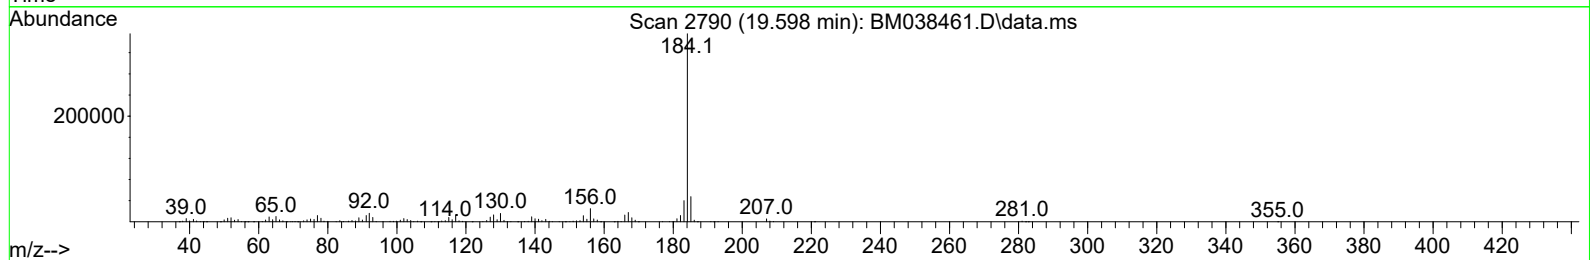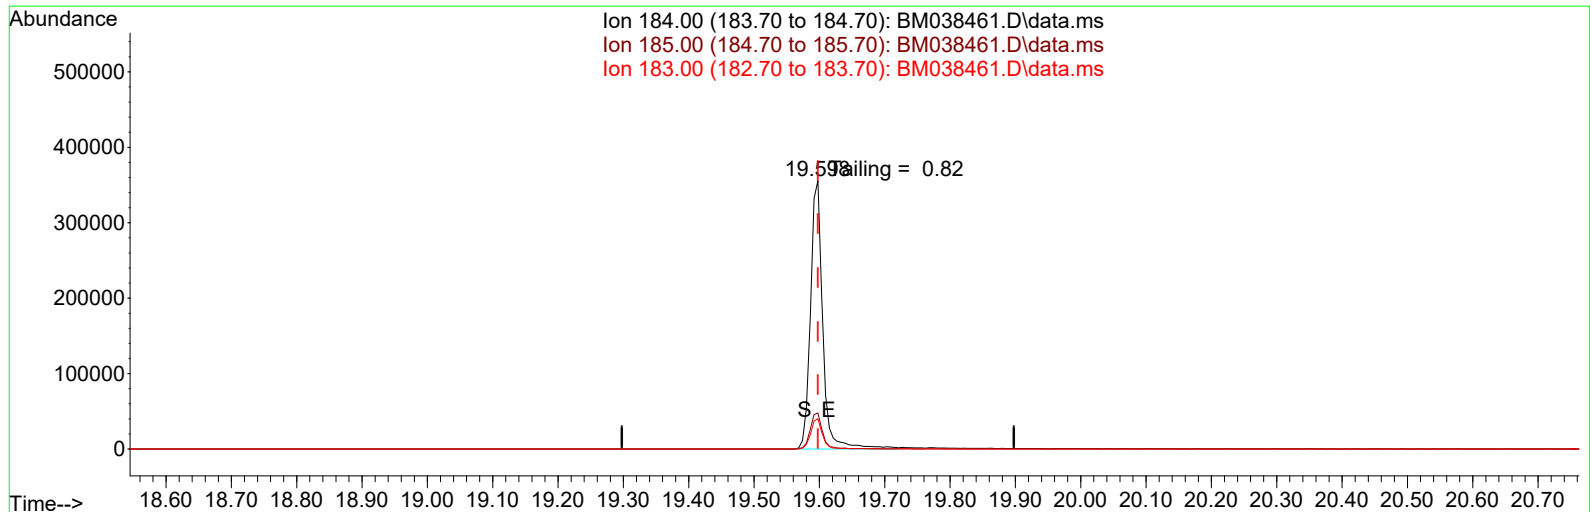

TIC: BM038461.D\data.ms

(77) Benzidine

19.598min (0.000) 0.00 ng

response 469273

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.41
183.00	10.80	11.29
0.00	0.00	0.00