


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011723\
Data File : BM038461.D
Acq On : 17 Jan 2023 09:50
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM011623.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jan 19 06:09:42 2023

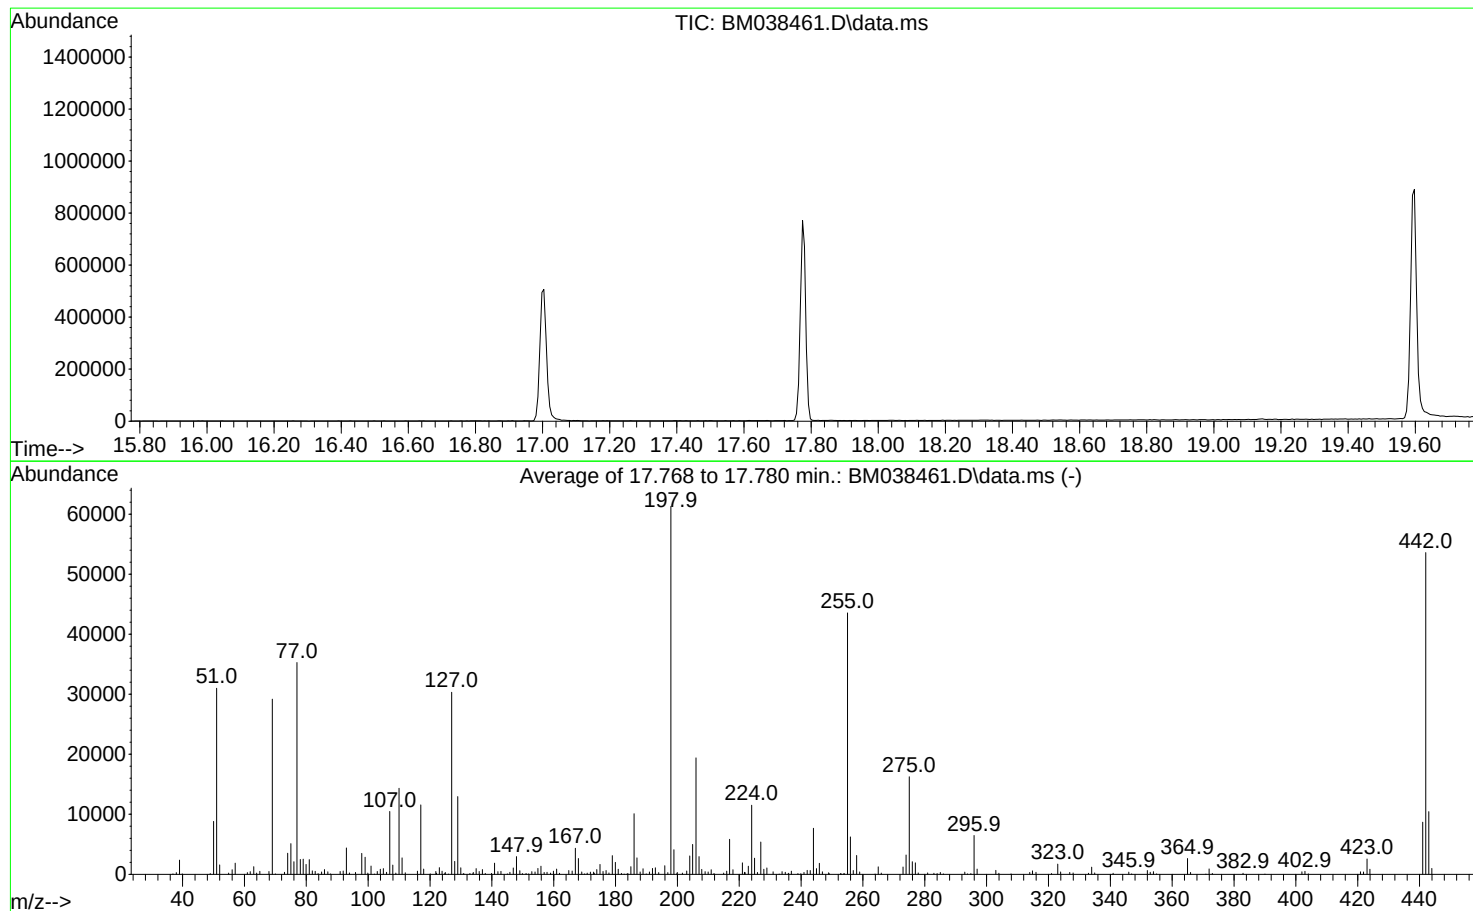




AutoFind: Scans 2479, 2480, 2481; Background Corrected with Scan 2473

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.6	31000	PASS
68	69	0.00	2	1.6	457	PASS
69	198	0.00	100	47.6	29197	PASS
70	69	0.00	2	0.2	64	PASS
127	198	10	80	49.5	30331	PASS
197	198	0.00	2	0.5	291	PASS
198	198	100	100	100.0	61301	PASS
199	198	5	9	6.7	4087	PASS
275	198	10	60	26.5	16263	PASS
365	198	1	100	4.3	2615	PASS
441	198	0.01	100	14.2	8675	PASS
442	442	50	100	100.0	53613	PASS
443	442	15	24	19.5	10431	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011723\
Data File : BM038461.D
Acq On : 17 Jan 2023 09:50
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jan 18 07:04:26 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM011623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 17 03:06:05 2023
Response via : Initial Calibration

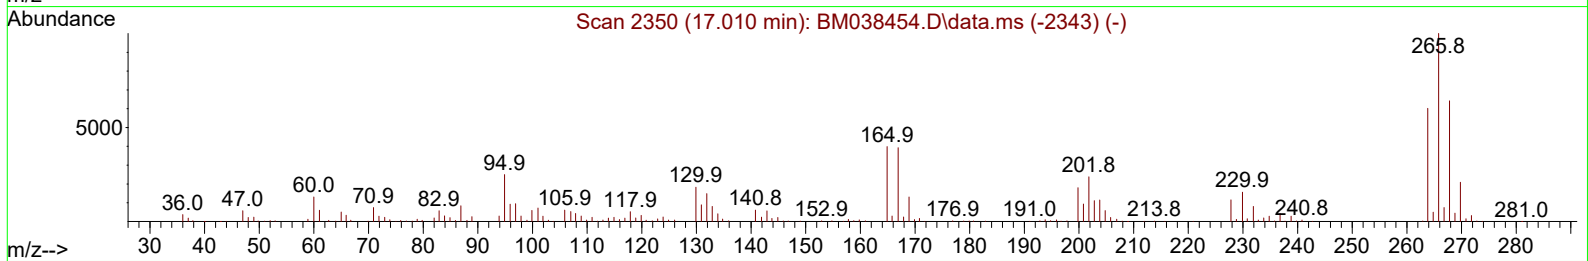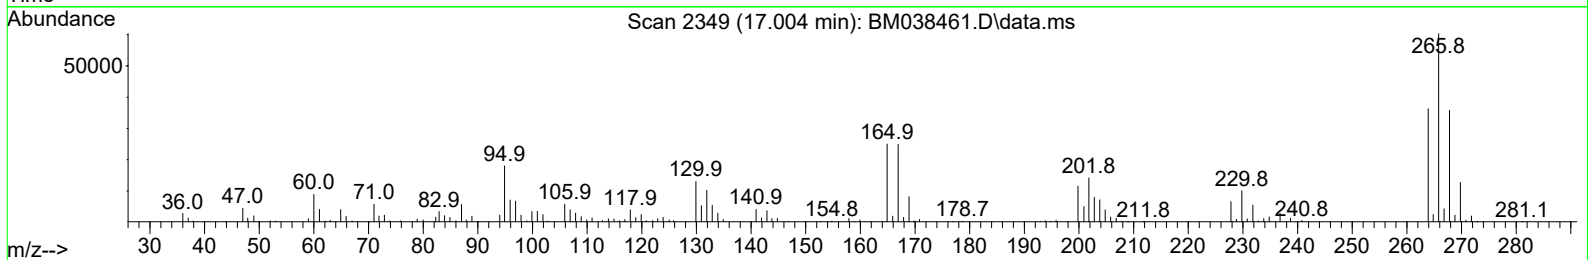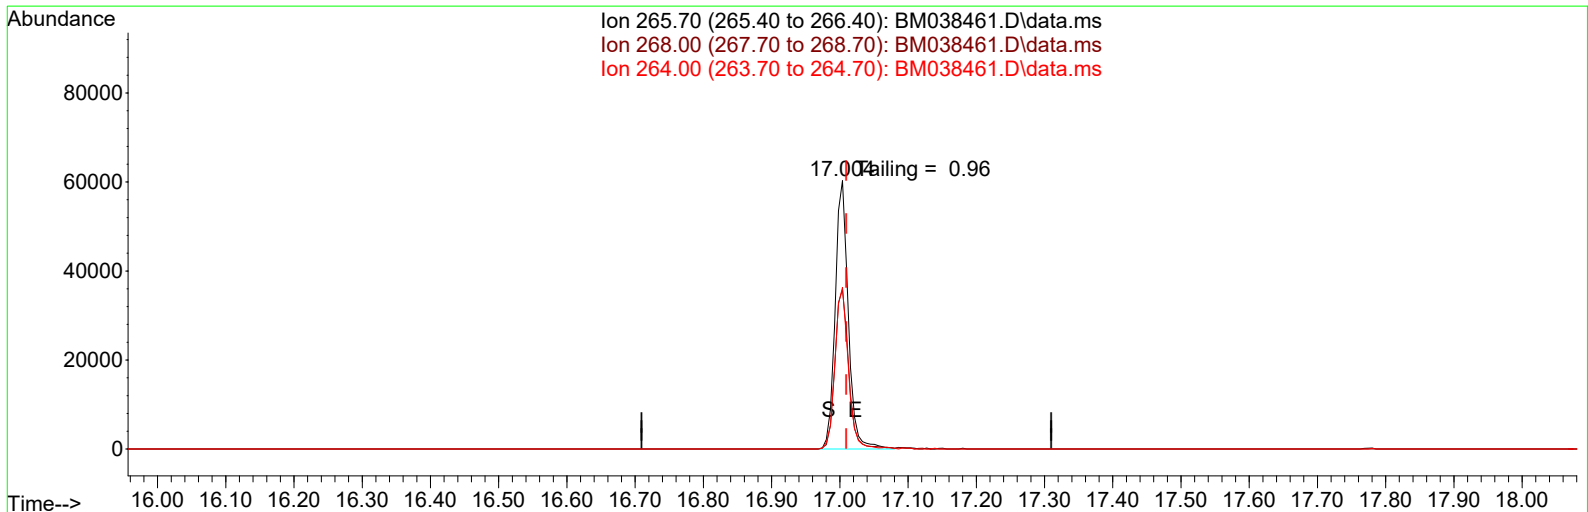

TIC: BM038461.D\data.ms

(70) Pentachlorophenol (C)

17.004min (-0.006) 0.00 ng




response 80790

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.20	59.38
264.00	60.20	60.20
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011723\
Data File : BM038461.D
Acq On : 17 Jan 2023 09:50
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jan 18 07:04:26 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM011623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 17 03:06:05 2023
Response via : Initial Calibration

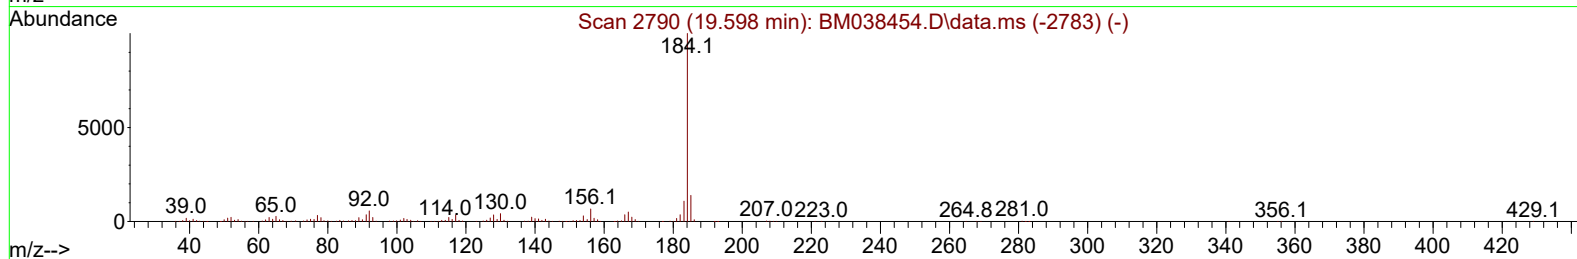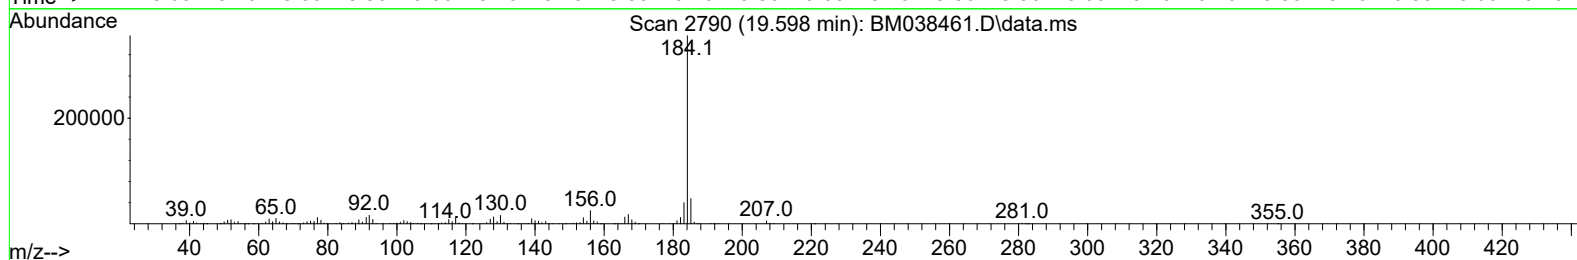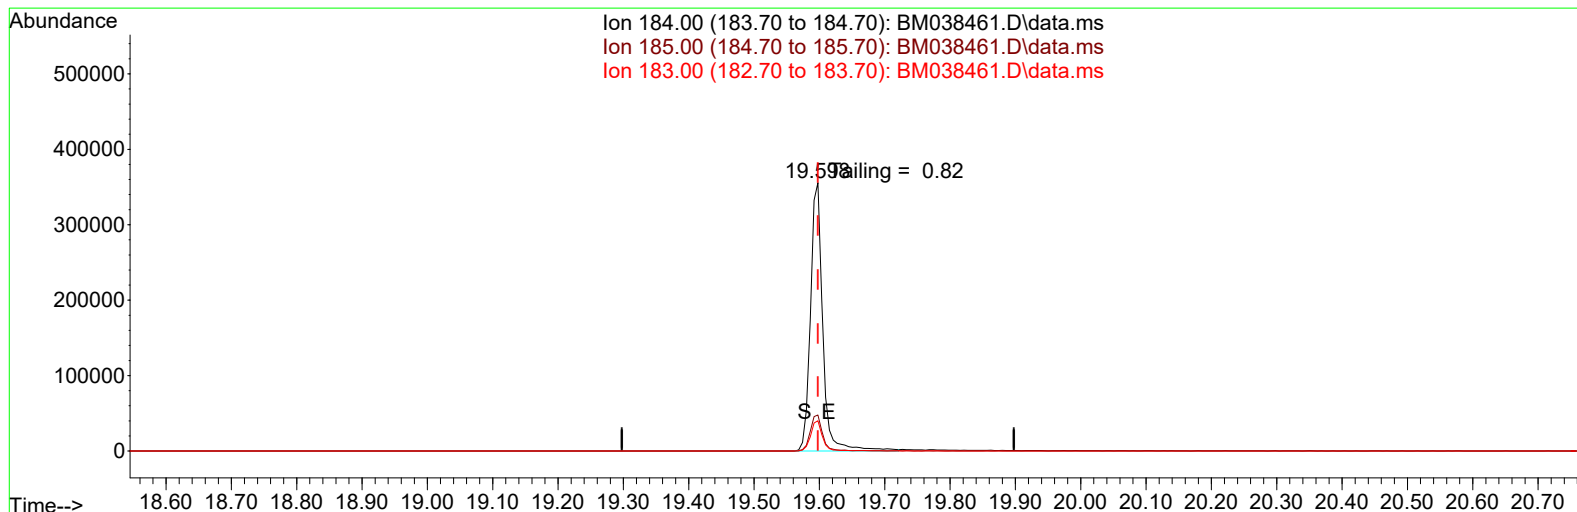

TIC: BM038461.D\data.ms

(77) Benzidine

19.598min (0.000) 0.00 ng

response 469273

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.41
183.00	10.80	11.29
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/17/2023	BNA_M	<u>BM038461.D</u>
Compound Name	Response	Retention Time
DDT	268251	20.815
DDD	2323	20.427
DDE	0	19.9
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2323	270574	0.86

Instrument :
BNA_M
ClientSampleId :
DFTPP