


Data Path : Z:\HPCHEM1\BNA M\DATA\BM011818\
Data File : BM013654.D
Acq On : 18 Jan 2018 23:00
Operator : SJ/JU
Sample : J1097-08
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
DAJM8

Manual Integrations
APPROVED

Sohil
1/19/2018 9:50:08 AM

Quant Time: Jan 19 04:11:10 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM011018.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 19 02:57:39 2018
Response via : Initial Calibration

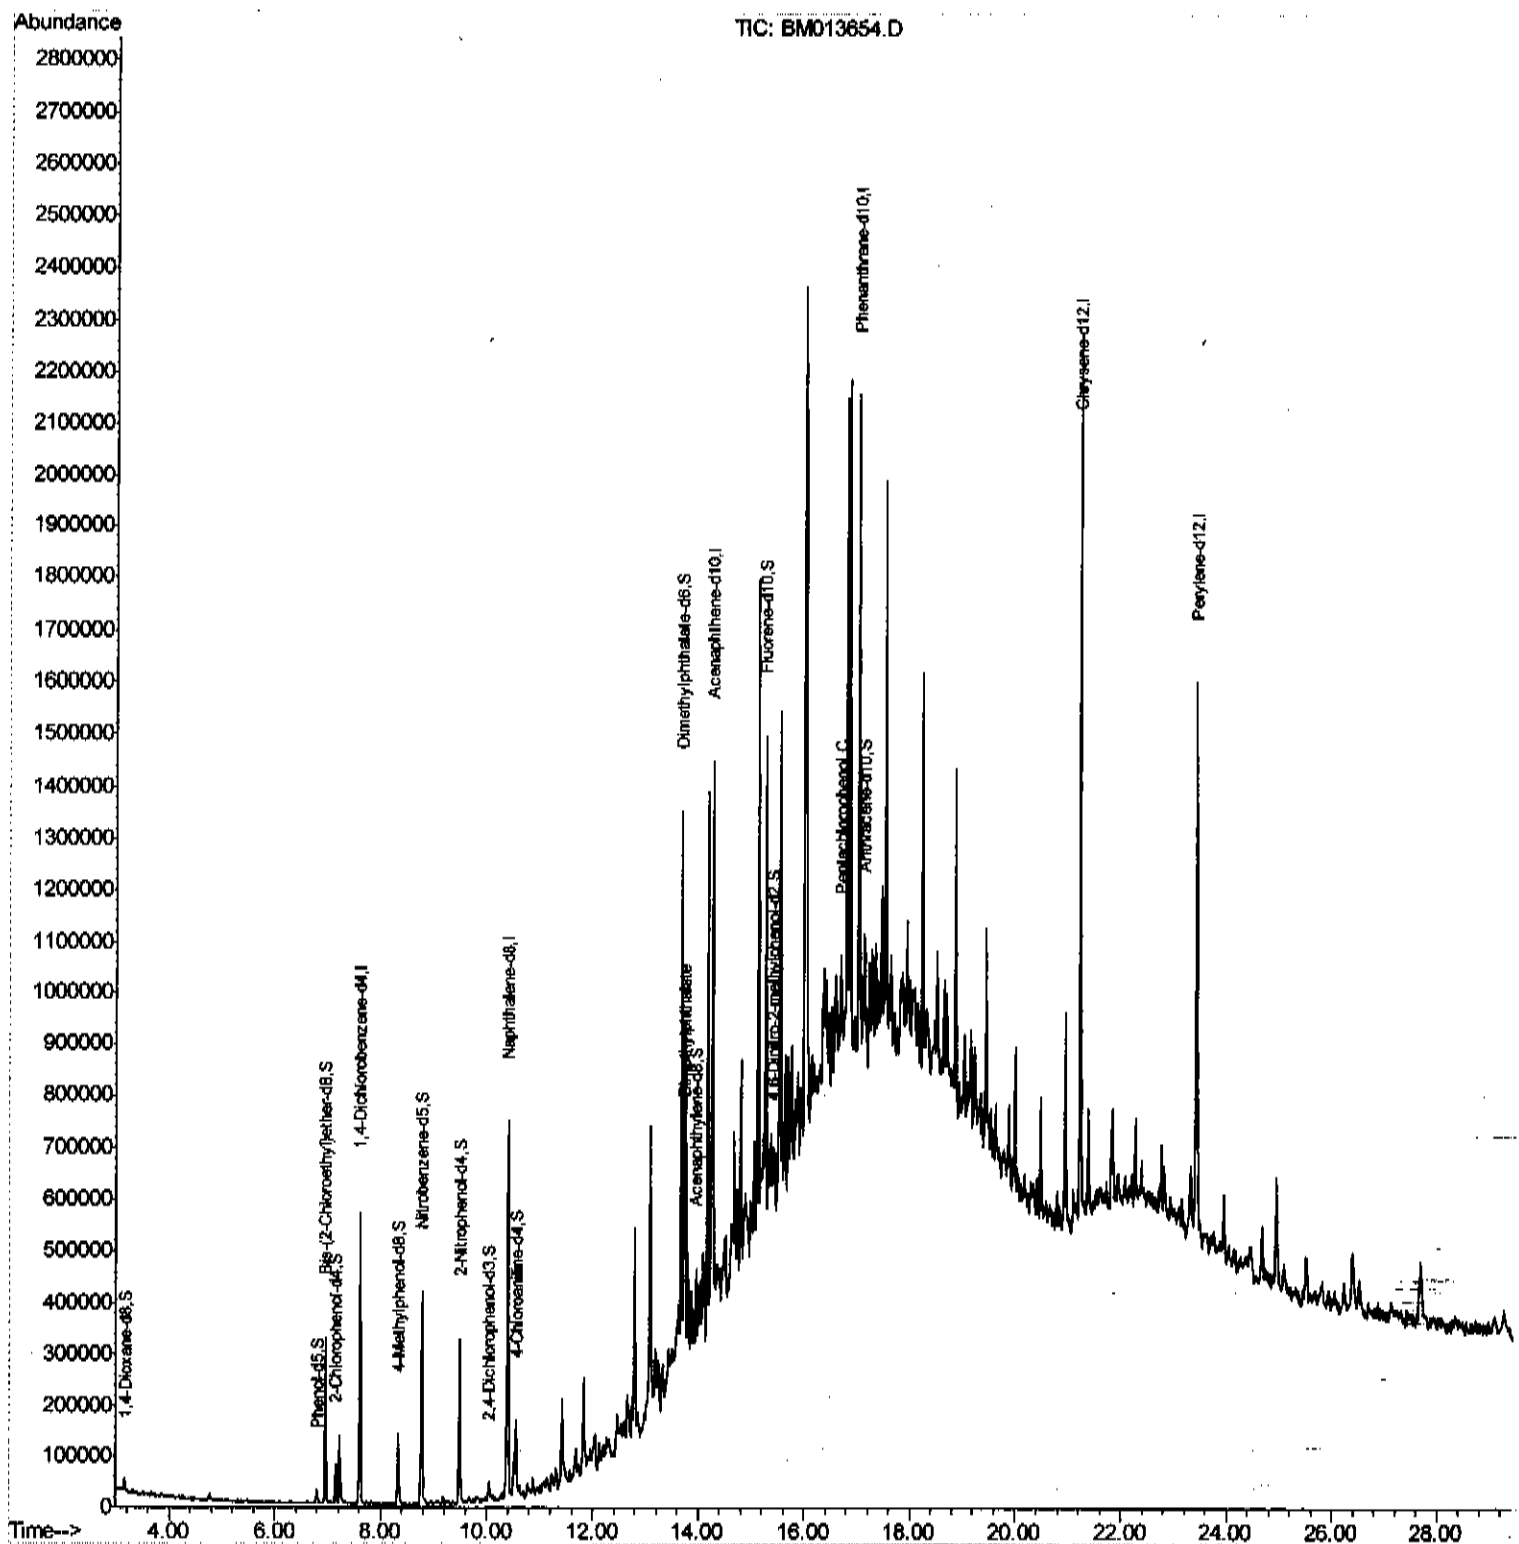




Data Path : Z:\HPCHEM1\BNA M\DATA\BM011818\
 Data File : BM013654.D
 Acq On : 18 Jan 2018 23:00
 Operator : SJ/JU
 Sample : J1097-08
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampled :
 DAJM8

Manual Integrations
 APPROVED

Sohil
 1/19/2018 9:50:08 AM

Quant Time: Jan 19 03:06:23 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM011018.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 19 02:57:39 2018
 Response via : Initial Calibration

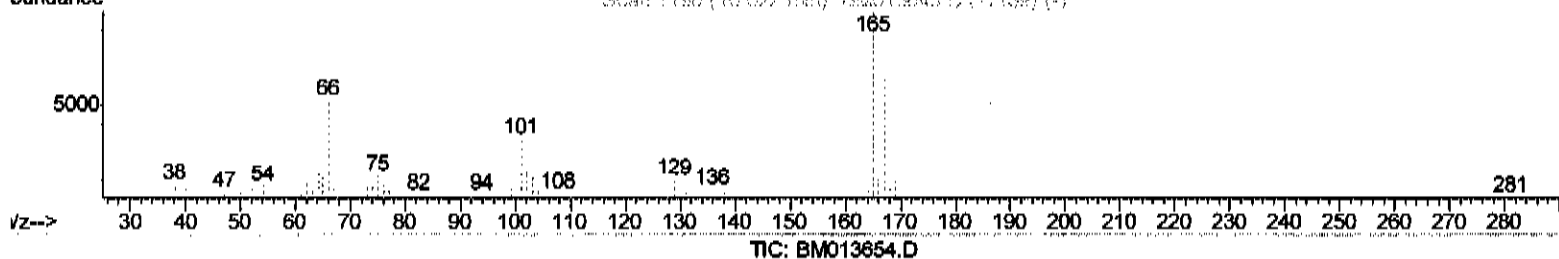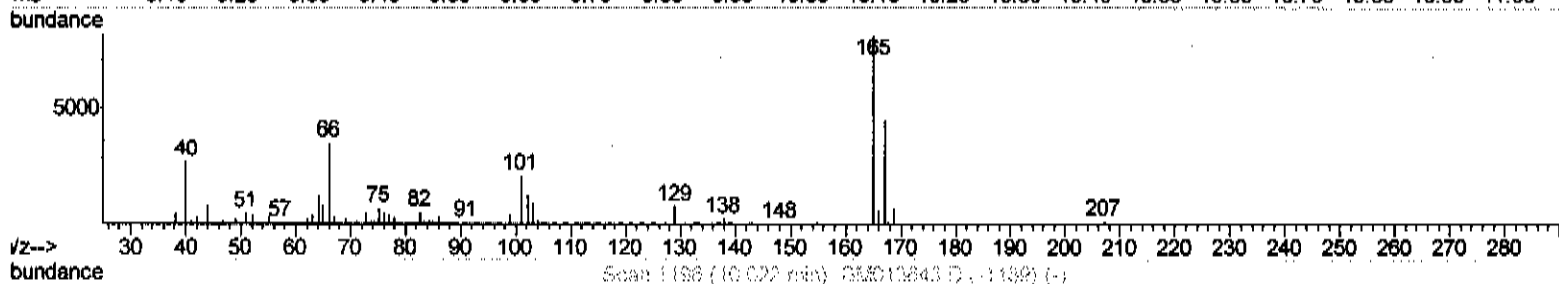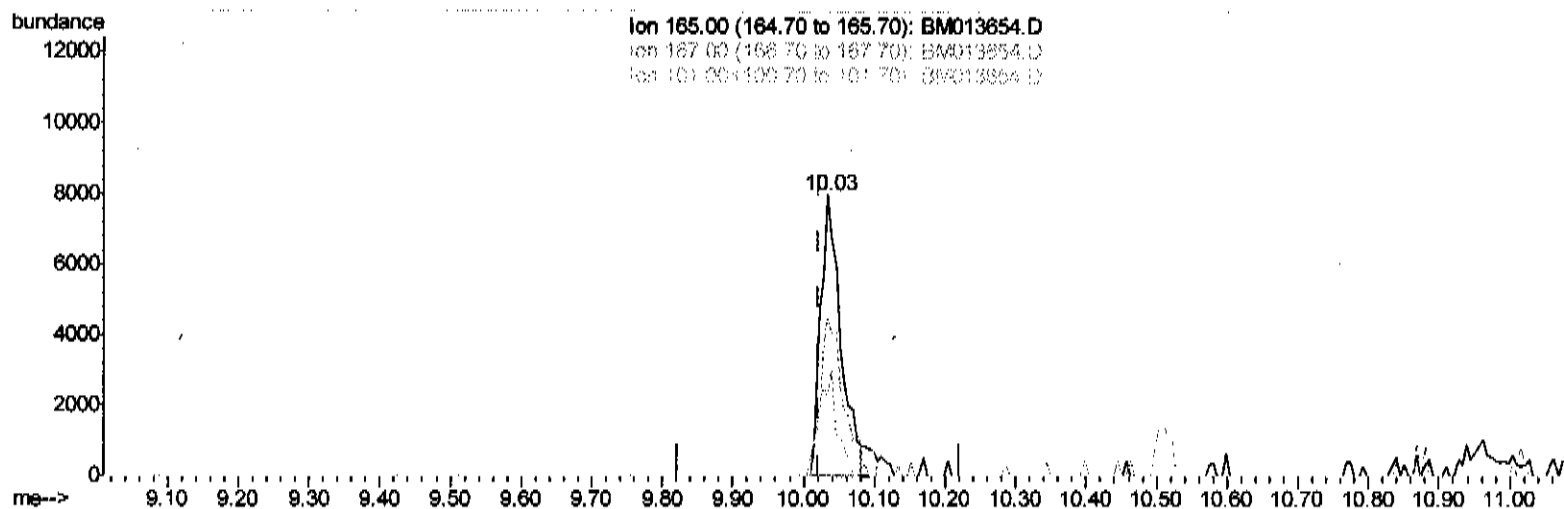

(26) 2,4-Dichlorophenol-d3 (S)

10.033min (+0.012) 1.73ng/ul

response 15662

Ion	Exp%	Act%
165.00	100	100
167.00	63.60	56.89
101.00	29.30	28.61
0.00	0.00	0.00


Data Path : Z:\HPCHEM1\BNA M\DATA\BM011818\
 Data File : BM013654.D
 Acq On : 18 Jan 2018 23:00
 Operator : SJ/JU
 Sample : J1097-08
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DAJM8

Manual Integrations
 APPROVED

Sohil
 1/19/2018 9:50:08 AM

Quant Time: Jan 19 03:06:23 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM011018.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 19 02:57:39 2018
 Response via : Initial Calibration

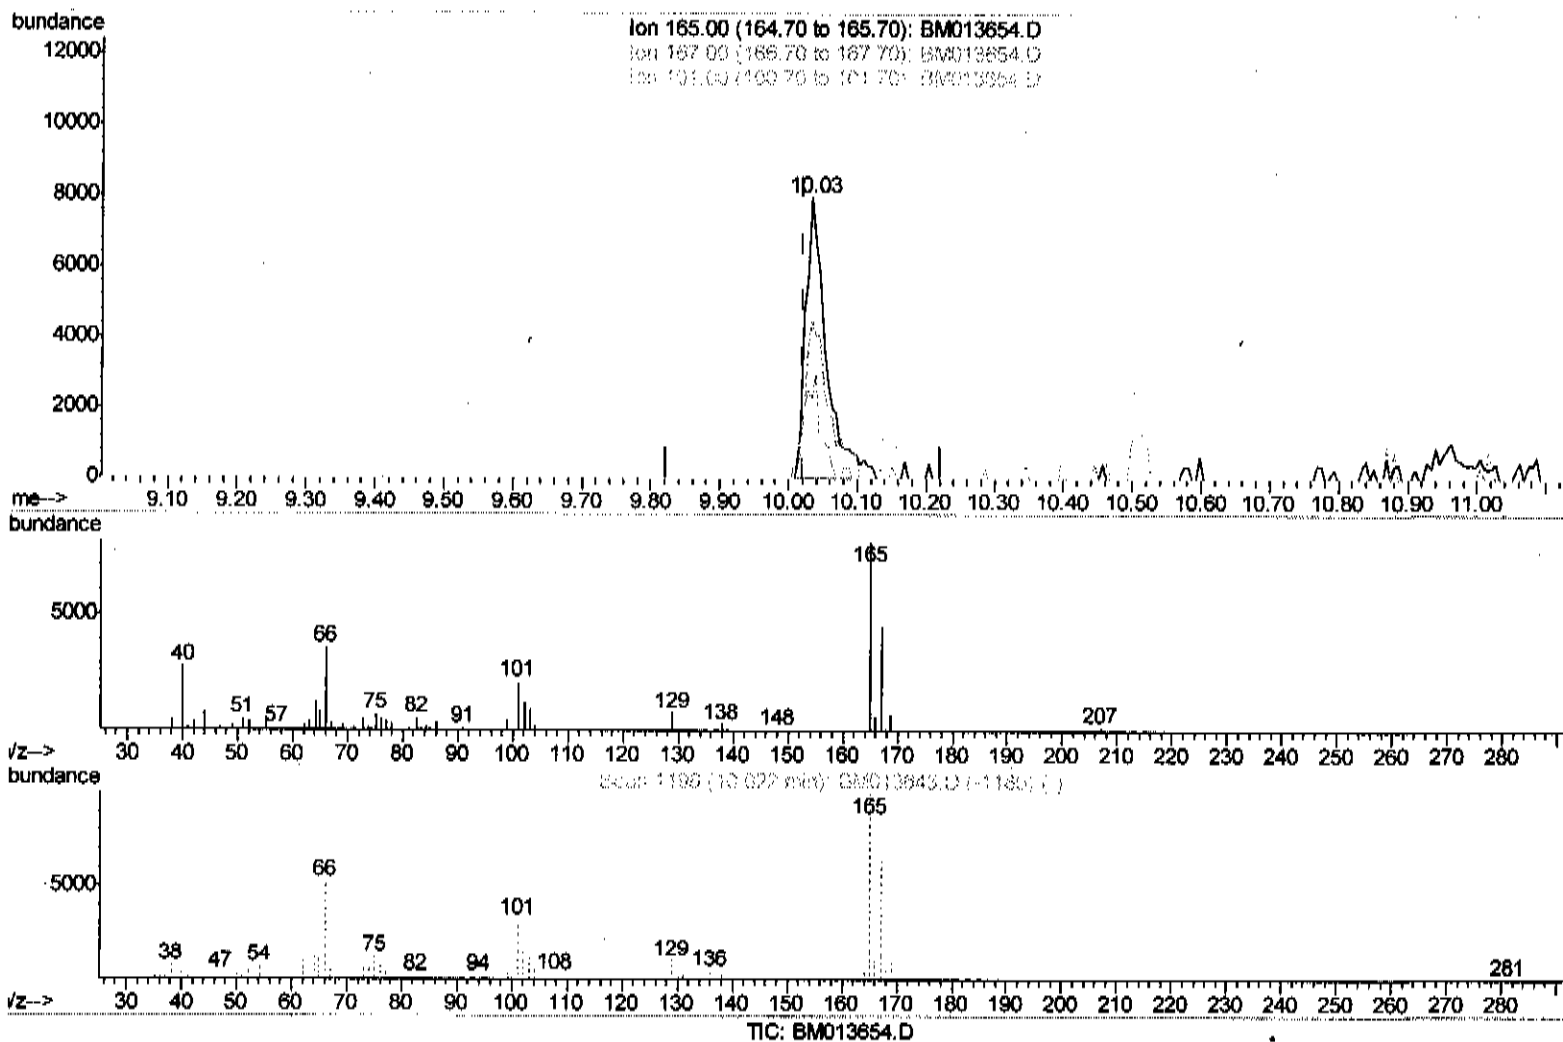

(26) 2,4-Dichlorophenol-d3 (S)

10.033min (+0.012) 1.89ng/ul m

SJ 1/19/18

response 17057

Ion	Exp%	Act%
165.00	100	100
167.00	63.60	56.89
101.00	29.30	28.61
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA M\DATA\BM011818\
 Data File : BM013654.D
 Acq On : 18 Jan 2018 23:00
 Operator : SJ/JU
 Sample : J1097-08
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampled :
 DAJM8

Manual Integrations
 APPROVED

Sohil
 1/19/2018 9:50:08 AM

Quant Time: Jan 19 04:11:10 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM011018.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 19 02:57:39 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	143613	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	570583	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.27	164	319248	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.02	188	694444	20.00	ng/ul	0.00
75) Chrysene-d12	21.22	240	769939	20.00	ng/ul	0.00
83) Perylene-d12	23.41	264	790888	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.16	96	10591	2.91	ng/uL	0.00
5) Phenol-d5	6.80	99	16221	1.47	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.96	67	131790	19.73	ng/ul	0.00
9) 2-Chlorophenol-d4	7.16	132	30563	3.40	ng/ul	0.00
13) 4-Methylphenol-d8	8.33	113	52584	6.20	ng/ul	0.00
19) Nitrobenzene-d5	8.77	128	88936	20.09	ng/ul	0.00
22) 2-Nitrophenol-d4	9.49	143	93968	20.09	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.03	165	17057m	1.89	ng/ul	0.01
29) 4-Chloroaniline-d4	10.55	131	58868	7.51	ng/ul	0.00
43) Dimethylphthalate-d6	13.68	166	546919	20.79	ng/ul	0.00
46) Acenaphthylene-d8	13.96	160	58166	1.73	ng/ul	0.00
51) 4-Nitrophenol-d4	14.50	143	1125	0.26	ng/ul	0.00
57) Fluorene-d10	15.26	176	337352	14.58	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.42	200	9417	2.25	ng/ul	0.01
70) Anthracene-d10	17.12	188	76583	2.26	ng/ul	0.00
76) Pyrene-d10	19.42	212	23994	0.67	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.28	264	14347	0.39	ng/ul	0.00

- 50/19/18

Target Compounds

				Ovalue	
44) Dimethylphthalate	13.73	163	127472	4.927	ng/ul 98
68) Pentachlorophenol	16.67	266	32653	6.960	ng/ul 99

(#) - qualifier out of range (m) = manual integration (+) = signals summed