
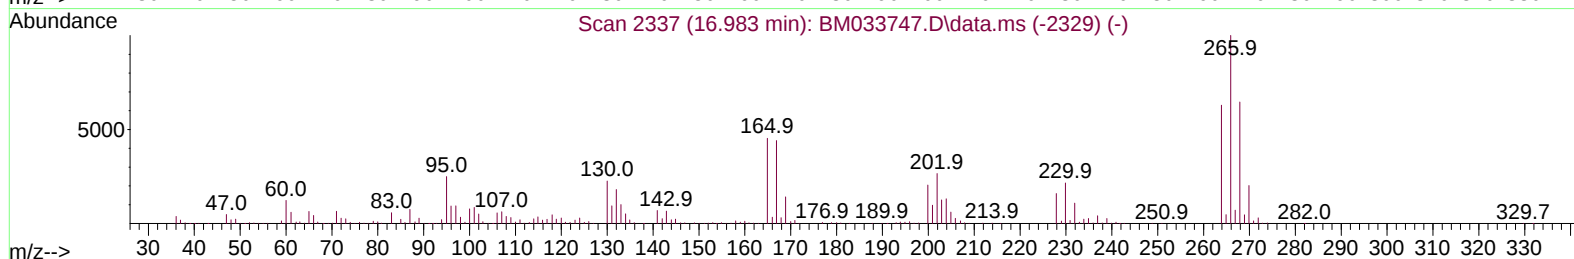
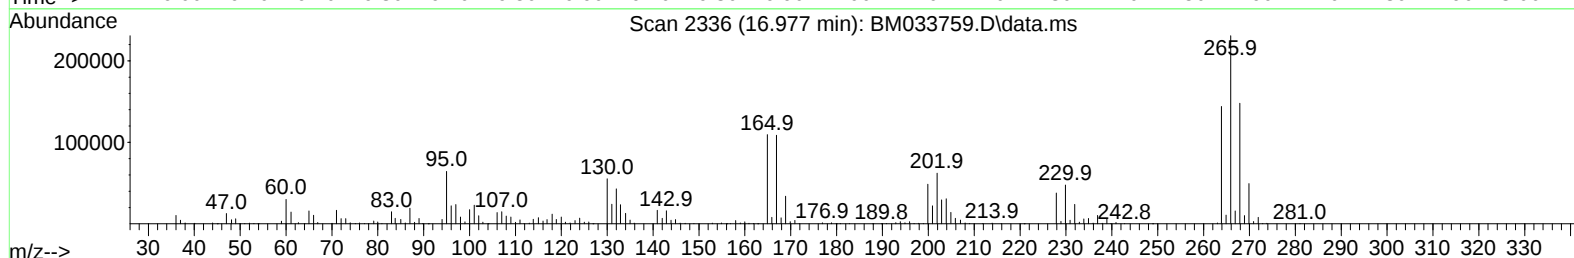


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011822\
 Data File : BM033759.D
 Acq On : 18 Jan 2022 11:56
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 19 04:50:00 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM011722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 17 16:30:56 2022
 Response via : Initial Calibration

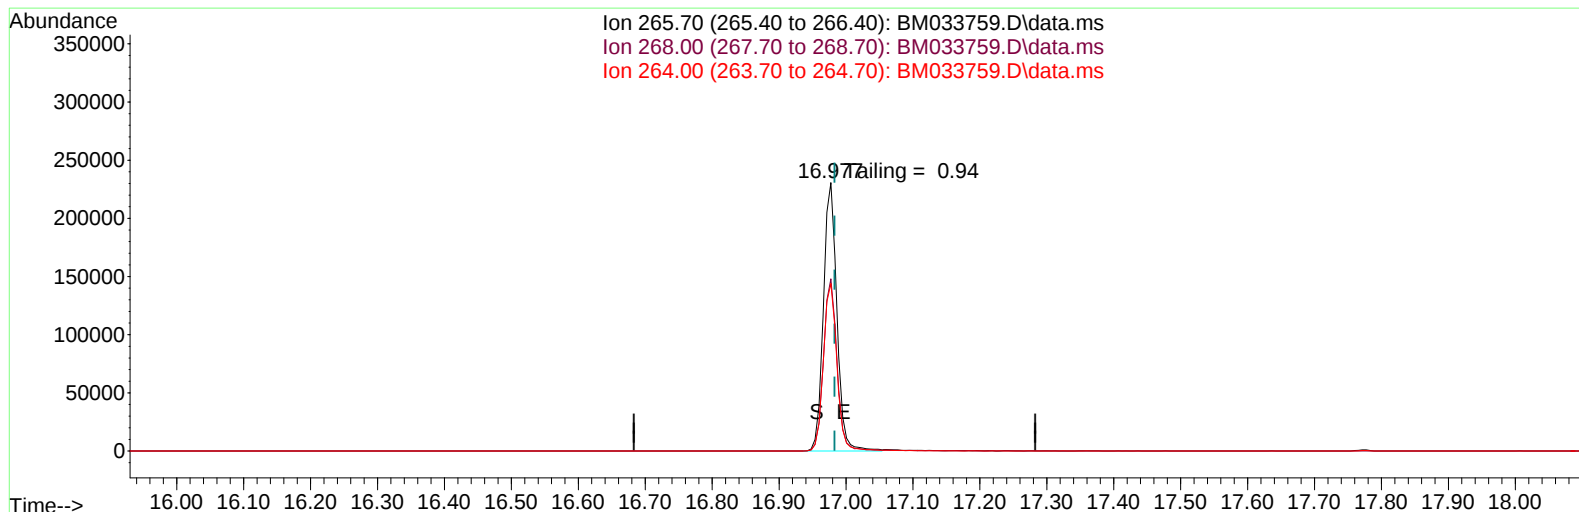

TIC: BM033759.D\data.ms

(70) Pentachlorophenol (C)




16.977min (-0.006) 0.00 ng

response 324582

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	64.13
264.00	61.40	62.44
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011822\
Data File : BM033759.D
Acq On : 18 Jan 2022 11:56
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 19 04:50:00 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM011722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 17 16:30:56 2022
Response via : Initial Calibration

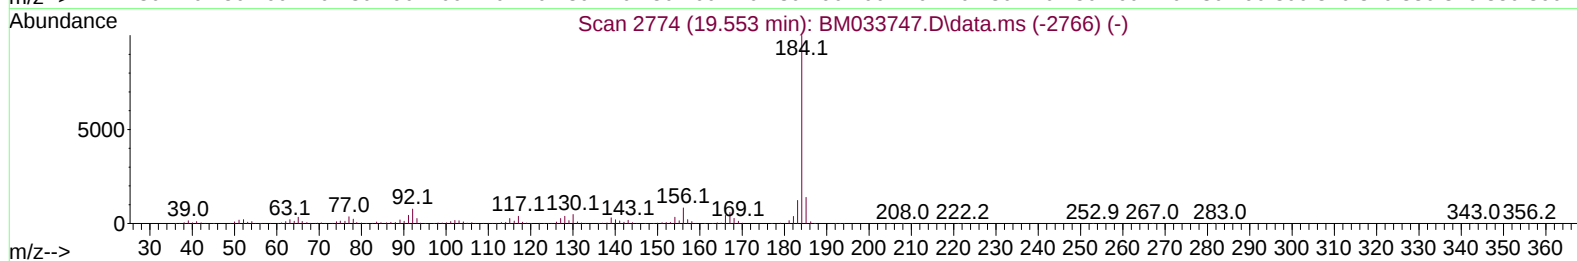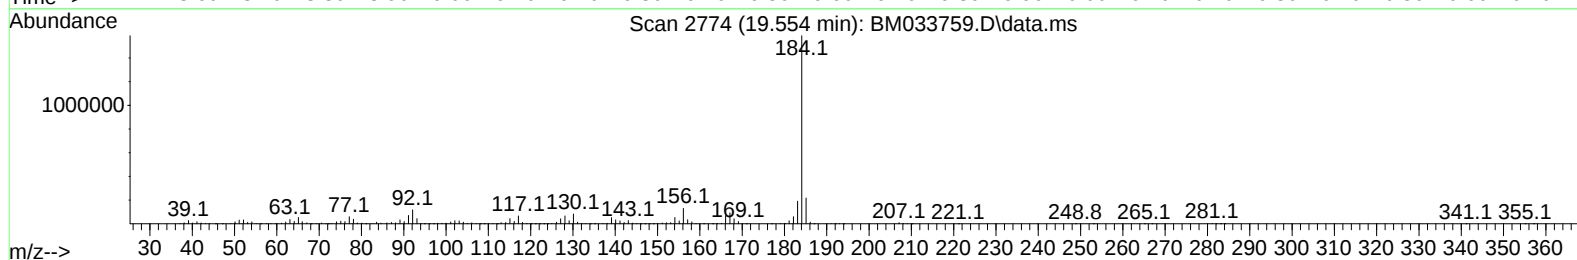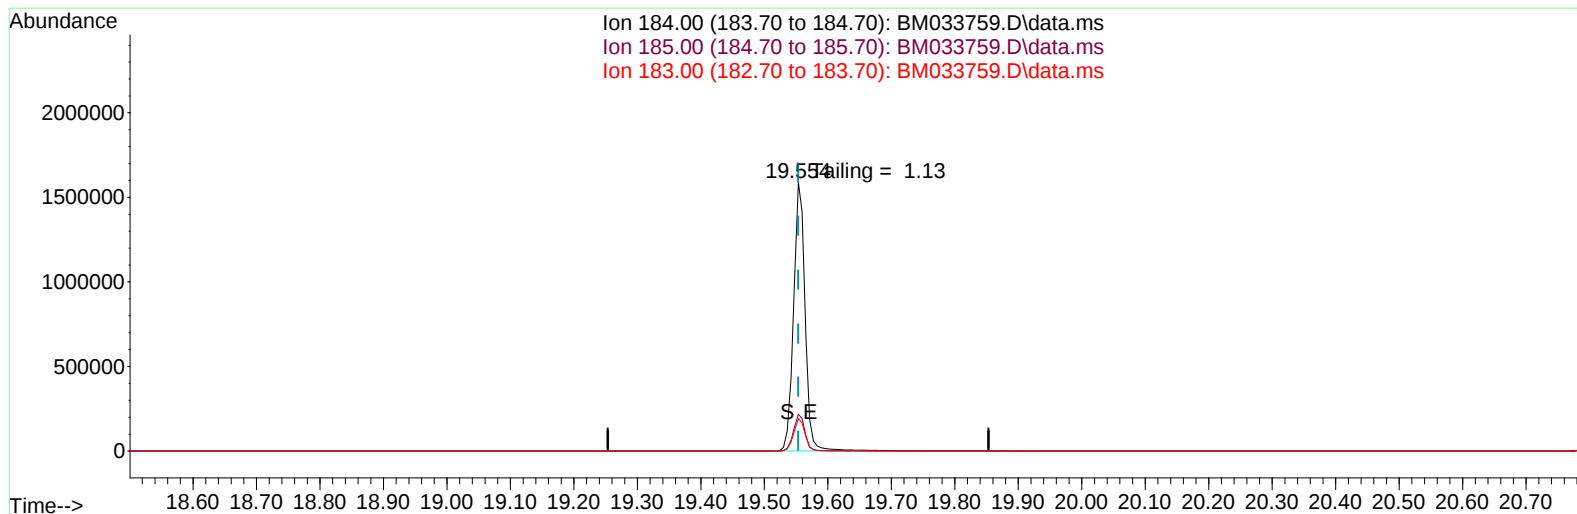

TIC: BM033759.D\data.ms

(77) Benzidine

19.554min (+ 0.000) 0.00 ng

response 2023513

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	13.71
183.00	12.10	12.04
0.00	0.00	0.00