

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011822\
 Data File : BM033761.D
 Acq On : 18 Jan 2022 13:25
 Operator : CG/JU
 Sample : PB142061BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB142061BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM011722.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM033761.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.501	378	385	397	rBV	3392188	4817829	40.17%	9.475%
2	7.113	650	659	675	rBV	3168429	5007409	41.75%	9.847%
3	7.954	795	802	810	rBV	628102	989202	8.25%	1.945%
4	9.119	991	1000	1015	rBV	1998697	3318844	27.67%	6.527%
5	10.766	1273	1280	1290	rBV	842895	1418093	11.82%	2.789%
6	13.218	1690	1697	1709	rBV	5108028	7783339	64.90%	15.306%
7	14.589	1923	1930	1942	rBV	1383044	2007889	16.74%	3.949%
8	16.071	2175	2182	2199	rBV	4315544	6052465	50.47%	11.903%
9	17.324	2388	2395	2408	rBV	1795667	2485623	20.73%	4.888%
10	19.936	2833	2839	2852	rBV	9299180	11992473	100.00%	23.584%
11	21.483	3097	3102	3111	rBV	1981130	2587195	21.57%	5.088%
12	23.894	3505	3512	3521	rVB2	1152164	2389595	19.93%	4.699%




Sum of corrected areas: 50849956

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011822\
Data File : BM033761.D
Acq On : 18 Jan 2022 13:25
Operator : CG/JU
Sample : PB142061BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB142061BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM011722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

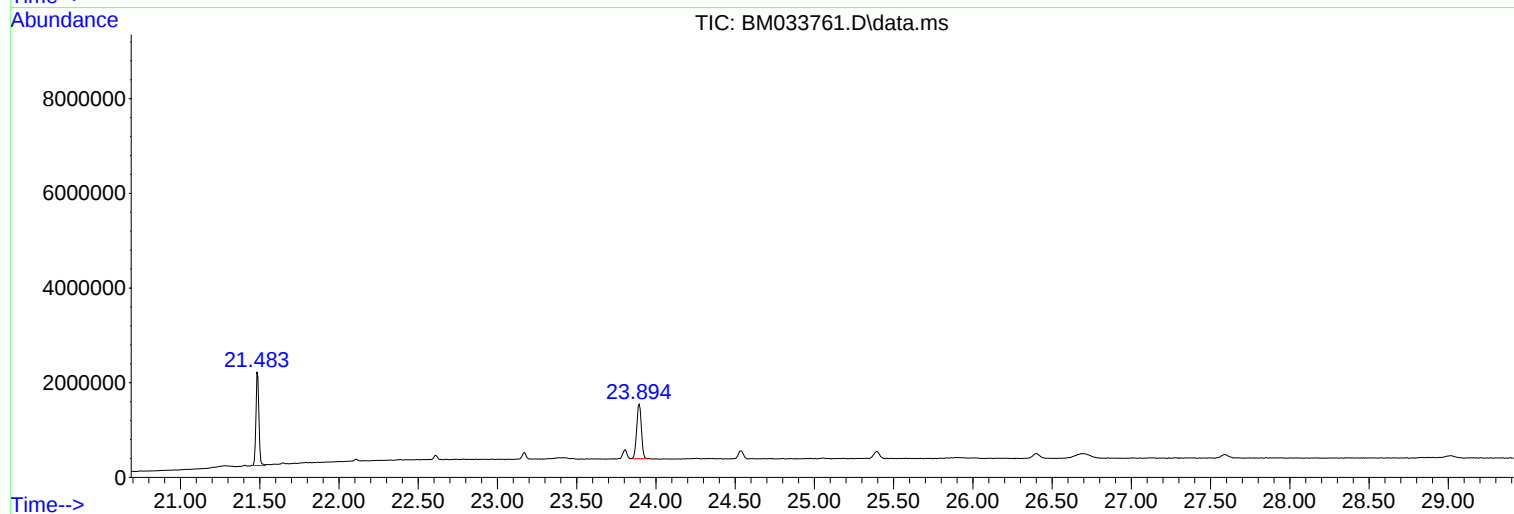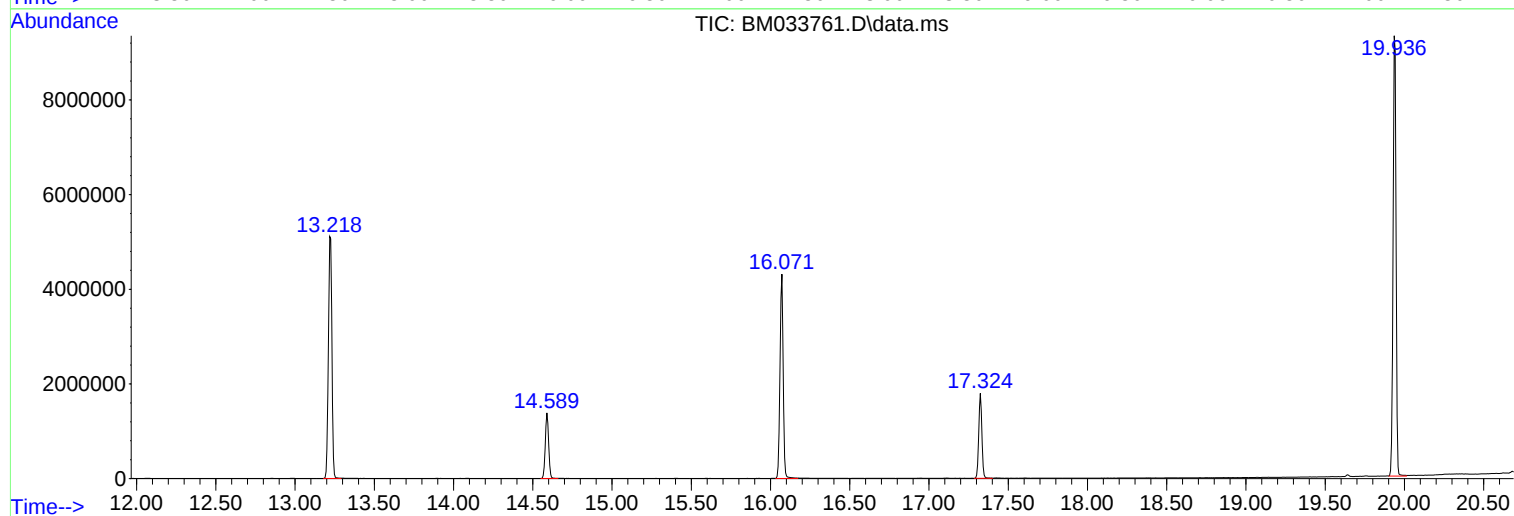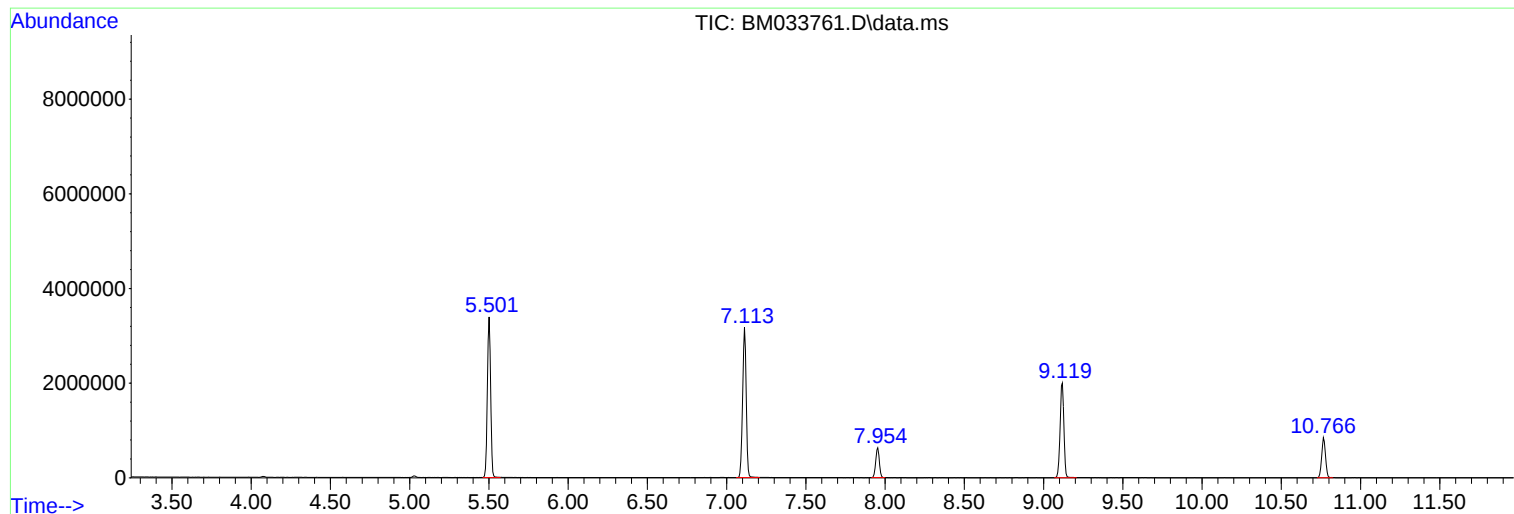

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011822\
Data File : BM033761.D
Acq On : 18 Jan 2022 13:25
Operator : CG/JU
Sample : PB142061BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB142061BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM011722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011822\
Data File : BM033761.D
Acq On : 18 Jan 2022 13:25
Operator : CG/JU
Sample : PB142061BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB142061BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM011722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------