
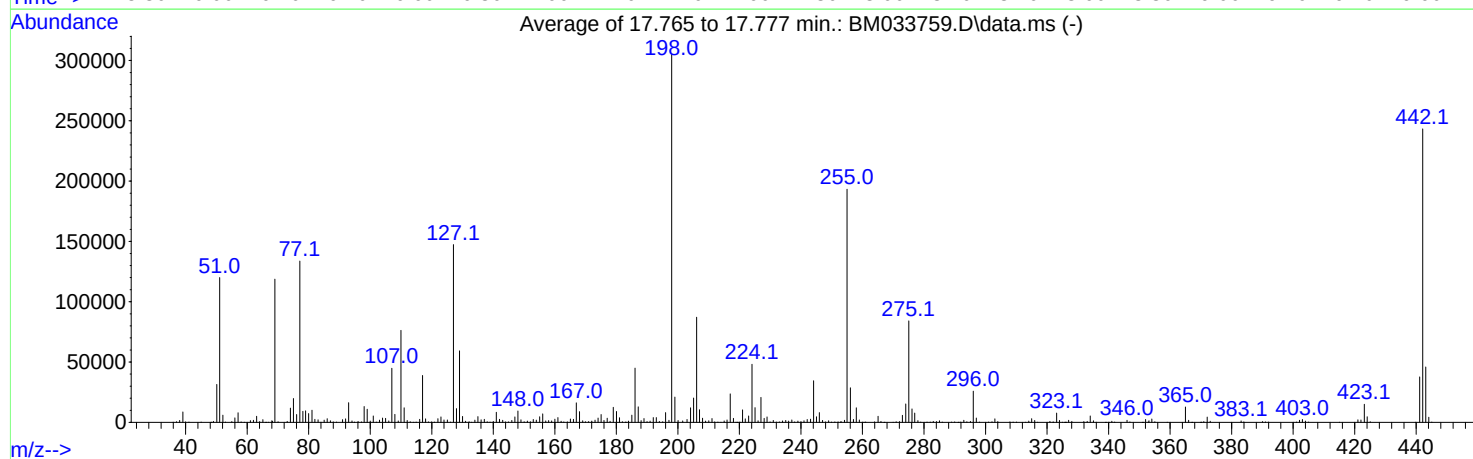


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011822\
 Data File : BM033759.D
 Acq On : 18 Jan 2022 11:56
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM011722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 17 16:30:56 2022

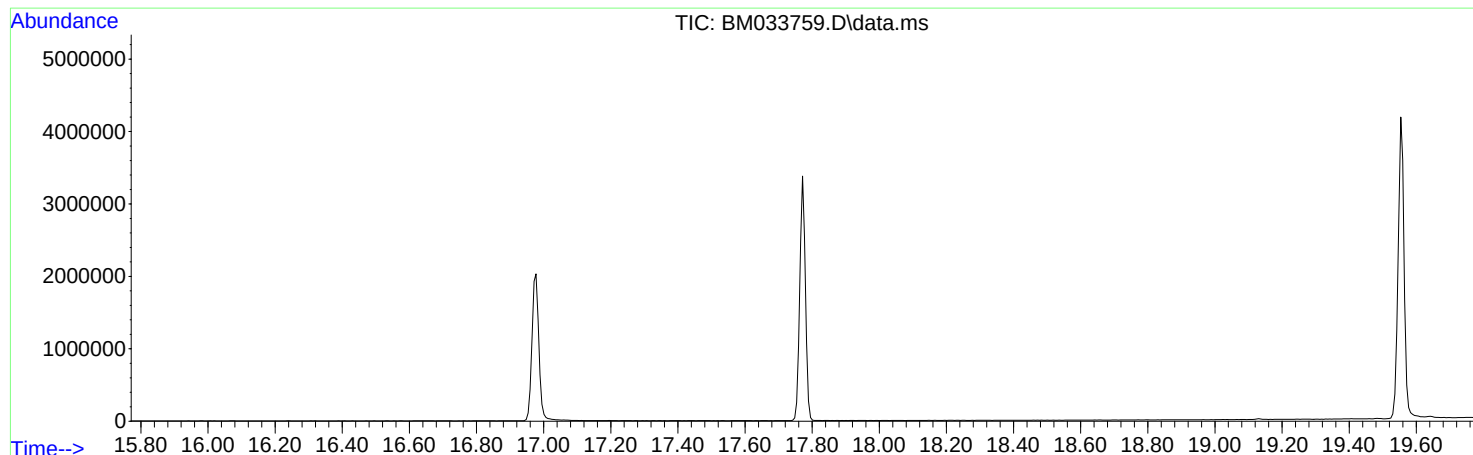




AutoFind: Scans 2470, 2471, 2472; Background Corrected with Scan 2463

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.4	120011	PASS
68	69	0.00	2	1.1	1307	PASS
69	198	0.00	100	38.9	118757	PASS
70	69	0.00	2	0.5	559	PASS
127	198	10	80	48.3	147347	PASS
197	198	0.00	2	0.6	1711	PASS
198	198	100	100	100.0	304981	PASS
199	198	5	9	6.9	20923	PASS
275	198	10	60	27.6	84080	PASS
365	198	1	100	4.2	12762	PASS
441	198	0.01	100	12.3	37664	PASS
442	442	50	100	100.0	243264	PASS
443	442	15	24	18.9	45899	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011822\
 Data File : BM033759.D
 Acq On : 18 Jan 2022 11:56
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Jan 19 04:50:00 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM011722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 17 16:30:56 2022
 Response via : Initial Calibration

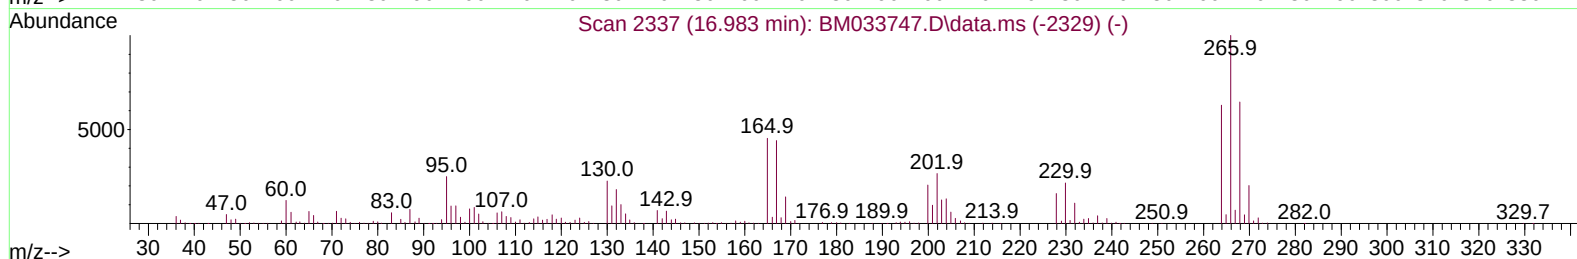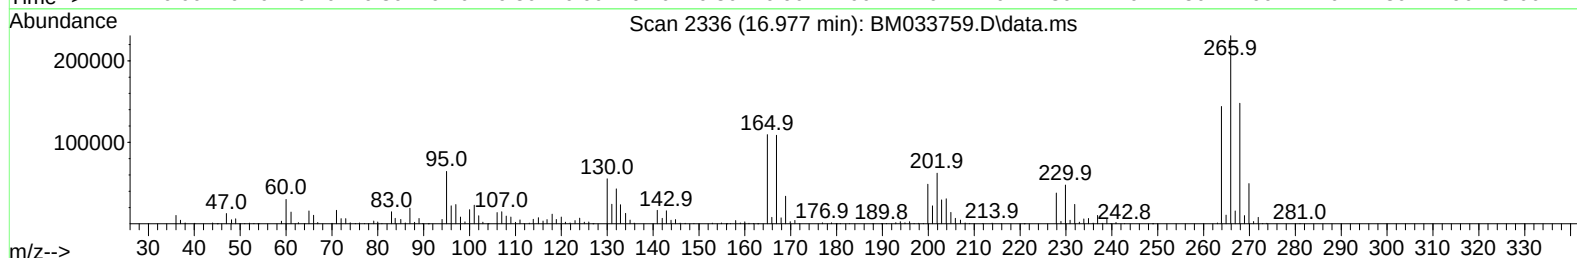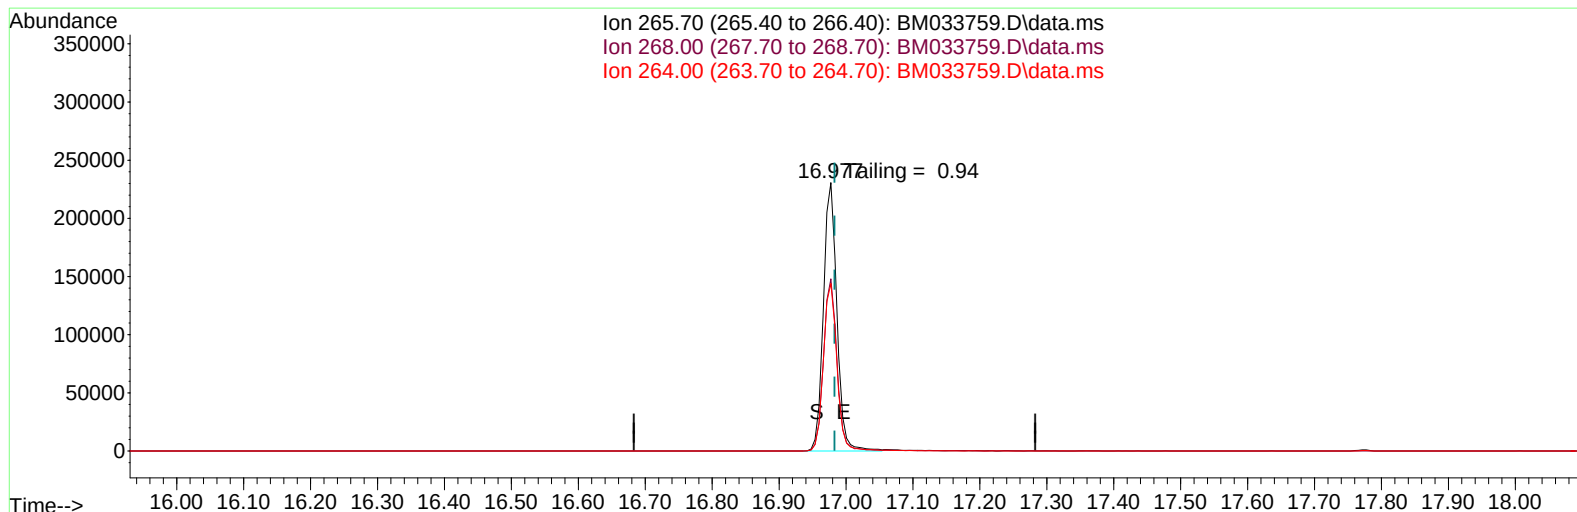

TIC: BM033759.D\data.ms

(70) Pentachlorophenol (C)

16.977min (-0.006) 0.00 ng




response 324582

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	64.13
264.00	61.40	62.44
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011822\
 Data File : BM033759.D
 Acq On : 18 Jan 2022 11:56
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Jan 19 04:50:00 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM011722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 17 16:30:56 2022
 Response via : Initial Calibration

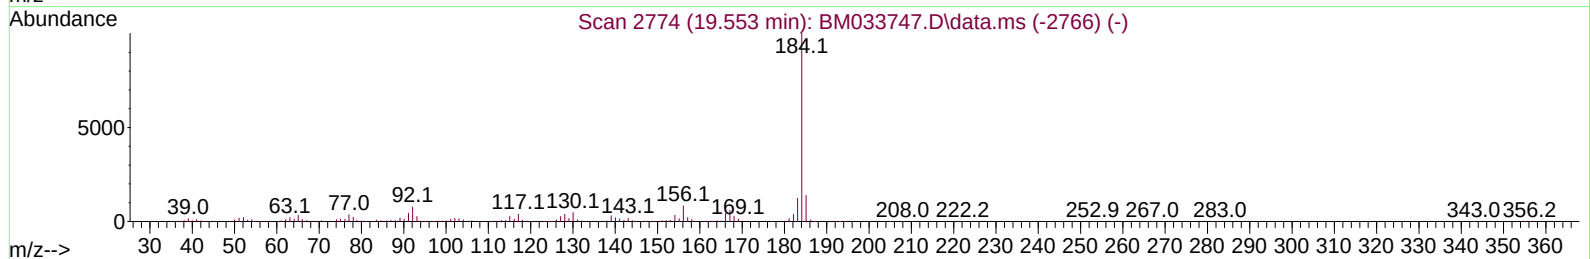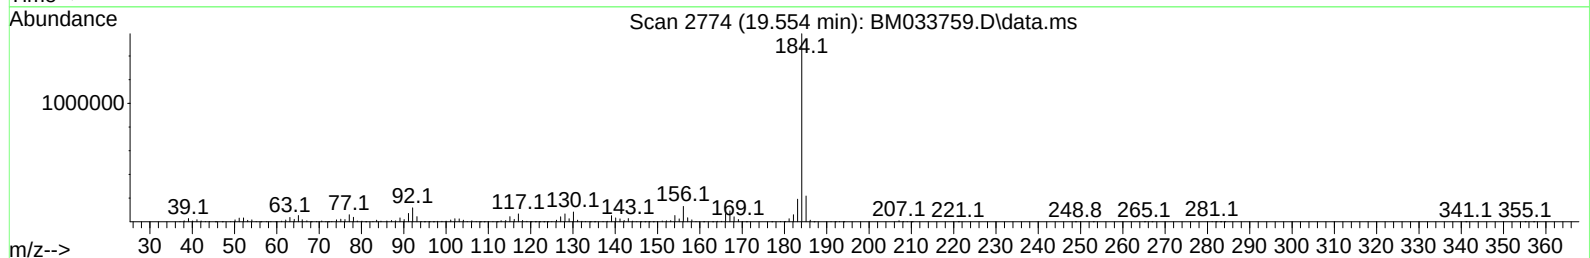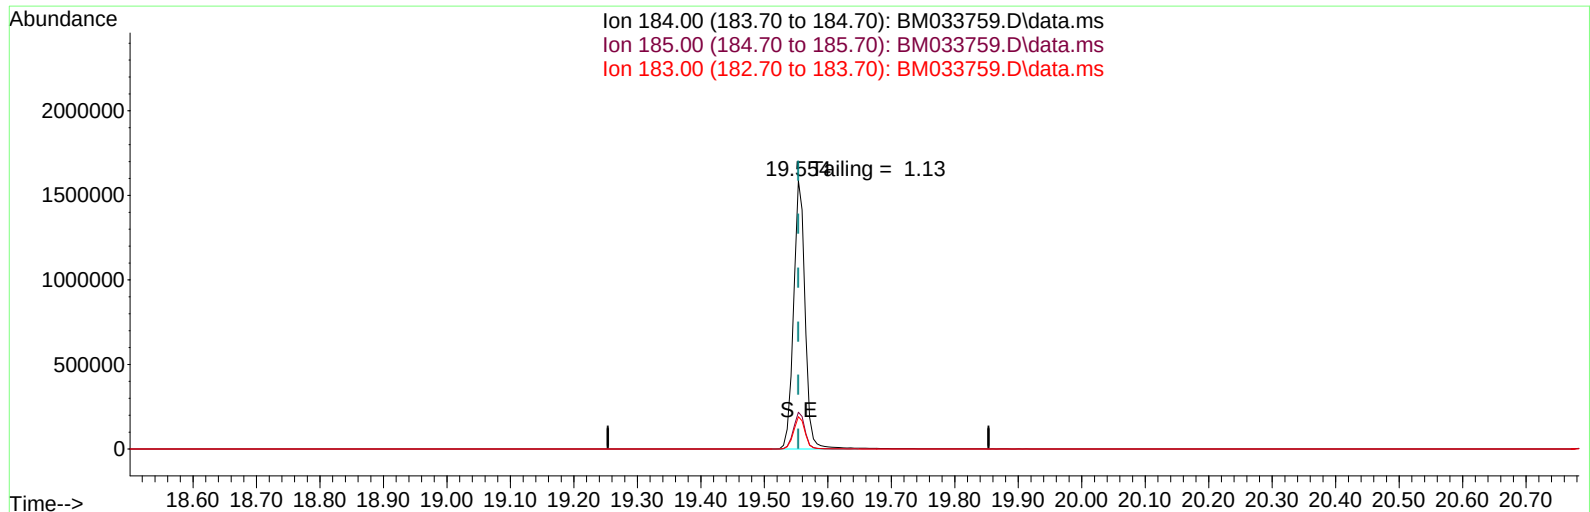

TIC: BM033759.D\data.ms

(77) Benzidine

19.554min (+ 0.000) 0.00 ng

response 2023513

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	13.71
183.00	12.10	12.04
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/18/2022	BNA_M	<u>BM033759.D</u>
Compound Name	Response	Retention Time
DDT	1096793	20.789
DDD	9489	20.354
DDE	1505	19.848
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10994	1107787	0.99

Instrument :
BNA_M
ClientSampleId :
DFTPP