

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM012015\
 Data File : BM000296.D
 Acq On : 21 Jan 2015 12:18
 Operator : TP/IZ
 Sample : PB81379BL
 Misc : SBLK02
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ClientSampleId :
 SBLK02

Quant Time: Jan 22 02:26:43 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM122914.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jan 22 02:18:27 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.82	152	131414	20.00	ng/ul	0.00
18) Naphthalene-d8	10.61	136	512274	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.46	164	322704	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.20	188	636852	20.00	ng/ul	0.00
75) Chrysene-d12	21.39	240	736720	20.00	ng/ul	0.00
83) Perylene-d12	23.68	264	712137	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.31	96	15405	6.80	ng/uL	0.00
5) Phenol-d5	6.98	99	305737	27.66	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.15	67	215379	30.82	ng/ul	0.00
9) 2-Chlorophenol-d4	7.35	132	231530	28.56	ng/ul	0.00
13) 4-Methylphenol-d8	8.52	113	225520	25.64	ng/ul	0.00
19) Nitrobenzene-d5	8.97	128	116886	32.99	ng/ul	0.00
22) 2-Nitrophenol-d4	9.69	143	111150	30.73	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.23	165	214152	26.80	ng/ul	0.00
29) 4-Chloroaniline-d4	10.75	131	63183	6.97	ng/ul	0.00
43) Dimethylphthalate-d6	13.86	166	674457	28.34	ng/ul	0.00
46) Acenaphthylene-d8	14.15	160	854072	29.95	ng/ul	0.00
51) 4-Nitrophenol-d4	14.64	143	82362	21.26	ng/ul	0.00
57) Fluorene-d10	15.44	176	591720	28.95	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.56	200	67627	22.41	ng/ul	0.00
70) Anthracene-d10	17.30	188	889449	30.20	ng/ul	0.00
76) Pyrene-d10	19.59	212	998794	29.39	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.53	264	979002	30.29	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) 2,6-Dinitrotoluene	13.86	165	5429	1.28	ng/ul#	27


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM012015\
Data File : BM000296.D
Acq On : 21 Jan 2015 12:18
Operator : TP/IZ
Sample : PB81379BL
Misc : SBLK02
ALS Vial : 36 Sample Multiplier: 1

Instrument :
ClientSampleId :
SBLK02

Quant Time: Jan 22 02:26:43 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM122914.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jan 22 02:18:27 2015
Response via : Initial Calibration

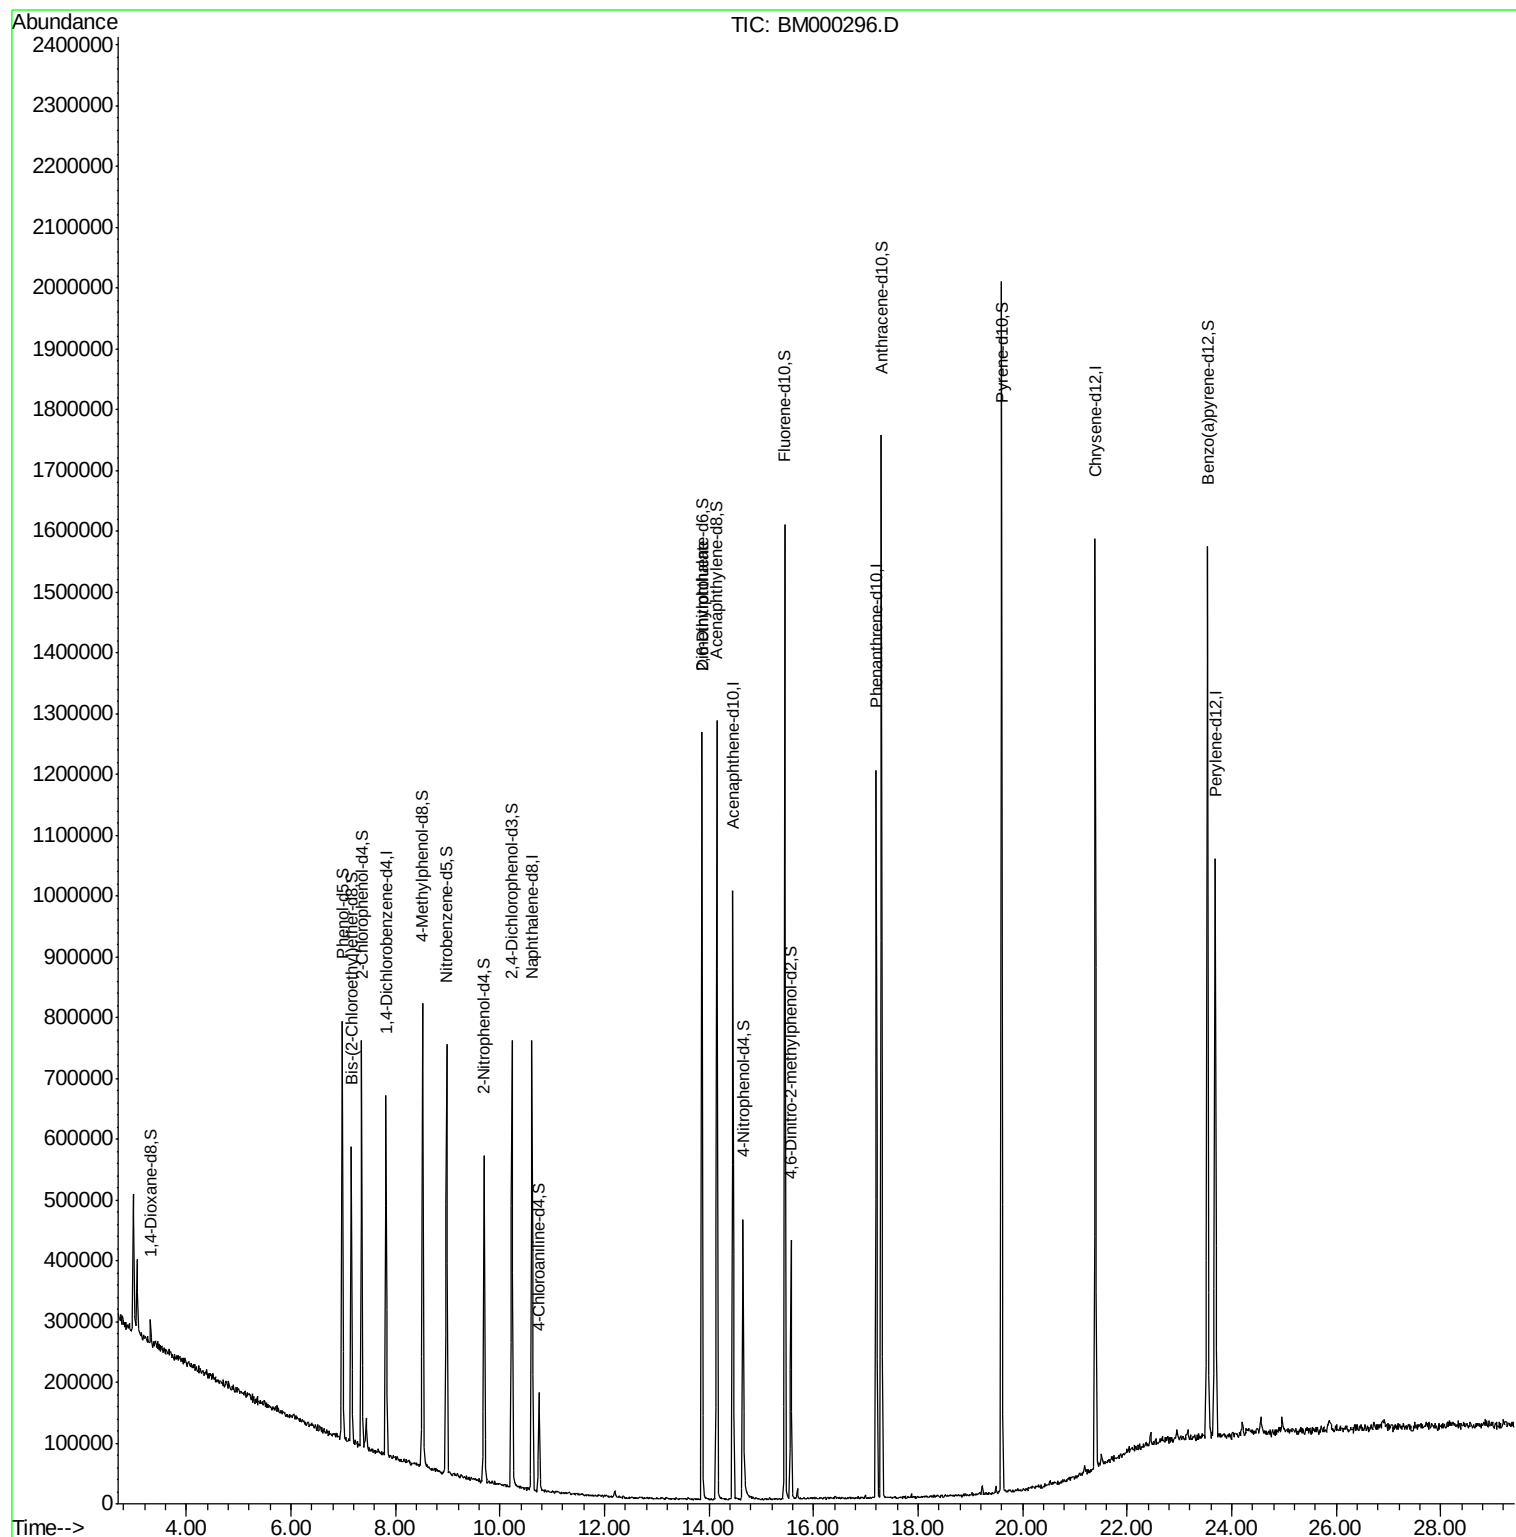

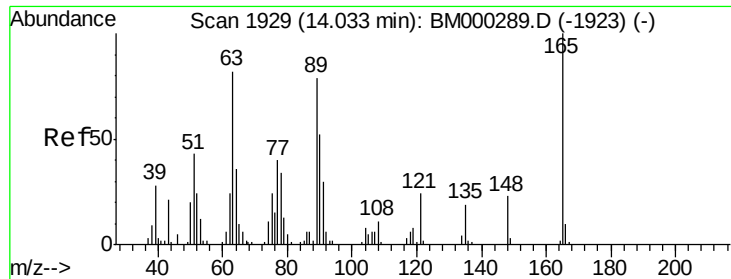

#45
 2,6-Dinitrotoluene
 Concen: 1.28 ng/ul
 RT: 13.86 min Scan# 1900
 Delta R.T. -0.17 min
 Lab File: BM000296.D
 Acq: 21 Jan 2015 12:18

Instrument :
 ClientSampleId :
 SBLK02

Tgt Ion:165 Resp: 5429
 Ion Ratio Lower Upper
 165 100
 89 0.0 54.4 81.6#
 121 43.2 18.6 28.0#

