

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM012015\
 Data File : BM000302.D
 Acq On : 21 Jan 2015 15:51
 Operator : TP/IZ
 Sample : G1105-14
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 ClientSampleId :
 C0AW0

Quant Time: Jan 22 02:27:32 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM122914.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jan 22 02:18:27 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.82	152	160075	20.00	ng/ul	0.00
18) Naphthalene-d8	10.61	136	642728	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.46	164	415852	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.20	188	787361	20.00	ng/ul	0.00
75) Chrysene-d12	21.39	240	813444	20.00	ng/ul	0.00
83) Perylene-d12	23.68	264	807911	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.31	96	14737	5.34	ng/uL	0.00
5) Phenol-d5	6.98	99	300631	22.33	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.15	67	221248	25.99	ng/ul	0.00
9) 2-Chlorophenol-d4	7.35	132	224900	22.78	ng/ul	0.00
13) 4-Methylphenol-d8	8.52	113	228980	21.37	ng/ul	0.00
19) Nitrobenzene-d5	8.98	128	121185	27.26	ng/ul	0.00
22) 2-Nitrophenol-d4	9.69	143	120519	26.56	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.23	165	216371	21.58	ng/ul	0.00
29) 4-Chloroaniline-d4	10.75	131	213431	18.76	ng/ul	0.00
43) Dimethylphthalate-d6	13.86	166	695082	22.66	ng/ul	0.00
46) Acenaphthylene-d8	14.15	160	846100	23.03	ng/ul	0.00
51) 4-Nitrophenol-d4	14.65	143	78263	15.68	ng/ul	0.00
57) Fluorene-d10	15.45	176	580488	22.04	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.56	200	65516	17.56	ng/ul	0.00
70) Anthracene-d10	17.30	188	851821	23.40	ng/ul	0.00
76) Pyrene-d10	19.59	212	911640	24.29	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.53	264	845379	23.05	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.91	163	119264	3.90	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM012015\
Data File : BM000302.D
Acq On : 21 Jan 2015 15:51
Operator : TP/IZ
Sample : G1105-14
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
ClientSampleId :
C0AW0

Quant Time: Jan 22 02:27:32 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM122914.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jan 22 02:18:27 2015
Response via : Initial Calibration

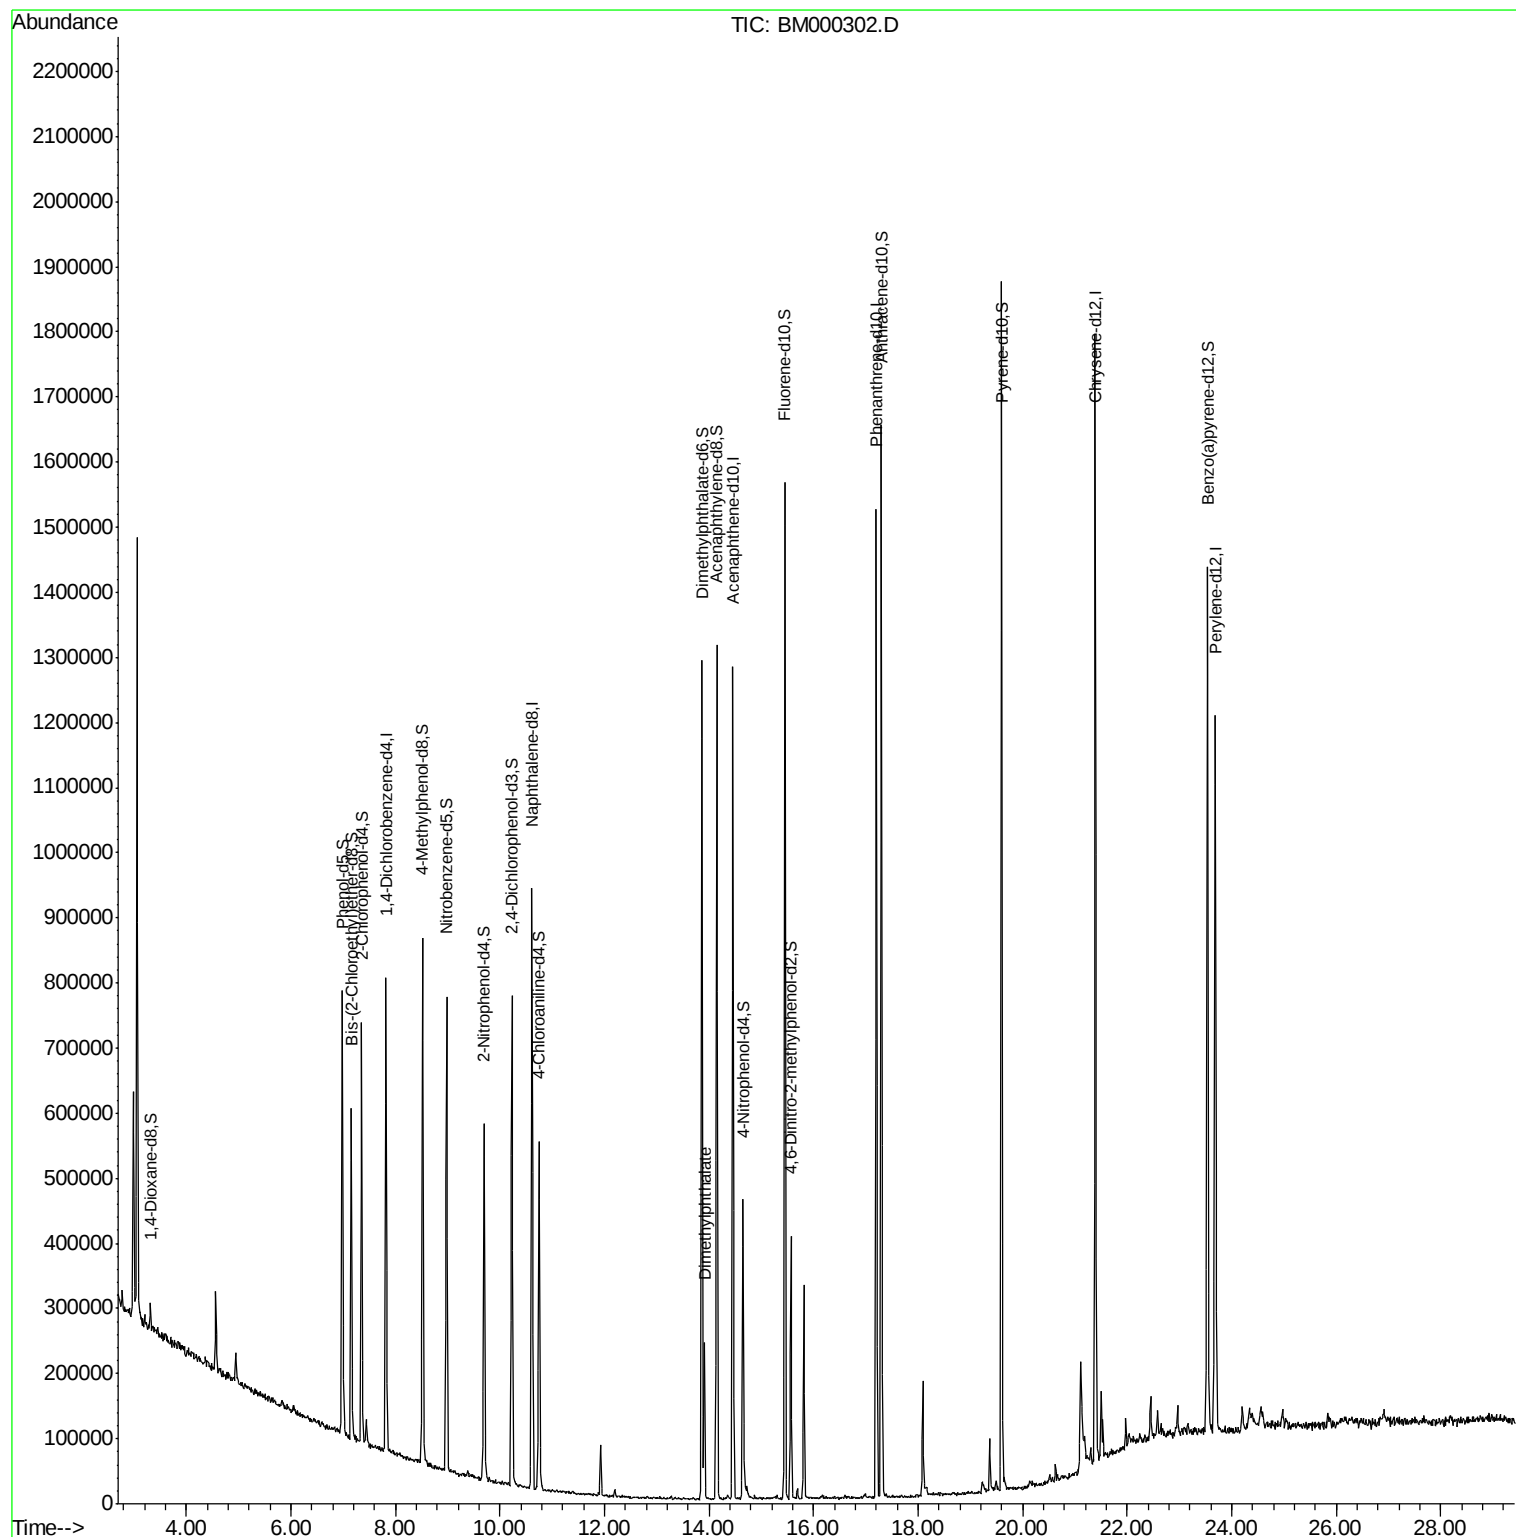

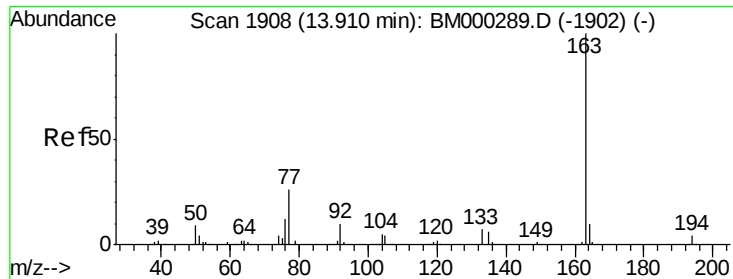

#44

Dimethylphthalate

Concen: 3.90 ng/ul

RT: 13.91 min Scan# 1908

Delta R.T. 0.00 min


Lab File: BM000302.D

Acq: 21 Jan 2015 15:51

Instrument :

ClientSampleId :

C0AW0

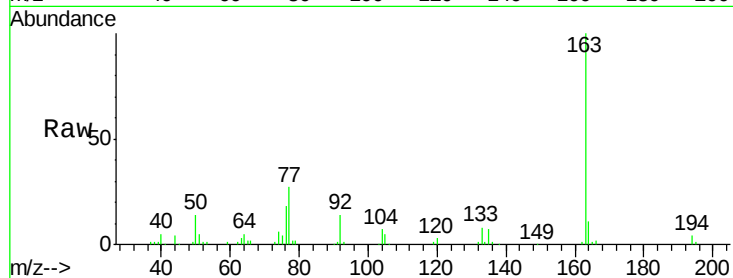

Tgt Ion:	163	Resp:	119264
Ion	Ratio	Lower	Upper
163	100		
194	3.9	3.0	4.4
164	11.0	8.5	12.7

