

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM012015\
 Data File : BM000308.D
 Acq On : 21 Jan 2015 20:35
 Operator : TP/IZ
 Sample : G1115-03
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 ClientSampleId :

Quant Time: Jan 22 02:28:51 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM122914.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jan 22 02:18:27 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.82	152	106574	20.00	ng/ul	0.00
18) Naphthalene-d8	10.61	136	392467	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.46	164	248729	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.20	188	489705	20.00	ng/ul	0.00
75) Chrysene-d12	21.39	240	580062	20.00	ng/ul	0.00
83) Perylene-d12	23.67	264	587541	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.29	96	67251	36.59	ng/uL	-0.02
5) Phenol-d5	6.98	99	58906	6.57	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.15	67	171796	30.32	ng/ul	0.00
9) 2-Chlorophenol-d4	7.35	132	145555	22.14	ng/ul	0.00
13) 4-Methylphenol-d8	8.52	113	94378	13.23	ng/ul	0.00
19) Nitrobenzene-d5	8.97	128	94113	34.68	ng/ul	0.00
22) 2-Nitrophenol-d4	9.69	143	90450	32.65	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.23	165	161835	26.44	ng/ul	0.00
29) 4-Chloroaniline-d4	10.75	131	8125	1.17	ng/ul	0.00
43) Dimethylphthalate-d6	13.86	166	569907	31.07	ng/ul	0.00
46) Acenaphthylene-d8	14.15	160	707395	32.19	ng/ul	0.00
51) 4-Nitrophenol-d4	14.65	143	12776	4.28	ng/ul	0.00
57) Fluorene-d10	15.44	176	503530	31.96	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.56	200	54897	23.65	ng/ul	0.00
70) Anthracene-d10	17.30	188	769989	34.00	ng/ul	0.00
76) Pyrene-d10	19.59	212	874556	32.68	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.53	264	868361	32.56	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) 1,4-Dioxane	3.35	88	2806	1.10	ng/uL	94
44) Dimethylphthalate	13.90	163	51214	2.80	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM012015\
Data File : BM000308.D
Acq On : 21 Jan 2015 20:35
Operator : TP/IZ
Sample : G1115-03
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
ClientSampleId :

Quant Time: Jan 22 02:28:51 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM122914.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jan 22 02:18:27 2015
Response via : Initial Calibration

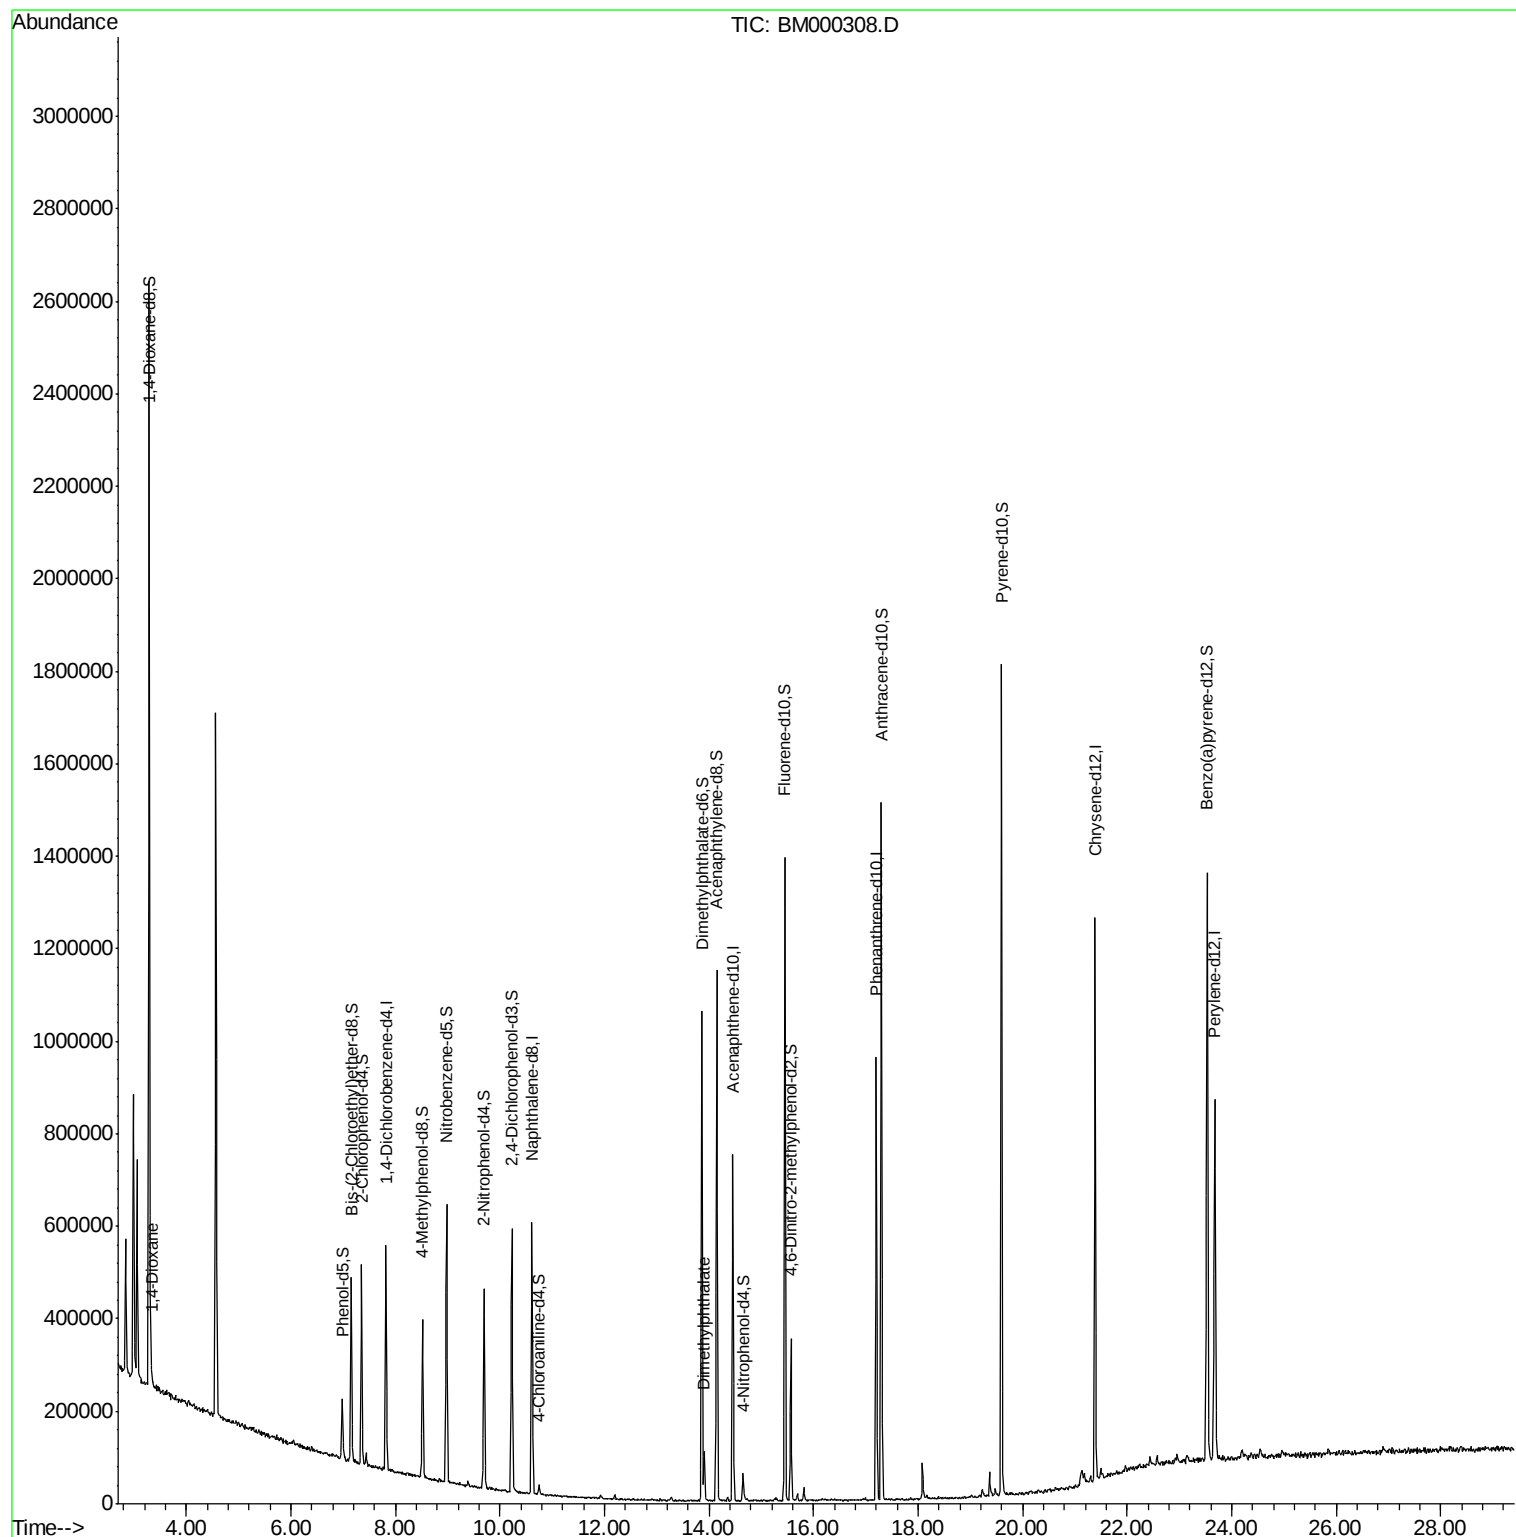

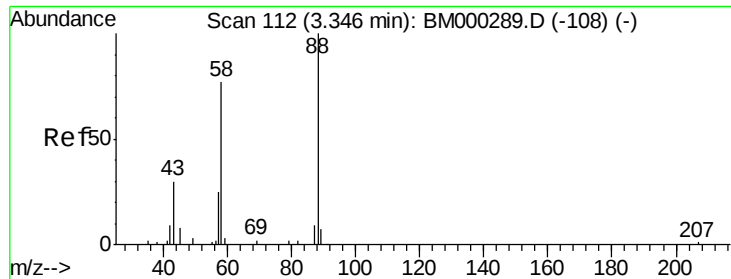

#2

1,4-Dioxane

Concen: 1.10 ng/uL

RT: 3.35 min Scan# 112





Delta R.T. 0.00 min

Lab File: BM000308.D

Acq: 21 Jan 2015 20:35

Instrument :
ClientSampled :

Tgt Ion:	88	Resp:	2806
Ion	Ratio	Lower	Upper
88	100		
43	45.5	34.9	52.3
58	76.9	67.3	100.9

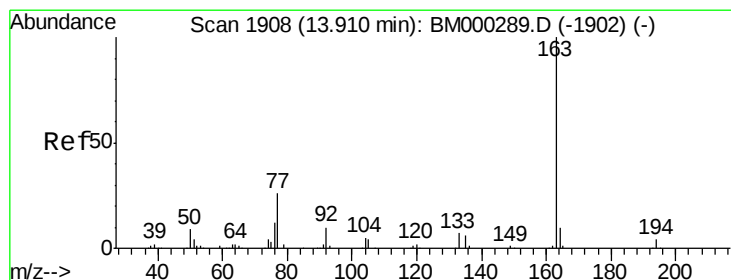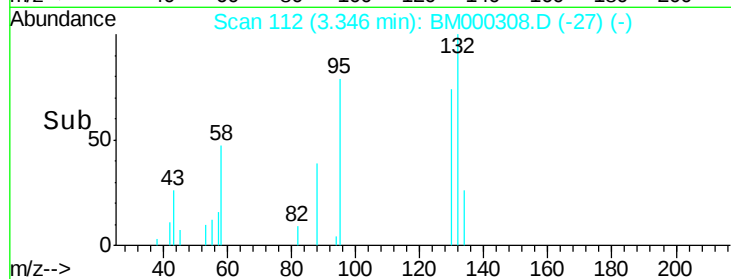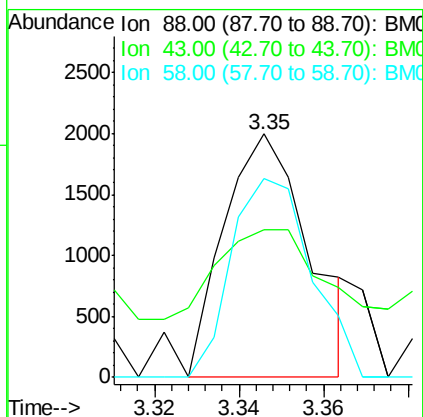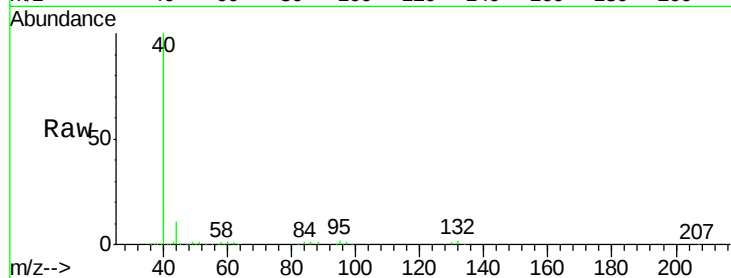

#44

Dimethylphthalate

Concen: 2.80 ng/uL

RT: 13.90 min Scan# 1907

Delta R.T. -0.01 min

Lab File: BM000308.D

Acq: 21 Jan 2015 20:35

Tgt Ion:	163	Resp:	51214
Ion	Ratio	Lower	Upper
163	100		
194	3.9	3.0	4.4
164	12.1	8.5	12.7

