

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM012015\
 Data File : BM000269.D
 Acq On : 20 Jan 2015 18:38
 Operator : TP/IZ
 Sample : G1065-09
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ClientSampleId :
 C0AJ1

Quant Time: Jan 21 01:19:29 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM122914.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 21 00:20:03 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.82	152	140472	20.00	ng/ul	0.00
18) Naphthalene-d8	10.61	136	550788	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.46	164	356613	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.20	188	726091	20.00	ng/ul	0.00
75) Chrysene-d12	21.39	240	807496	20.00	ng/ul	0.00
83) Perylene-d12	23.68	264	778087	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.31	96	10055	4.15	ng/uL	0.00
5) Phenol-d5	6.98	99	224078	18.96	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.15	67	162441	21.75	ng/ul	0.00
9) 2-Chlorophenol-d4	7.35	132	169699	19.58	ng/ul	0.00
13) 4-Methylphenol-d8	8.52	113	174194	18.53	ng/ul	0.00
19) Nitrobenzene-d5	8.97	128	88242	23.17	ng/ul	0.00
22) 2-Nitrophenol-d4	9.70	143	89785	23.09	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.23	165	164002	19.09	ng/ul	0.00
29) 4-Chloroaniline-d4	10.75	131	202307	20.76	ng/ul	0.00
43) Dimethylphthalate-d6	13.86	166	527892	20.07	ng/ul	0.00
46) Acenaphthylene-d8	14.15	160	670705	21.29	ng/ul	0.00
51) 4-Nitrophenol-d4	14.65	143	67751	15.83	ng/ul	0.00
57) Fluorene-d10	15.45	176	465563	20.61	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.56	200	56460	16.41	ng/ul	0.00
70) Anthracene-d10	17.30	188	707952	21.09	ng/ul	0.00
76) Pyrene-d10	19.60	212	783862	21.04	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.53	264	728486	20.63	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
6) Phenol	7.01	94	34015	2.73	ng/ul#	86
44) Dimethylphthalate	13.91	163	59070	2.25	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM012015\
Data File : BM000269.D
Acq On : 20 Jan 2015 18:38
Operator : TP/IZ
Sample : G1065-09
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ClientSampled :
C0AJ1

Quant Time: Jan 21 01:19:29 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM122914.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jan 21 00:20:03 2015
Response via : Initial Calibration

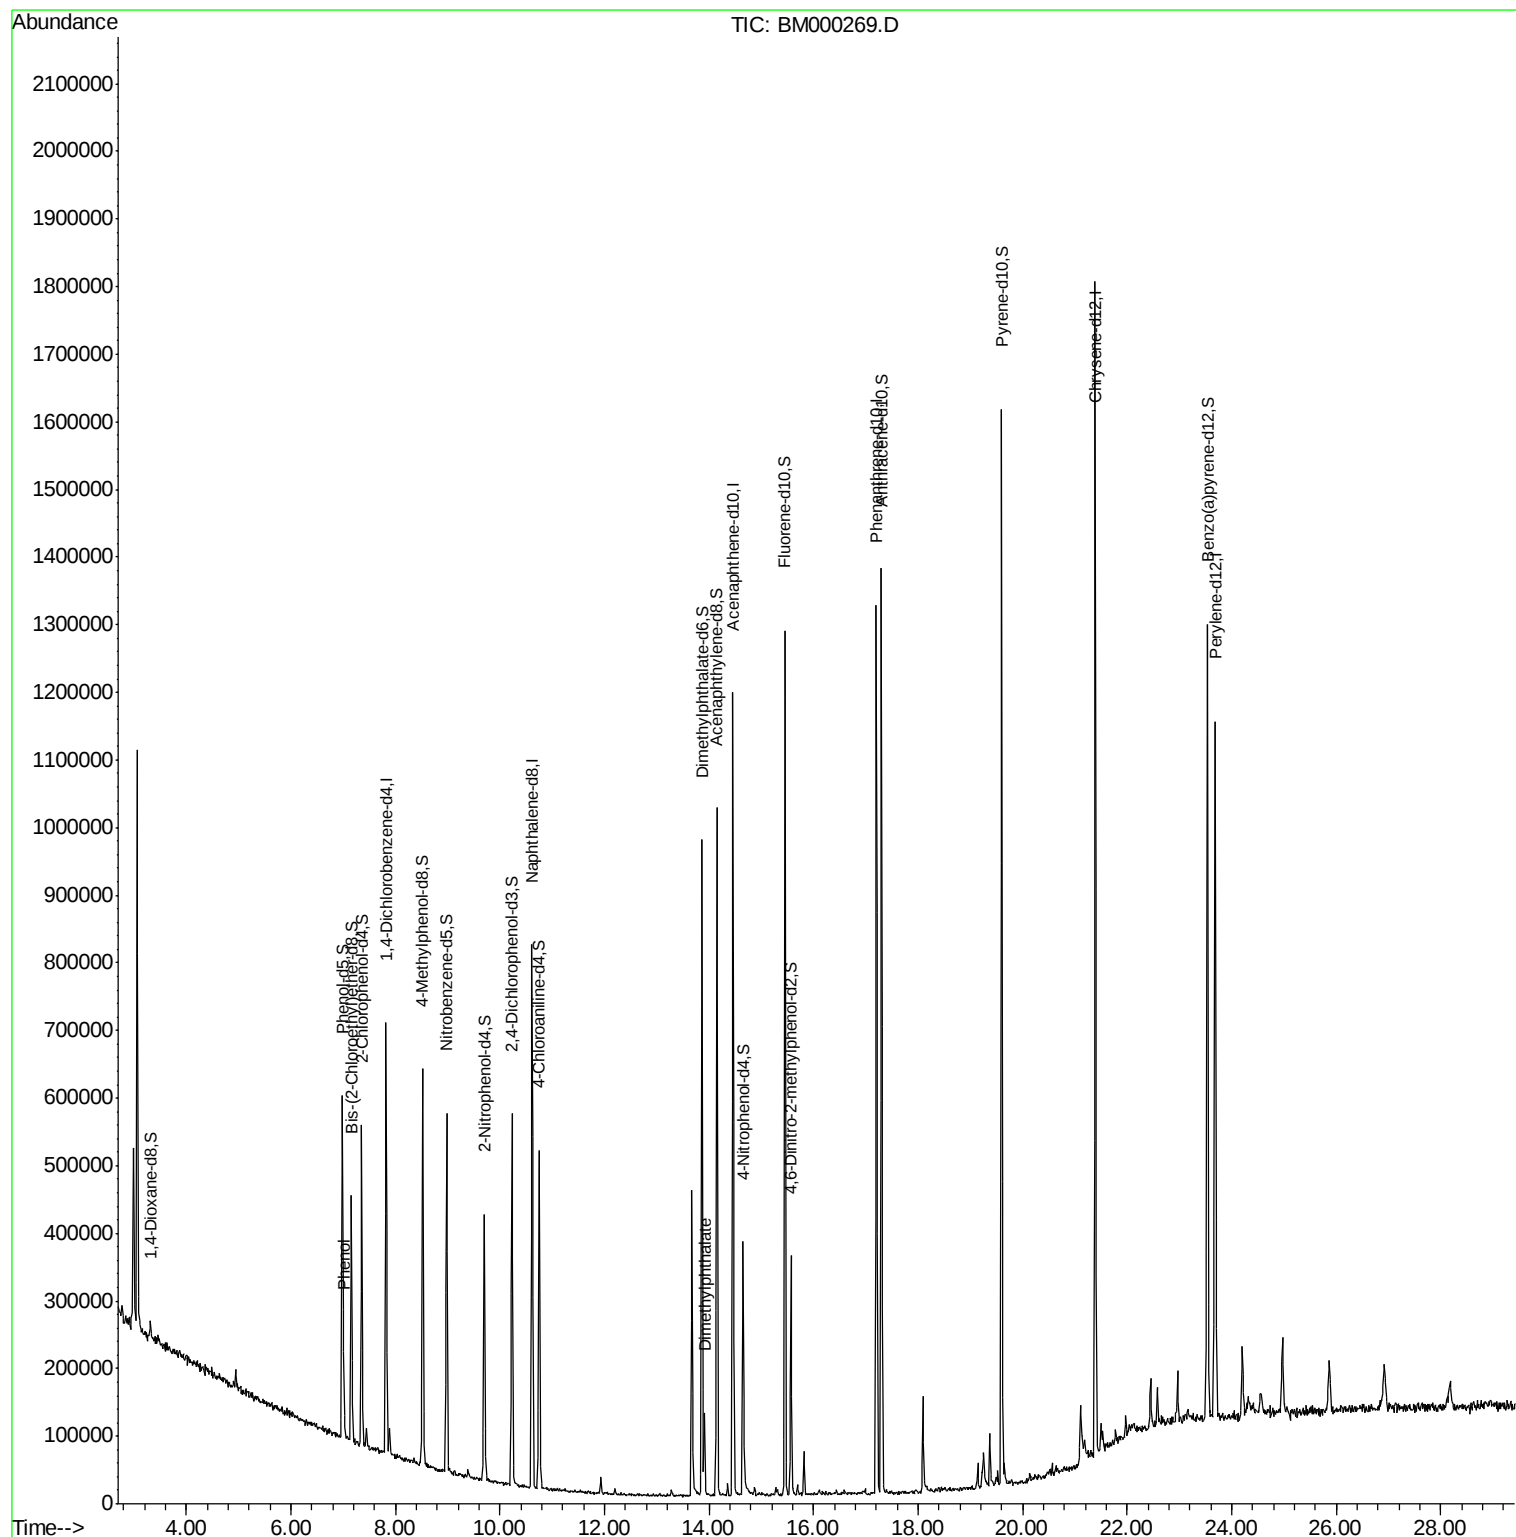

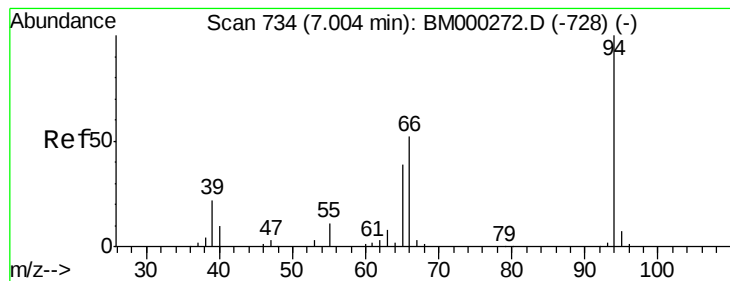

#6

Phenol

Concen: 2.73 ng/ul

RT: 7.01 min Scan# 735

Delta R.T. 0.00 min


Lab File: BM000269.D

Acq: 20 Jan 2015 18:38

Instrument :
ClientSampled :
C0AJ1

Tgt Ion: 94 Resp: 34015




Ion	Ratio	Lower	Upper
94	100		
65	42.2	27.4	41.0#
66	63.3	42.5	63.7

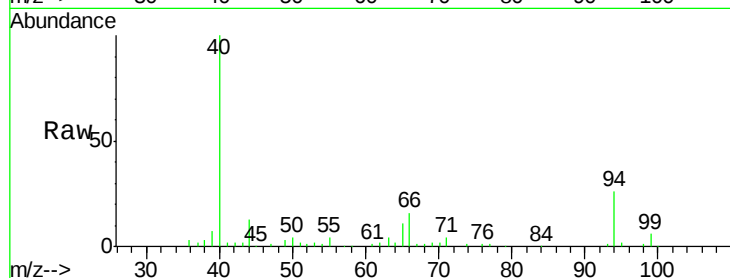

Abundance Ion 94.00 (93.70 to 94.70): BM000272.D (-728) (-)

Ion 65.00 (64.70 to 65.70): BM000272.D (-728) (-)

Ion 66.00 (65.70 to 66.70): BM000272.D (-728) (-)

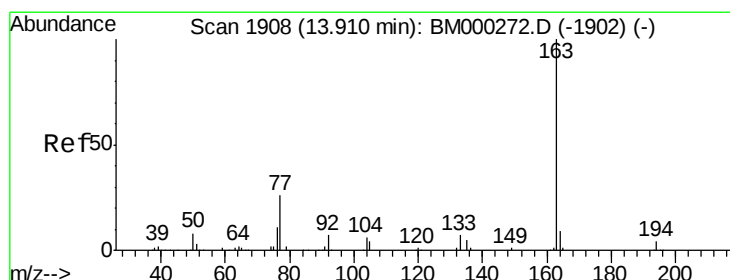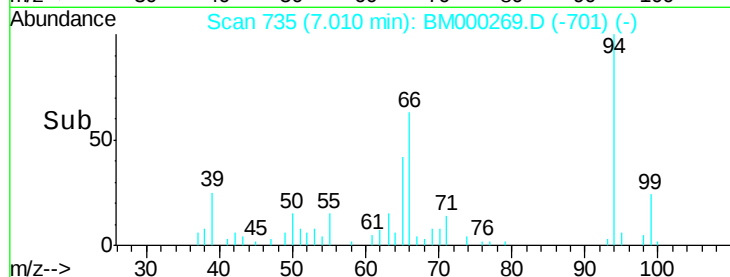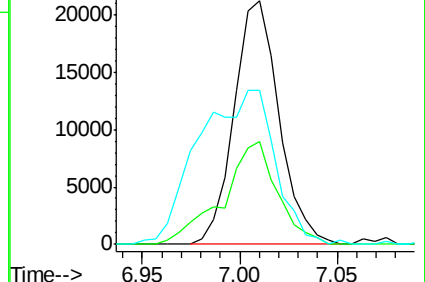

#44

Dimethylphthalate

Concen: 2.25 ng/ul

RT: 13.91 min Scan# 1908


Delta R.T. -0.01 min

Lab File: BM000269.D

Acq: 20 Jan 2015 18:38

Tgt Ion: 163 Resp: 59070

Ion	Ratio	Lower	Upper
163	100		
194	3.9	3.0	4.4
164	9.7	8.5	12.7

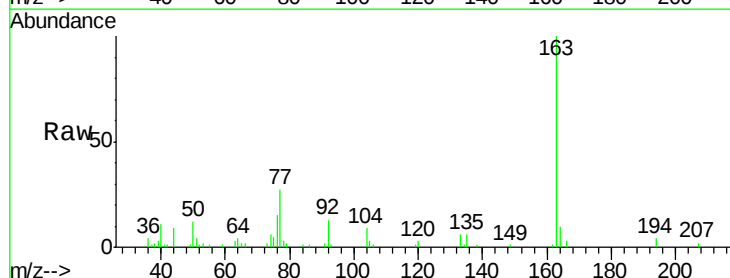

Abundance Ion 163.00 (162.70 to 163.70): BM000272.D (-1902) (-)

Ion 194.00 (193.70 to 194.70): BM000272.D (-1902) (-)

Ion 164.00 (163.70 to 164.70): BM000272.D (-1902) (-)

