

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM012015\
 Data File : BM000273.D
 Acq On : 20 Jan 2015 21:35
 Operator : TP/IZ
 Sample : G1102-04
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ClientSampleId :
 C0AD4

Quant Time: Jan 21 02:33:09 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM122914.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 21 02:17:47 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.82	152	125454	20.00	ng/ul	0.00
18) Naphthalene-d8	10.61	136	481878	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.46	164	320848	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.20	188	645520	20.00	ng/ul	0.00
75) Chrysene-d12	21.39	240	726835	20.00	ng/ul	0.00
83) Perylene-d12	23.68	264	719601	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.31	96	16514	7.63	ng/uL	0.00
5) Phenol-d5	6.98	99	357191	33.85	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.15	67	241697	36.23	ng/ul	0.00
9) 2-Chlorophenol-d4	7.35	132	263871	34.10	ng/ul	0.00
13) 4-Methylphenol-d8	8.52	113	262564	31.27	ng/ul	0.00
19) Nitrobenzene-d5	8.97	128	135408	40.63	ng/ul	0.00
22) 2-Nitrophenol-d4	9.70	143	131563	38.67	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.23	165	245839	32.71	ng/ul	0.00
29) 4-Chloroaniline-d4	10.75	131	323963	37.99	ng/ul	0.00
43) Dimethylphthalate-d6	13.86	166	804560	34.00	ng/ul	0.00
46) Acenaphthylene-d8	14.15	160	1003841	35.41	ng/ul	0.00
51) 4-Nitrophenol-d4	14.64	143	107443	27.90	ng/ul	0.00
57) Fluorene-d10	15.45	176	693885	34.15	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.56	200	89288	29.19	ng/ul	0.00
70) Anthracene-d10	17.30	188	1080748	36.21	ng/ul	0.00
76) Pyrene-d10	19.60	212	1183902	35.31	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.53	264	1123974	34.41	ng/ul	0.00


Target Compounds						Qvalue
6) Phenol	7.01	94	55231	4.96	ng/ul	87
44) Dimethylphthalate	13.91	163	73010	3.10	ng/ul#	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM012015\
Data File : BM000273.D
Acq On : 20 Jan 2015 21:35
Operator : TP/IZ
Sample : G1102-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ClientSampleId :
C0AD4

Quant Time: Jan 21 02:33:09 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM122914.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jan 21 02:17:47 2015
Response via : Initial Calibration

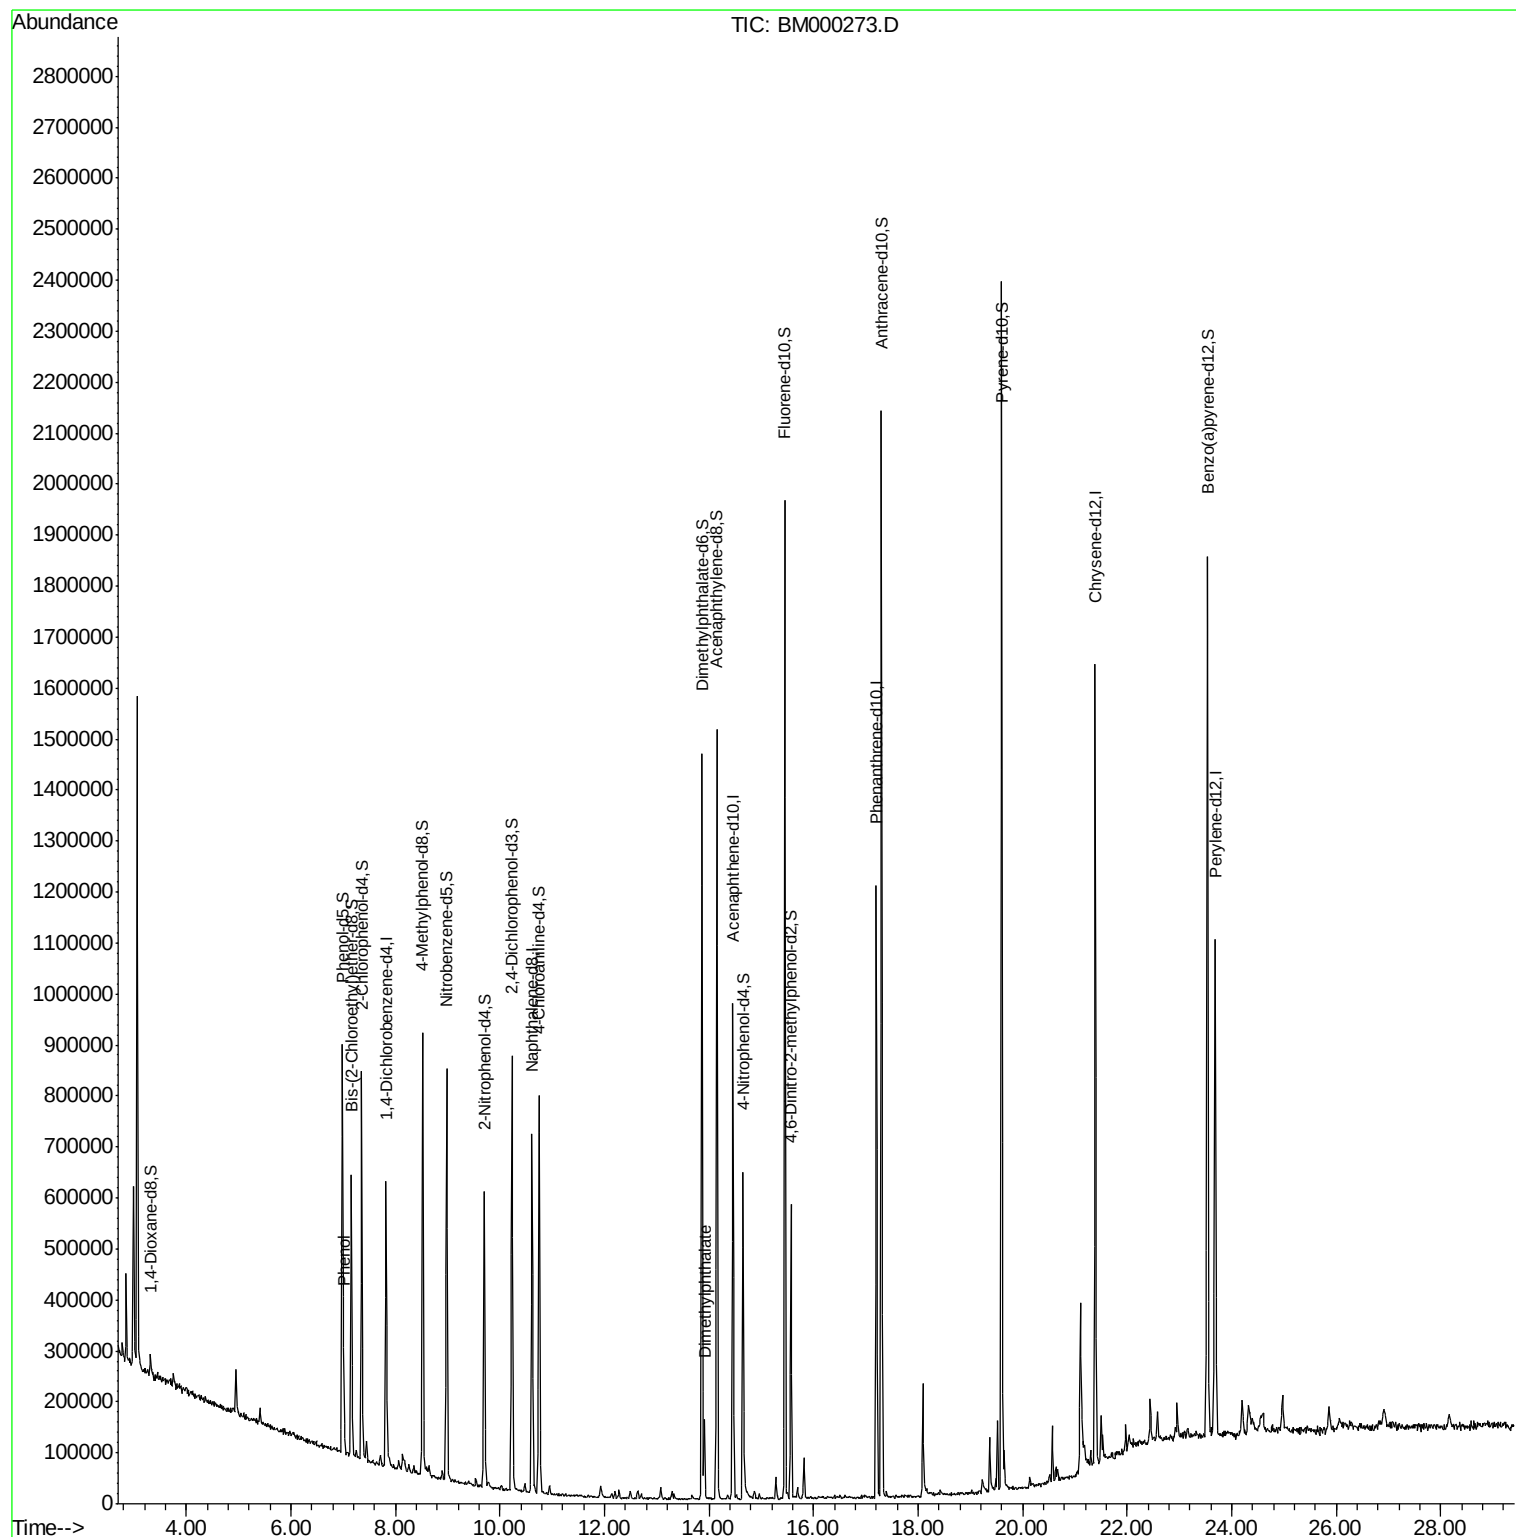

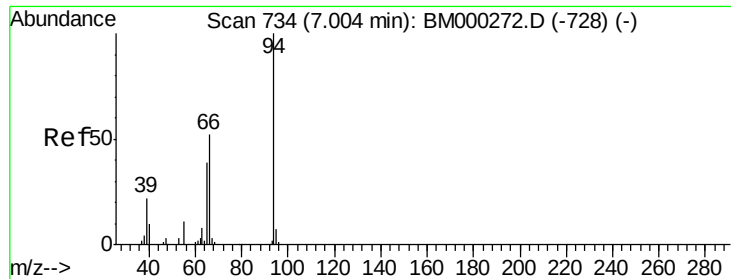

#6

Phenol

Concen: 4.96 ng/ul

RT: 7.01 min Scan# 735

Delta R.T. 0.01 min

Lab File: BM000273.D

Acq: 20 Jan 2015 21:35

Instrument :

ClientSampled :

C0AD4





Tgt Ion: 94 Resp: 55231

Ion Ratio Lower Upper

94 100

65 40.9 27.4 41.0

66 63.0 42.5 63.7

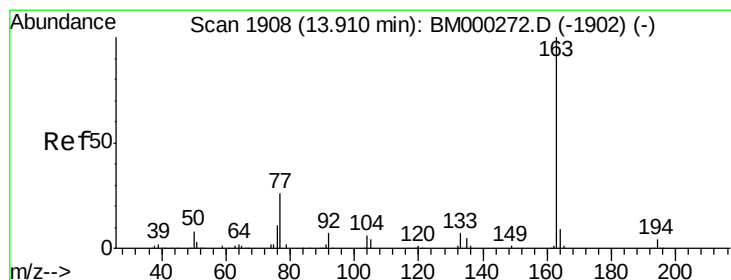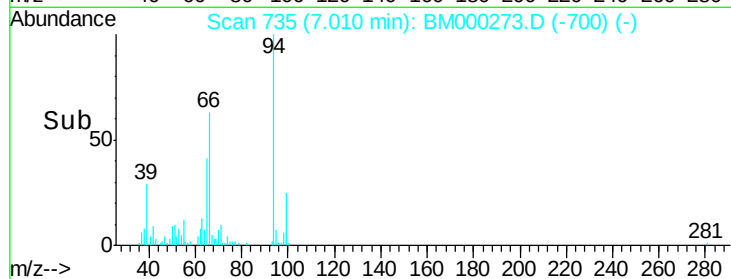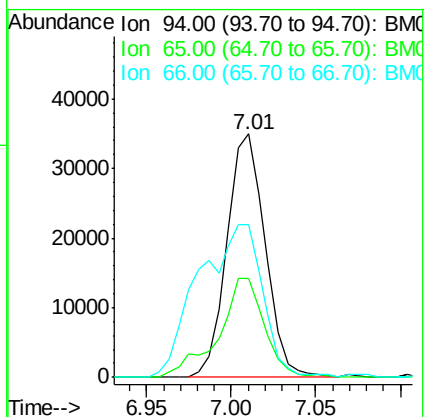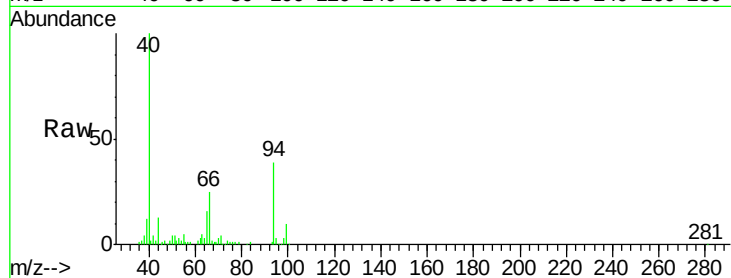

#44

Dimethylphthalate

Concen: 3.10 ng/ul

RT: 13.91 min Scan# 1908

Delta R.T. -0.00 min

Lab File: BM000273.D

Acq: 20 Jan 2015 21:35

Tgt Ion: 163 Resp: 73010

Ion Ratio Lower Upper

163 100

194 4.9 3.0 4.4#

164 10.8 8.5 12.7

