


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM012015\
 Data File : BM000259.D
 Acq On : 20 Jan 2015 09:51
 Operator : TP/IZ
 Sample : DFTPP10
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ClientSampleId :
 DFTPP10

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM122914.M
 Title : SVOA CALIBRATION
 Last Update : Wed Jan 14 12:47:10 2015

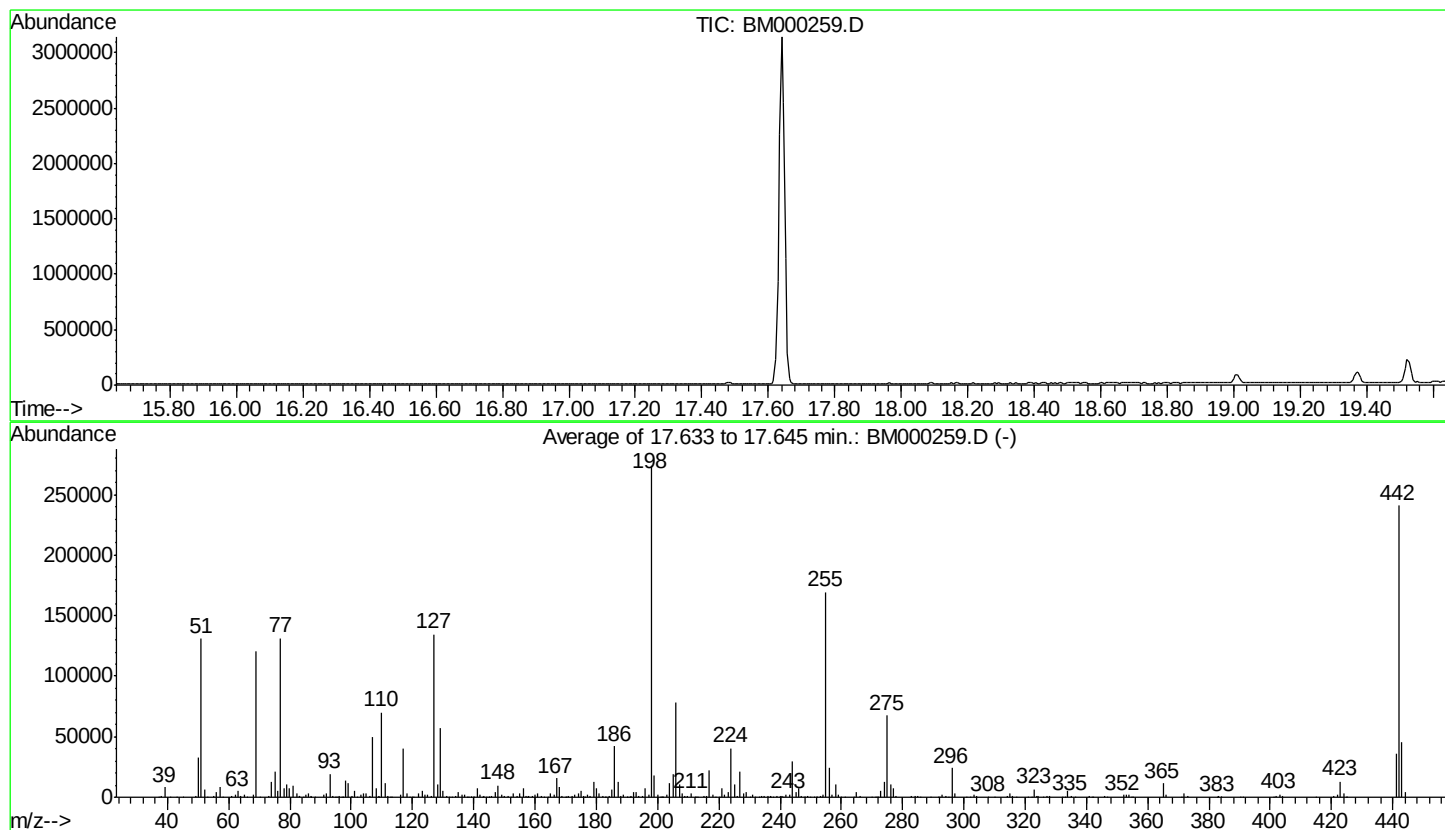

AutoFind: Scans 2541, 2542, 2543; Background Corrected with Scan 2535

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.8	130818	PASS
68	69	0.00	2	1.7	2083	PASS
69	198	0.00	100	43.9	120357	PASS
70	69	0.00	2	0.4	424	PASS
127	198	10	80	49.2	134784	PASS
197	198	0.00	2	0.8	2156	PASS
198	198	100	100	100.0	273962	PASS
199	198	5	9	6.7	18373	PASS
275	198	10	60	24.5	67245	PASS
365	198	1	100	4.2	11590	PASS
441	443	0.01	100	78.4	36098	PASS
442	198	50	100	87.9	240853	PASS
443	442	15	24	19.1	46021	PASS

m/z	Abundance
36.90	331.0
38.10	1003.0
39.10	8571.0
40.00	4922.0
41.10	516.0
44.00	6156.0
49.00	757.0
50.00	33056.0
51.00	128448.0
52.00	6900.0
53.00	326.0
54.90	839.0
56.00	4307.0
57.00	7849.0
58.00	578.0
61.00	1504.0
62.00	2184.0
63.00	4593.0
64.10	603.0
65.10	1896.0
66.00	424.0
68.00	1817.0
69.00	115192.0
70.00	632.0
73.10	1228.0
74.00	12028.0
75.00	20320.0
76.00	5395.0
77.00	127472.0
78.10	7457.0
79.10	9815.0
79.90	6997.0
81.00	10476.0
82.00	2918.0
82.90	1958.0
84.20	452.0
85.00	1752.0
86.00	2956.0
86.90	1502.0
87.90	483.0
91.00	2286.0
92.10	2409.0
93.00	17872.0
94.00	1223.0
94.80	308.0
96.00	731.0
98.00	12238.0
99.00	11861.0
100.10	1121.0
101.00	4937.0
102.00	423.0
103.00	1662.0
104.00	3486.0
105.10	2760.0
106.00	817.0
107.00	44112.0
108.00	7697.0
109.10	1010.0
110.00	65656.0
111.00	10676.0
112.10	1329.0
112.90	844.0
116.10	2027.0
117.00	36800.0
118.00	2907.0
119.00	456.0
122.00	2416.0
122.90	4260.0
124.10	2116.0
125.00	2397.0
126.00	614.0
127.00	127888.0
128.00	9018.0
129.00	51808.0
129.90	4871.0
131.00	1006.0
132.10	368.0
134.00	1074.0
135.00	3642.0
136.10	1297.0
137.10	2399.0
138.10	774.0
139.00	618.0
140.00	758.0
141.00	5478.0
141.90	2007.0
142.90	1700.0
143.90	471.0
145.20	415.0
145.90	1099.0
147.00	3437.0

Instrument :
ClientSampleId :
DFTPP10

148.00	8700.0
149.00	2193.0
150.00	648.0
151.20	1104.0
152.00	450.0
152.90	2736.0
154.00	1308.0
154.90	3093.0
156.00	6305.0
157.30	1205.0
158.00	1193.0
159.00	1481.0
160.00	2773.0
161.00	3440.0
162.00	893.0
163.00	431.0
164.00	459.0
165.00	2536.0
166.10	2402.0
167.00	13883.0
168.00	9096.0
169.00	1376.0
169.90	561.0
171.00	971.0
171.90	1435.0
173.00	1762.0
174.10	3427.0
175.00	4641.0
175.90	1145.0
176.20	1222.0
177.00	2184.0
178.00	1042.0
179.00	11359.0
180.00	7416.0
180.90	2657.0
182.10	540.0
184.10	785.0
185.00	5350.0
186.00	36432.0
187.00	11101.0
188.00	1297.0
189.00	1668.0
190.00	737.0
190.80	1684.0
192.00	3103.0
193.00	2859.0
194.00	1046.0
195.00	514.0
196.00	7368.0
197.00	1684.0
198.00	235072.0
199.00	16640.0
200.00	1291.0
201.30	765.0
203.00	1808.0
204.00	9082.0
205.10	15470.0
206.10	66744.0
207.10	10398.0
207.90	3411.0
209.00	953.0
210.00	872.0
211.00	2556.0
215.00	741.0
216.00	1635.0
217.00	16888.0
218.00	2254.0
221.00	5602.0
222.00	1970.0
223.00	3853.0
224.00	30736.0
225.00	9054.0
226.20	875.0
227.00	17984.0
227.90	2284.0
229.00	3359.0
230.10	469.0
231.00	1597.0
232.00	355.0
233.00	532.0
233.80	709.0
234.90	844.0
236.00	792.0
236.90	1400.0
238.90	674.0
239.80	345.0
240.10	305.0
240.80	577.0
242.00	1806.0
243.10	1736.0
244.00	21960.0
245.10	3288.0
246.00	6806.0
247.00	728.0
249.00	1008.0

Instrument :
ClientSampleId :
DFTPP10

251.80	337.0
252.10	314.0
253.10	604.0
253.50	952.0
254.10	1992.0
255.00	136064.0
256.00	20856.0
257.00	1722.0
258.00	7561.0
259.00	1601.0
265.00	3539.0
265.90	485.0
271.00	497.0
273.00	4409.0
274.00	11342.0
275.00	50832.0
276.00	8897.0
277.00	7077.0
278.00	988.0
283.00	895.0
284.00	488.0
285.10	819.0
285.90	419.0
291.70	313.0
293.00	1026.0
294.10	543.0
296.00	19440.0
297.20	1906.0
303.10	1865.0
304.10	708.0
314.00	920.0
315.10	1732.0
315.90	730.0
321.10	562.0
322.00	345.0
323.10	5033.0
323.90	676.0
326.90	894.0
327.90	563.0
331.90	374.0
333.90	3041.0
335.00	1068.0
341.00	774.0
346.00	1683.0
347.00	531.0
352.10	1278.0
353.00	1323.0
353.90	1644.0
355.10	304.0
364.90	8801.0
366.00	855.0
371.00	322.0
372.00	2749.0
373.00	719.0
382.80	680.0
390.00	724.0
401.00	398.0
401.90	1082.0
403.00	2078.0
404.00	691.0
420.80	1053.0
422.00	1437.0
423.00	9430.0
424.00	2454.0
425.10	524.0
441.00	25744.0
442.00	150656.0
443.00	32136.0
444.00	2832.0

Instrument :
ClientSampleId :
DFTPP10

m/z	Abundance
37.00	331.0
38.10	1827.0
39.00	9472.0
40.00	4699.0
41.00	577.0
44.00	7141.0
44.90	340.0
49.10	1258.0
50.00	38520.0
51.00	156352.0
52.10	7705.0
55.00	855.0
56.00	5730.0
57.00	10575.0
61.00	1766.0
62.00	2346.0
63.00	5284.0
63.90	782.0
65.00	3339.0
66.10	694.0
68.00	2698.0
69.00	145536.0
70.00	641.0
73.00	1789.0
74.00	15535.0
75.00	25272.0
76.00	6928.0
77.10	156864.0
78.00	9767.0
79.00	12523.0
80.00	9449.0
81.00	11324.0
82.10	3081.0
83.10	2720.0
85.00	1999.0
86.00	3631.0
87.10	2351.0
88.00	835.0
91.00	3172.0
92.10	3152.0
93.00	22952.0
93.90	1240.0
95.00	421.0
96.10	672.0
96.70	305.0
97.20	314.0
98.00	15691.0
98.90	13397.0
100.00	915.0
101.00	5751.0
102.00	568.0
102.90	2365.0
104.00	4247.0
105.00	4755.0
106.10	1143.0
107.00	59776.0
108.00	8541.0
108.80	1341.0
110.00	83872.0
111.00	13542.0
112.00	1298.0
112.90	427.0
116.00	3496.0
117.00	46048.0
118.00	4223.0
118.90	603.0
119.80	354.0
122.00	4149.0
123.00	6472.0
124.00	2787.0
125.00	1807.0
126.10	820.0
127.00	158656.0
128.00	12493.0
129.00	68000.0
130.00	6466.0
131.00	1192.0
131.90	398.0
132.90	470.0
133.90	1999.0
135.00	5719.0
136.00	2776.0
137.00	3173.0
137.80	459.0
139.20	450.0
140.10	798.0
141.00	9650.0
142.00	2272.0
143.10	2442.0
143.80	484.0
144.80	538.0

Instrument :
ClientSampleId :
DFTPP10

145.90	1721.0
147.10	4857.0
148.00	12368.0
149.10	2683.0
150.10	786.0
151.00	1415.0
152.00	336.0
153.00	2995.0
153.90	1745.0
155.10	5389.0
156.10	8292.0
156.90	1175.0
158.10	1515.0
159.00	1403.0
159.90	3038.0
161.00	3181.0
162.00	1489.0
163.00	459.0
164.10	560.0
164.90	3614.0
166.00	2805.0
167.00	18560.0
168.00	8755.0
168.90	1986.0
169.80	555.0
171.00	923.0
172.00	1666.0
173.00	1974.0
174.00	3758.0
175.00	7010.0
175.90	1982.0
176.90	3260.0
178.10	1235.0
179.00	15142.0
180.00	9640.0
181.00	4287.0
181.90	531.0
182.10	537.0
182.80	400.0
184.00	1536.0
185.00	7895.0
186.00	49848.0
187.00	15852.0
188.00	2242.0
189.00	3605.0
189.90	504.0
191.20	1586.0
192.00	4219.0
193.10	6175.0
194.00	1218.0
195.00	850.0
196.00	7130.0
197.00	2990.0
198.00	322048.0
199.00	21056.0
200.10	2561.0
201.50	1311.0
203.00	2807.0
204.00	13329.0
205.00	22776.0
206.10	94240.0
207.00	12467.0
208.00	4466.0
209.00	943.0
210.00	1211.0
211.00	3648.0
212.10	508.0
212.70	376.0
213.20	626.0
215.00	908.0
216.00	1655.0
217.00	28192.0
218.10	2981.0
219.10	413.0
220.10	570.0
221.00	9806.0
221.90	2922.0
223.00	5441.0
224.00	50160.0
225.10	11832.0
226.00	2052.0
227.00	25760.0
227.90	3281.0
229.00	5130.0
230.10	628.0
231.00	2257.0
232.90	611.0
233.90	1647.0
235.00	1732.0
235.90	1040.0
237.10	1681.0
237.80	373.0
238.90	937.0
240.00	1035.0
241.00	989.0

Instrument :
ClientSampleId :
DFTPP10

241.90	2717.0
243.00	2898.0
244.10	36592.0
245.10	5204.0
246.10	7958.0
247.10	1183.0
247.90	409.0
249.10	1105.0
249.80	399.0
251.80	329.0
253.10	1044.0
254.10	1774.0
255.00	197888.0
256.00	29856.0
257.10	2044.0
258.00	13287.0
259.00	2466.0
265.00	5614.0
265.90	520.0
269.90	315.0
270.90	501.0
271.70	507.0
272.10	743.0
273.00	6146.0
274.00	15086.0
275.00	79296.0
276.00	11570.0
276.90	7714.0
278.10	1344.0
283.00	1692.0
284.00	859.0
285.10	1002.0
285.90	545.0
289.00	458.0
292.10	419.0
292.90	2579.0
293.90	760.0
295.00	668.0
296.00	29096.0
297.00	3556.0
300.80	314.0
302.10	447.0
303.10	3572.0
303.90	815.0
310.10	315.0
313.90	1248.0
314.90	3415.0
316.00	1756.0
316.90	601.0
320.90	335.0
321.90	731.0
323.10	8241.0
324.10	1805.0
326.90	1300.0
328.00	896.0
332.00	726.0
332.90	630.0
334.00	6045.0
335.00	1520.0
336.20	306.0
340.90	1064.0
341.90	479.0
345.90	1141.0
346.90	353.0
352.00	2380.0
353.00	2382.0
354.00	2097.0
354.80	372.0
364.90	13002.0
366.00	2580.0
371.10	325.0
372.00	3757.0
373.10	834.0
383.00	1360.0
383.80	557.0
390.10	377.0
391.00	673.0
402.00	1381.0
403.00	2659.0
403.90	958.0
415.00	463.0
420.90	1966.0
422.00	2488.0
423.00	15200.0
424.00	3312.0
425.00	584.0
441.00	39792.0
442.00	282496.0
443.00	50440.0
443.90	4257.0

Instrument :
ClientSampleId :
DFTPP10

m/z	Abundance
37.00	451.0
38.10	1192.0
39.10	7036.0
40.00	5231.0
41.10	509.0
43.10	486.0
44.00	7195.0
44.90	476.0
49.00	830.0
50.00	28272.0
51.10	107656.0
52.00	5944.0
55.10	749.0
55.90	3030.0
57.00	8327.0
58.10	448.0
61.00	1504.0
61.90	1473.0
63.00	4552.0
64.00	816.0
65.00	1869.0
68.00	1734.0
69.00	100344.0
73.10	1373.0
74.00	10479.0
75.00	16784.0
76.10	5102.0
77.00	110552.0
78.10	6176.0
79.00	8107.0
80.00	6677.0
81.00	8129.0
82.00	2198.0
83.10	1380.0
85.00	1742.0
86.10	2926.0
87.00	904.0
91.00	2085.0
92.00	2822.0
93.00	16568.0
94.10	1098.0
95.10	426.0
96.00	826.0
98.00	12466.0
99.00	10298.0
100.00	1097.0
101.00	4149.0
102.00	417.0
103.00	1644.0
104.10	2204.0
104.90	2497.0
106.00	903.0
107.00	45448.0
108.00	6540.0
109.00	1210.0
110.00	59936.0
111.00	9784.0
112.00	1484.0
113.10	324.0
116.00	2288.0
117.00	39176.0
118.00	2776.0
118.90	373.0
120.10	413.0
121.90	2617.0
123.10	4469.0
123.90	2114.0
125.00	1750.0
126.10	688.0
127.00	117808.0
128.10	9170.0
129.00	51144.0
129.90	4099.0
131.10	913.0
132.00	306.0
133.90	1276.0
135.00	4728.0
135.90	2305.0
136.90	2334.0
137.80	375.0
139.80	457.0
141.00	7022.0
142.00	2281.0
143.10	1203.0
144.00	576.0
145.00	316.0
146.00	1748.0
147.00	3482.0
148.00	7936.0
148.90	1713.0
149.90	616.0

Instrument :
ClientSampleId :
DFTPP10

151.20	907.0
152.00	391.0
152.90	2770.0
153.90	1831.0
155.00	3596.0
156.00	6367.0
157.00	1008.0
157.90	1358.0
159.10	1260.0
160.00	2006.0
161.00	3002.0
162.10	722.0
164.00	319.0
165.10	2991.0
166.20	2003.0
167.00	14765.0
168.00	7166.0
169.00	1040.0
170.10	784.0
171.00	676.0
171.90	1746.0
173.00	1810.0
174.00	2469.0
175.00	5735.0
176.00	1585.0
177.10	2428.0
178.00	1356.0
179.00	13185.0
180.10	6492.0
181.00	2942.0
182.10	871.0
183.10	415.0
184.10	964.0
185.00	6546.0
186.00	39336.0
187.00	10351.0
188.00	1047.0
189.00	2587.0
190.20	482.0
191.20	1154.0
192.00	4015.0
193.00	3101.0
194.00	1183.0
194.90	671.0
196.00	6473.0
197.00	1794.0
198.00	264768.0
198.90	17424.0
200.00	1636.0
201.00	326.0
201.70	954.0
203.00	2082.0
204.00	11255.0
205.10	19408.0
206.10	74912.0
207.00	11440.0
208.10	3462.0
209.00	1170.0
209.80	1391.0
211.00	3103.0
212.00	433.0
215.00	942.0
216.00	1362.0
217.00	22952.0
218.00	2602.0
219.10	474.0
220.10	366.0
221.00	6860.0
221.90	2147.0
223.00	3856.0
224.10	41224.0
225.00	10555.0
226.10	1343.0
227.00	20192.0
228.00	2583.0
229.00	4486.0
230.00	487.0
230.90	1073.0
232.10	325.0
233.90	1076.0
234.90	1147.0
236.00	1102.0
237.00	2284.0
239.00	1308.0
240.00	658.0
240.80	1619.0
241.90	1950.0
243.00	2284.0
244.10	31408.0
245.00	3232.0
246.00	7653.0
247.10	1424.0
248.10	334.0
249.00	1204.0
251.10	463.0

Instrument :
ClientSampleId :
DFTPP10

253.10	839.0
254.10	1934.0
255.00	175168.0
256.00	23488.0
256.90	2152.0
258.00	11206.0
259.00	1550.0
260.00	654.0
260.90	326.0
264.00	432.0
265.10	4436.0
266.00	789.0
270.00	469.0
271.10	606.0
271.90	711.0
273.00	4640.0
274.00	12924.0
275.00	71608.0
276.00	9943.0
277.00	7435.0
277.90	1362.0
282.90	1185.0
284.10	582.0
285.00	1483.0
285.90	327.0
288.90	709.0
291.80	512.0
292.90	1409.0
294.00	697.0
295.00	876.0
296.00	23584.0
297.10	3295.0
301.90	685.0
303.10	2324.0
304.00	483.0
308.00	515.0
314.10	791.0
315.00	3154.0
316.10	1201.0
316.90	377.0
321.10	805.0
323.10	7186.0
323.90	1716.0
325.90	367.0
327.00	1722.0
328.00	698.0
332.10	425.0
332.90	918.0
334.00	5704.0
335.00	1362.0
336.10	302.0
341.00	765.0
342.10	671.0
346.00	1712.0
352.10	2155.0
353.10	1591.0
354.00	2673.0
354.90	311.0
365.00	12968.0
366.00	1974.0
371.10	365.0
372.00	3474.0
373.00	1209.0
382.90	1079.0
384.00	397.0
390.10	581.0
391.00	336.0
400.90	481.0
402.00	1562.0
403.00	2366.0
404.10	1208.0
421.00	1324.0
421.90	1900.0
423.00	14153.0
424.10	2936.0
424.80	412.0
441.00	42760.0
442.00	289408.0
443.10	55488.0
443.90	4303.0

Instrument :
ClientSampleId :
DFTPP10

Scan 2535 (17.598 min): BM000259.D
DFTPP10

m/z	Abundance
40.00	5086.0
44.00	6900.0
73.10	542.0
76.90	301.0
206.90	1070.0
208.00	326.0

Instrument :
ClientSampleId :
DFTPP10