

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM012020\
 Data File : BM024550.D
 Acq On : 20 Jan 2020 18:09
 Operator : JU
 Sample : L1169-16
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Jan 21 01:02:55 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM011520MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jan 20 15:42:34 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.46	152	182659	20.00	ng/ul	0.00
18) Naphthalene-d8	10.21	136	782233	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.10	164	564502	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.85	188	1330710	20.00	ng/ul	0.00
78) Chrysene-d12	21.06	240	1394226	20.00	ng/ul	0.00
86) Perylene-d12	23.18	264	1434953	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.06	96	17821	4.77	ng/uL	0.00
5) Phenol-d5	6.65	99	82903	6.12	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.80	67	211596	28.14	ng/ul	0.00
9) 2-Chlorophenol-d4	6.99	132	277235	23.98	ng/ul	0.00
13) 4-Methylphenol-d8	8.16	113	175323	14.04	ng/ul	0.00
19) Nitrobenzene-d5	8.59	128	179829	32.72	ng/ul	0.00
22) 2-Nitrophenol-d4	9.31	143	204862	34.42	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.85	165	364928	27.24	ng/ul	0.00
29) 4-Chloroaniline-d4	10.36	131	28945	1.94	ng/ul	0.00
44) Dimethylphthalate-d6	13.53	166	1420293	32.11	ng/ul	0.00
47) Acenaphthylene-d8	13.79	160	1619139	31.81	ng/ul	0.00
52) 4-Nitrophenol-d4	14.32	143	40244	5.45	ng/ul	0.00
58) Fluorene-d10	15.10	176	1259285	32.34	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.23	200	233860	30.79	ng/ul	0.00
71) Anthracene-d10	16.95	188	2188960	35.37	ng/ul	0.00
79) Pyrene-d10	19.26	212	2642293	35.46	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.05	264	2610035	35.07	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.57	163	52702	1.172	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM012020\
Data File : BM024550.D
Acq On : 20 Jan 2020 18:09
Operator : JU
Sample : L1169-16
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Jan 21 01:02:55 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM011520MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jan 20 15:42:34 2020
Response via : Initial Calibration

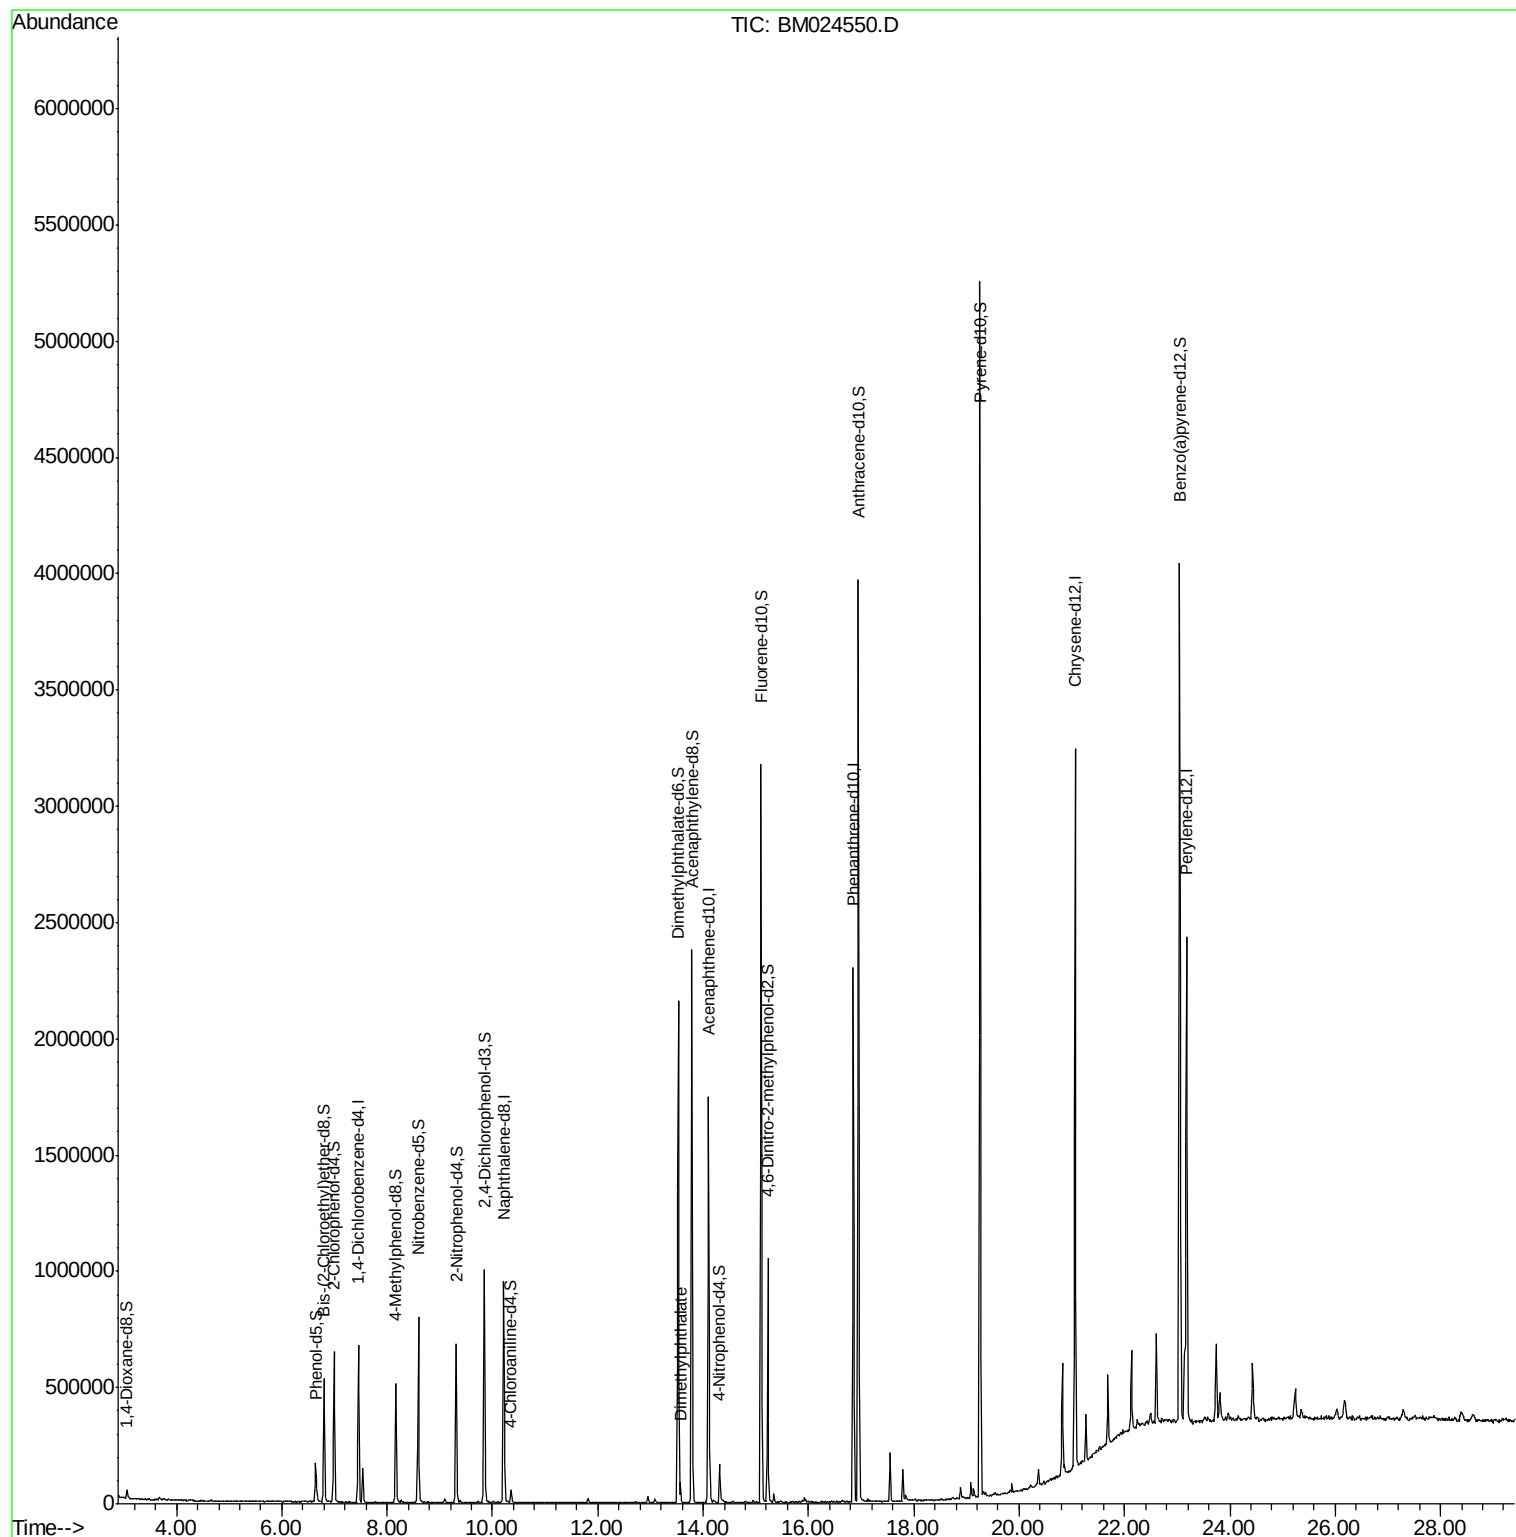

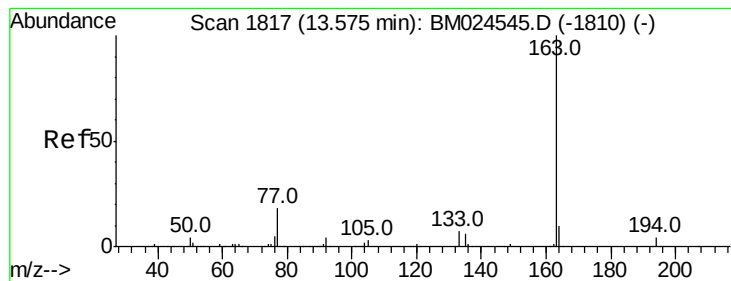

#45

Dimethylphthalate

Concen: 1.172 ng/ul

RT: 13.57 min Scan# 1816

Delta R.T. -0.01 min

Lab File: BM024550.D

Acq: 20 Jan 2020 18:09

Instrument :

BNA_M

ClientSampleId :



Tot Ion:163 Resp: 52702

Ion Ratio Lower Upper

163 100

194 5.0 3.4 5.0

164 10.3 8.0 12.0

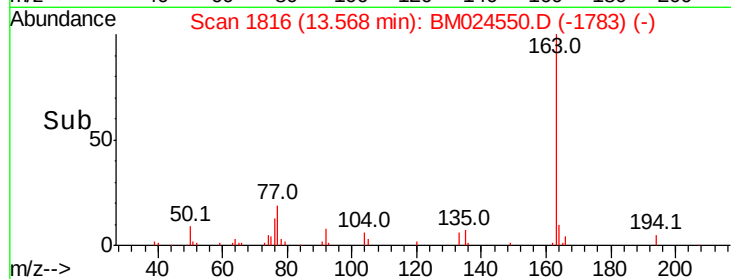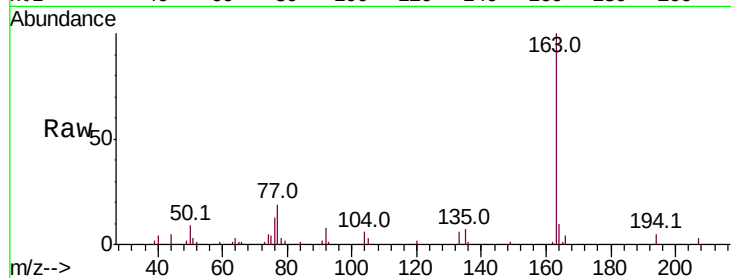

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

