

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM012020\
 Data File : BM024554.D
 Acq On : 20 Jan 2020 20:32
 Operator : JU
 Sample : L1195-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Jan 21 01:03:15 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM011520MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jan 20 15:42:34 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.46	152	174464	20.00	ng/ul	0.00
18) Naphthalene-d8	10.21	136	744670	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.10	164	542132	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.85	188	1283276	20.00	ng/ul	0.00
78) Chrysene-d12	21.06	240	1306111	20.00	ng/ul	0.00
86) Perylene-d12	23.18	264	1321323	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.06	96	4787	1.34	ng/uL	0.00
5) Phenol-d5	6.65	99	79434	6.14	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.80	67	211677	29.47	ng/ul	0.00
9) 2-Chlorophenol-d4	6.99	132	277003	25.08	ng/ul	0.00
13) 4-Methylphenol-d8	8.16	113	166113	13.93	ng/ul	0.00
19) Nitrobenzene-d5	8.59	128	186216	35.59	ng/ul	0.00
22) 2-Nitrophenol-d4	9.30	143	211842	37.38	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.85	165	371667	29.14	ng/ul	0.00
29) 4-Chloroaniline-d4	10.35	131	23418	1.65	ng/ul	0.00
44) Dimethylphthalate-d6	13.53	166	1476768	34.76	ng/ul	0.00
47) Acenaphthylene-d8	13.79	160	1683778	34.44	ng/ul	0.00
52) 4-Nitrophenol-d4	14.32	143	43636	6.16	ng/ul	0.00
58) Fluorene-d10	15.10	176	1332180	35.63	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.23	200	255104	34.82	ng/ul	0.00
71) Anthracene-d10	16.95	188	2407769	40.35	ng/ul	0.00
79) Pyrene-d10	19.26	212	2870258	41.11	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.04	264	2780774	40.57	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.57	163	59524	1.378	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM012020\
Data File : BM024554.D
Acq On : 20 Jan 2020 20:32
Operator : JU
Sample : L1195-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Jan 21 01:03:15 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM011520MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jan 20 15:42:34 2020
Response via : Initial Calibration

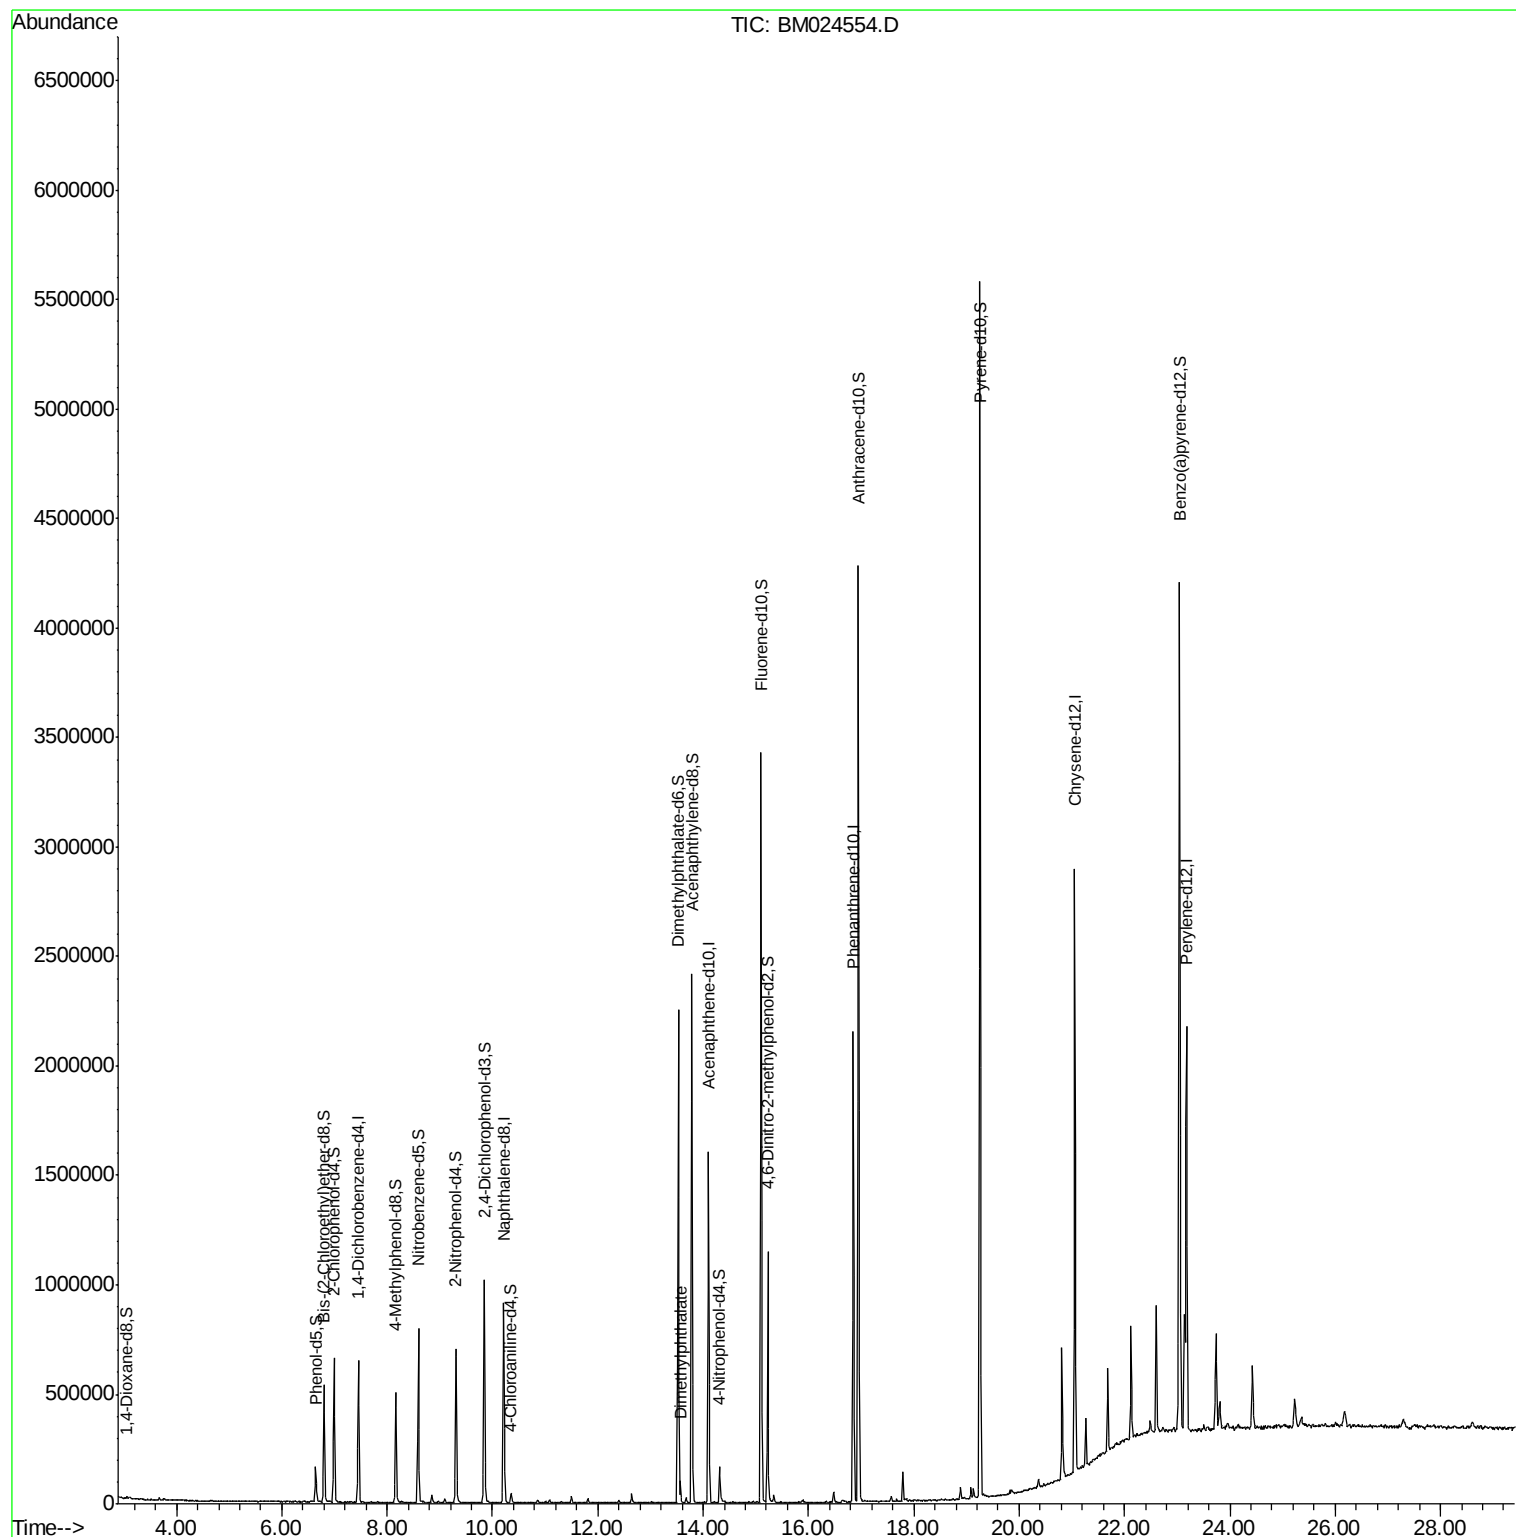

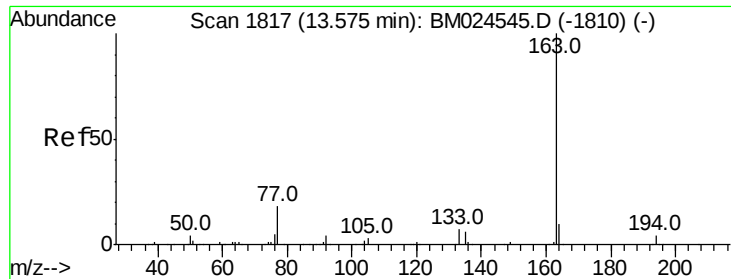

#45

Dimethylphthalate

Concen: 1.378 ng/ul

RT: 13.57 min Scan# 1816

Delta R.T. -0.01 min

Lab File: BM024554.D

Acq: 20 Jan 2020 20:32

Instrument :

BNA_M

ClientSampleId :

Tot Ion:163 Resp: 59524

Ion Ratio Lower Upper

163 100

194 4.0 3.4 5.0

164 10.1 8.0 12.0

