

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM012020\
 Data File : BM024553.D
 Acq On : 20 Jan 2020 19:56
 Operator : JU
 Sample : L1169-19
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BF785

Quant Time: Jan 21 01:03:10 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM011520MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jan 20 15:42:34 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.46	152	156144	20.00	ng/ul	0.00
18) Naphthalene-d8	10.22	136	658961	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.10	164	484754	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.85	188	1156111	20.00	ng/ul	0.00
78) Chrysene-d12	21.06	240	1129720	20.00	ng/ul	0.00
86) Perylene-d12	23.18	264	1106091	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.06	96	18651	5.84	ng/uL	0.00
5) Phenol-d5	6.65	99	93800	8.10	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.80	67	230032	35.78	ng/ul	0.00
9) 2-Chlorophenol-d4	6.99	132	312570	31.62	ng/ul	0.00
13) 4-Methylphenol-d8	8.16	113	197191	18.48	ng/ul	0.00
19) Nitrobenzene-d5	8.59	128	201469	43.52	ng/ul	0.00
22) 2-Nitrophenol-d4	9.30	143	231672	46.20	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.85	165	420297	37.24	ng/ul	0.00
29) 4-Chloroaniline-d4	10.35	131	31569	2.52	ng/ul	0.00
44) Dimethylphthalate-d6	13.53	166	1675694	44.12	ng/ul	0.00
47) Acenaphthylene-d8	13.79	160	1879791	43.00	ng/ul	0.00
52) 4-Nitrophenol-d4	14.31	143	47551	7.50	ng/ul	-0.01
58) Fluorene-d10	15.10	176	1449615	43.36	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.23	200	260067	39.41	ng/ul	0.00
71) Anthracene-d10	16.95	188	2450007	45.57	ng/ul	0.00
79) Pyrene-d10	19.26	212	2927988	48.49	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.04	264	2623640	45.73	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.57	163	50060	1.297	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM012020\
Data File : BM024553.D
Acq On : 20 Jan 2020 19:56
Operator : JU
Sample : L1169-19
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BF785

Quant Time: Jan 21 01:03:10 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM011520MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jan 20 15:42:34 2020
Response via : Initial Calibration

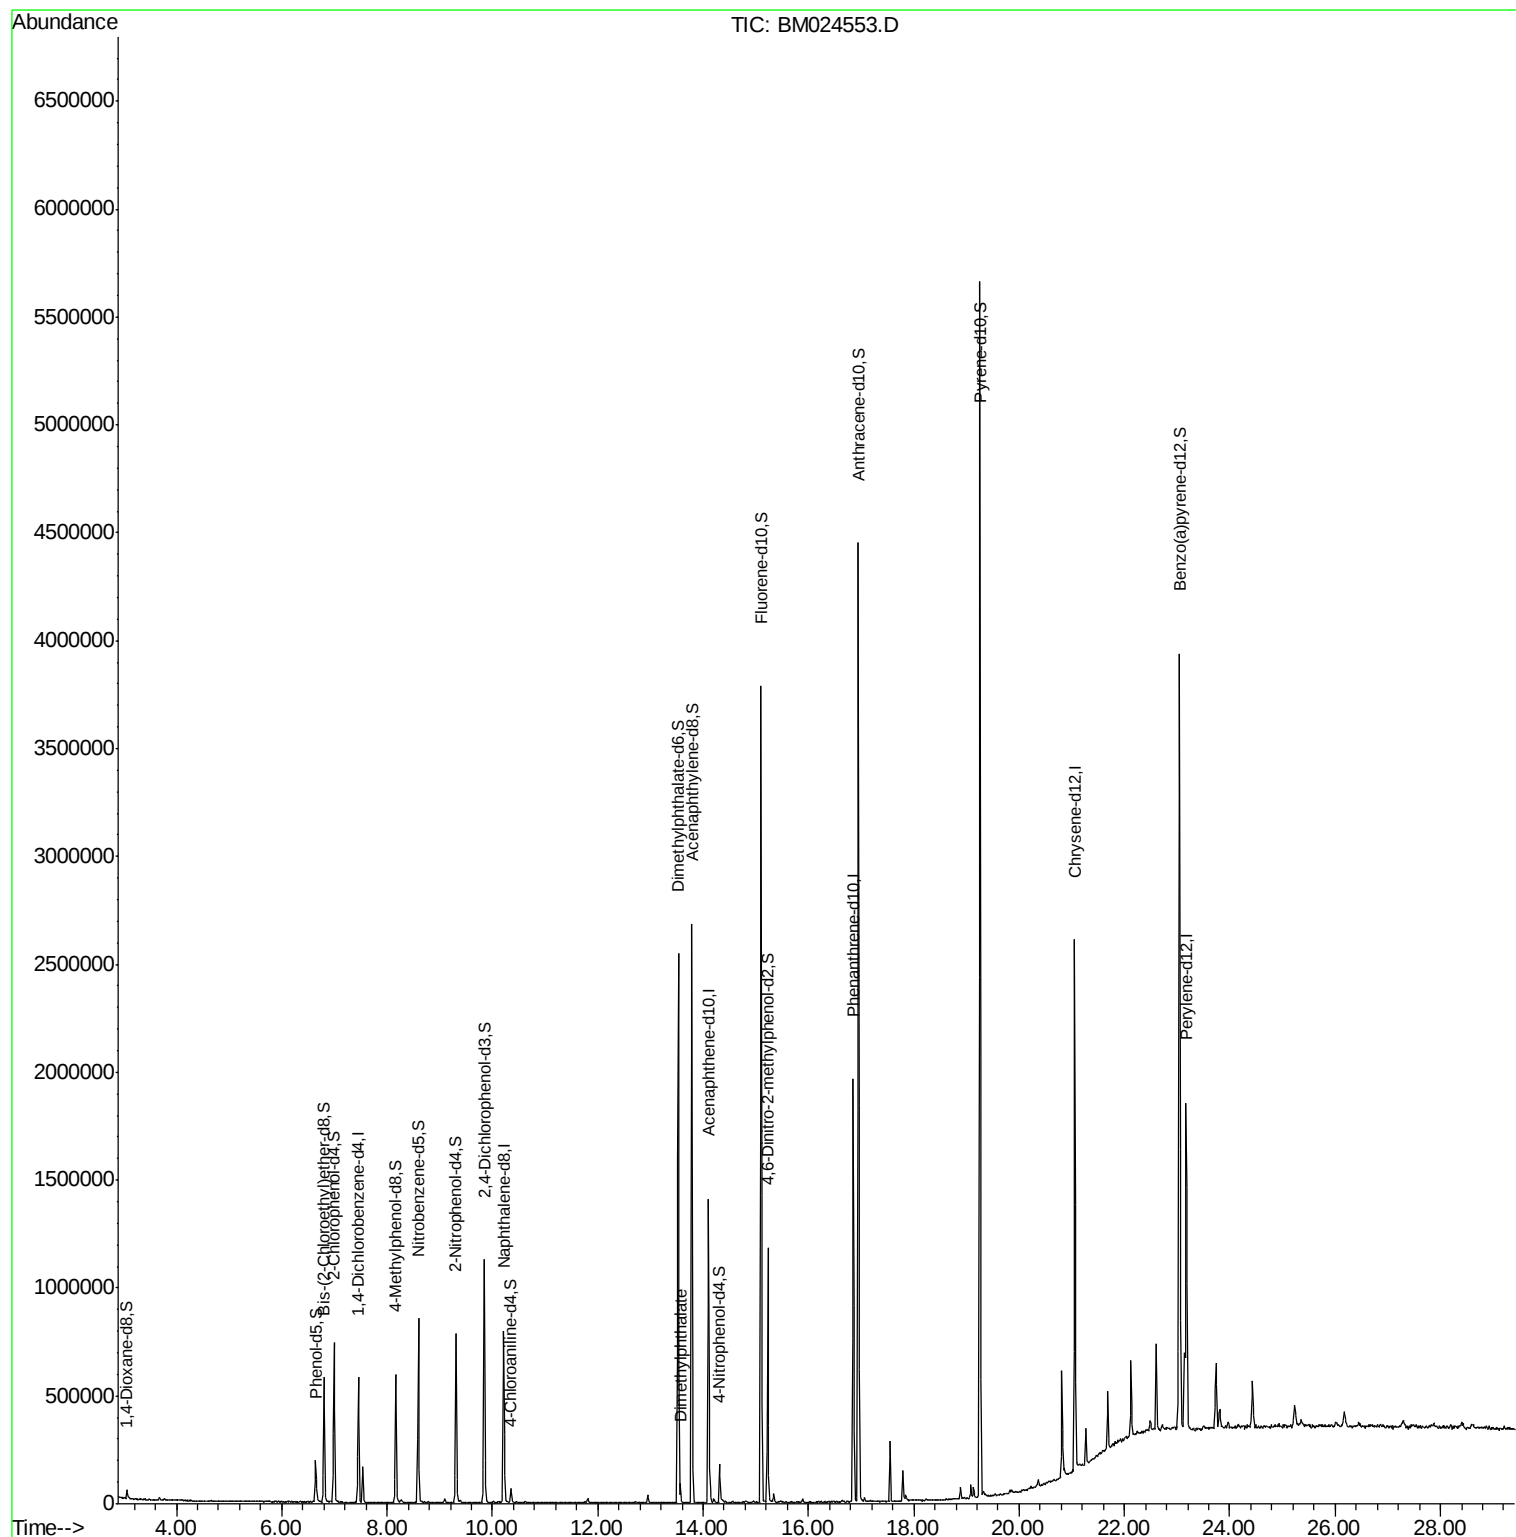

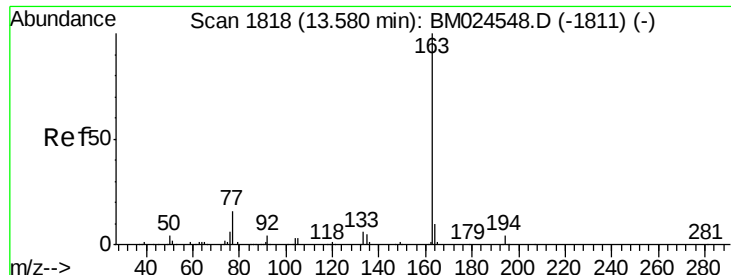

#45

Dimethylphthalate

Concen: 1.297 ng/ul

RT: 13.57 min Scan# 1816

Delta R.T. -0.01 min

Lab File: BM024553.D

Acq: 20 Jan 2020 19:56

Instrument :

BNA_M

ClientSampleId :

BF785

Tot Ion:163 Resp: 50060

Ion Ratio Lower Upper

163 100

194 4.4 3.4 5.0

164 9.3 8.0 12.0

