


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012021\
 Data File : BM028459.D
 Acq On : 20 Jan 2021 09:18
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jan 20 14:45:01 2021

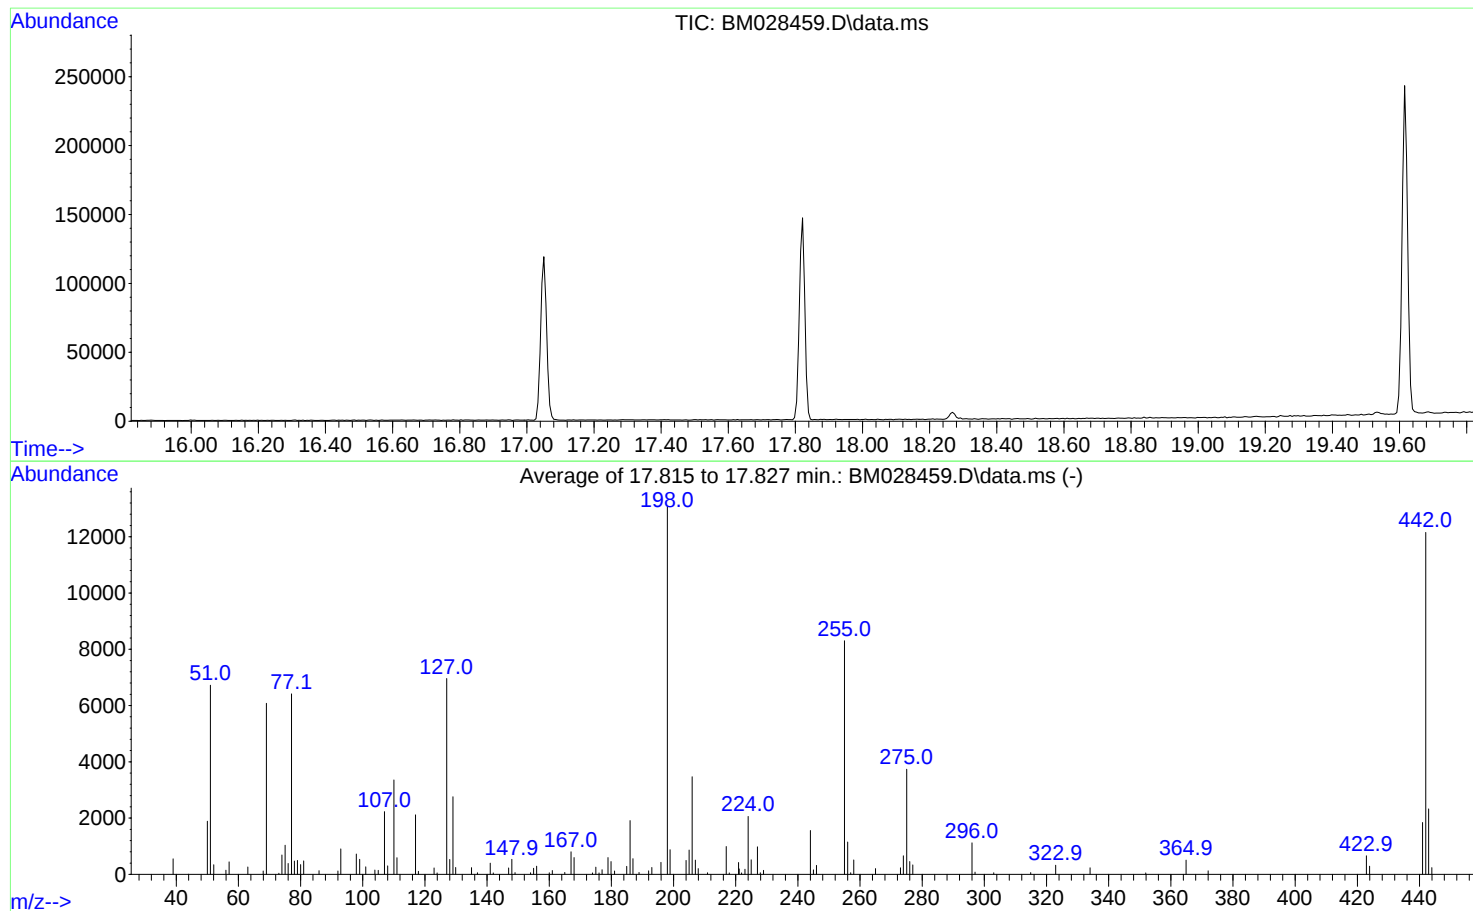

AutoFind: Scans 2487, 2488, 2489; Background Corrected with Scan 2481

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	51.4	6724	PASS
68	69	0.00	2	1.9	117	PASS
69	198	0.00	100	46.5	6081	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.2	6961	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	13074	PASS
199	198	5	9	6.7	874	PASS
275	198	10	60	28.6	3738	PASS
365	198	1	100	3.9	506	PASS
441	198	0.01	100	14.1	1842	PASS
442	198	50	100	93.0	12154	PASS
443	442	15	24	19.1	2325	PASS

Instrument :
BNA_M
ClientSampleId :
DFTPP




DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/20/2021	BNA_M	<u>BM028459.D</u>
Compound Name	Response	Retention Time
DDT	53894	20.833
DDD	0	0
DDE	393	17.821
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
393	54287	0.72

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012021\
Data File : BM028459.D
Acq On : 20 Jan 2021 09:18
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Feb 09 07:57:18 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 29 16:19:07 2021
Response via : Initial Calibration

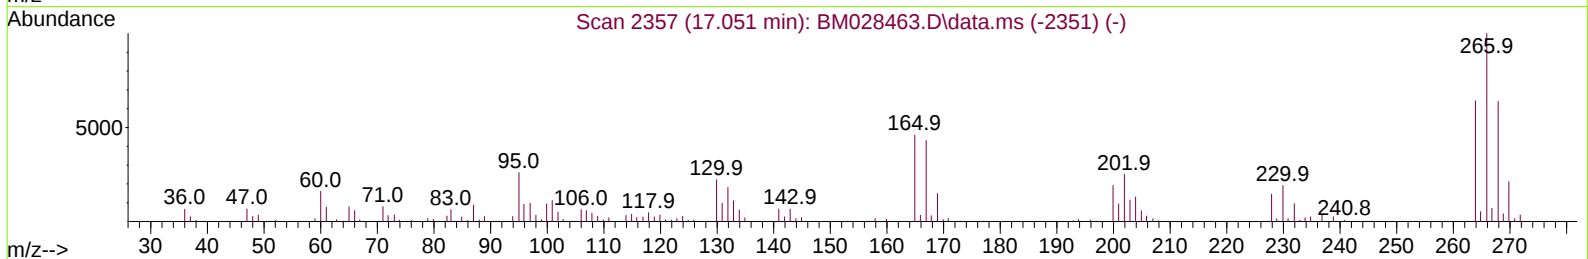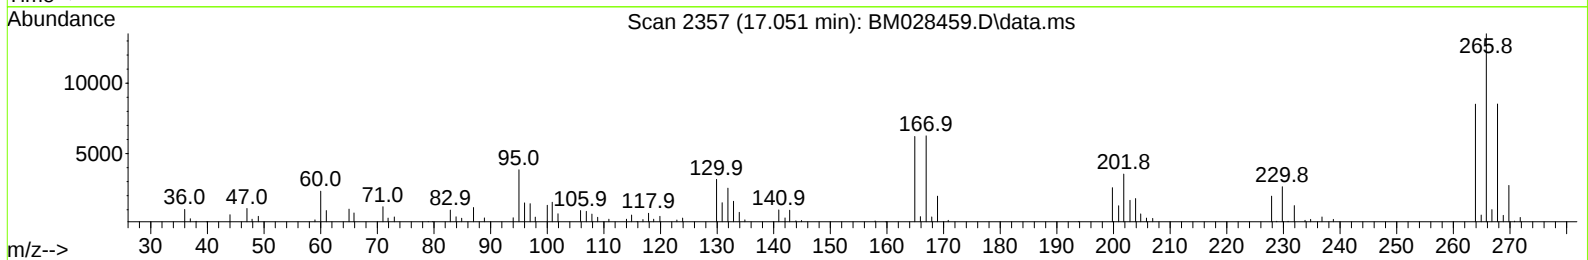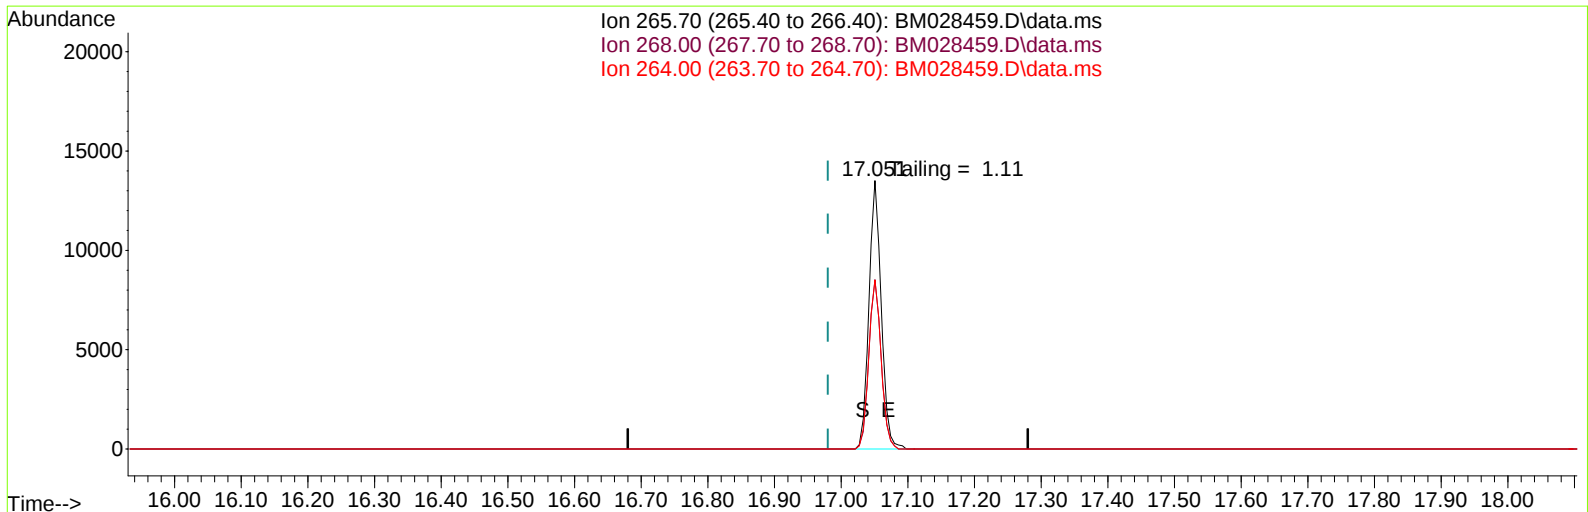

TIC: BM028459.D\data.ms

(70) Pentachlorophenol (C)

17.051min (+ 0.070) 0.00 ng




response 17397

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	63.10
264.00	63.30	62.98
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012021\
Data File : BM028459.D
Acq On : 20 Jan 2021 09:18
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Feb 09 07:57:18 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 29 16:19:07 2021
Response via : Initial Calibration

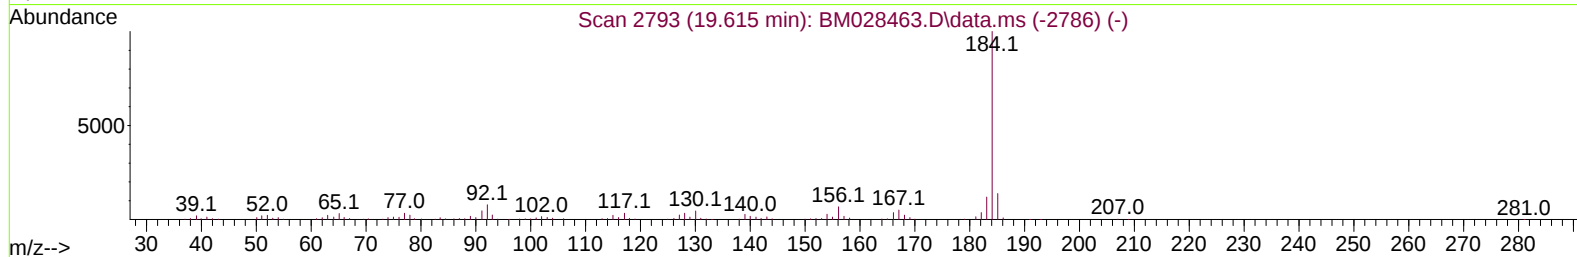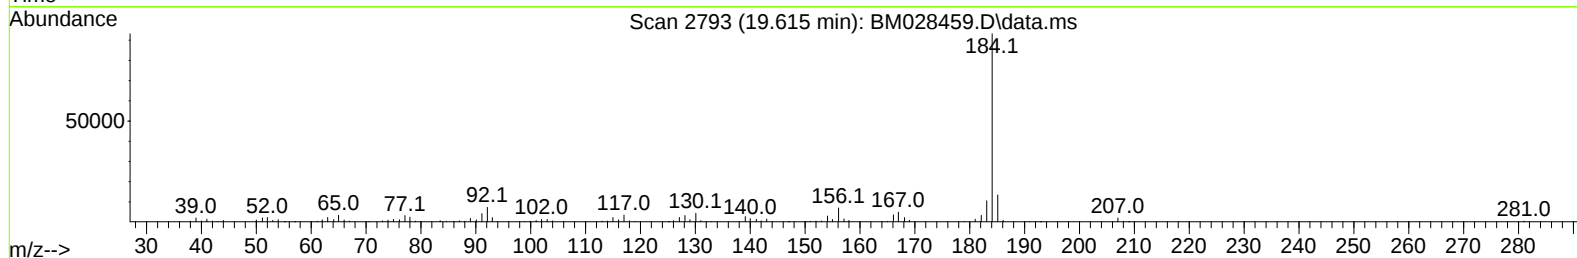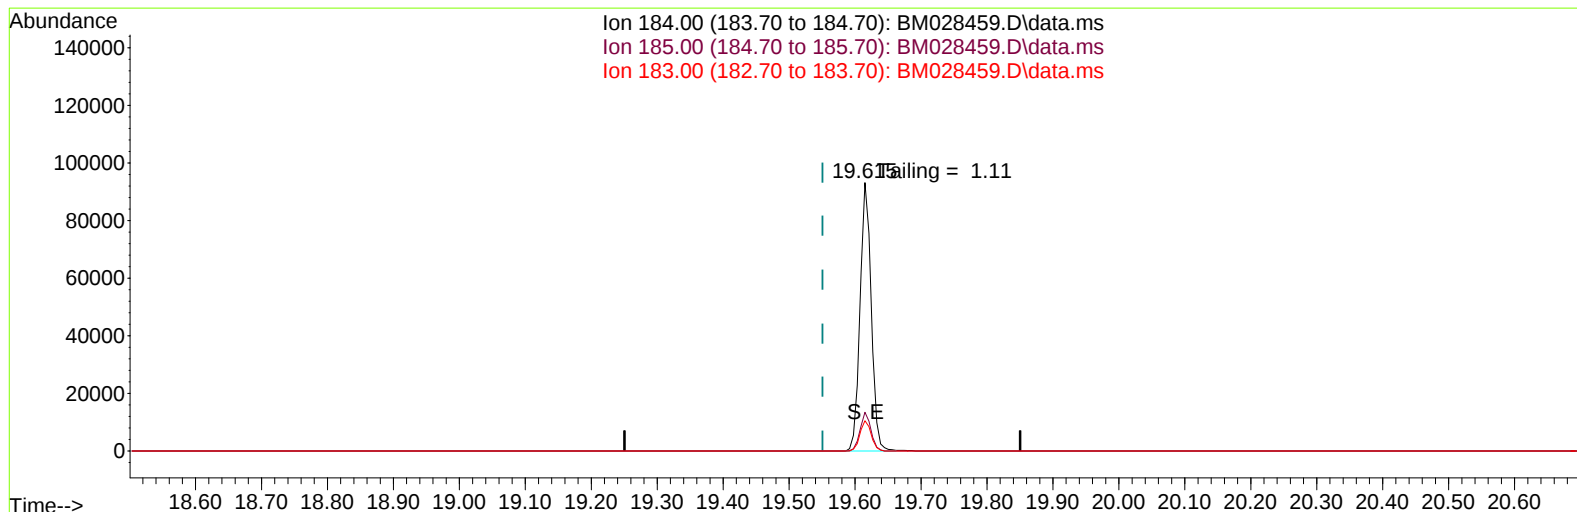

TIC: BM028459.D\data.ms

(77) Benzidine

19.615min (+ 0.064) 0.00 ng

response 109536

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	14.46
183.00	12.10	11.28
0.00	0.00	0.00