


Data Path : Z:\HPCHEM1\BNA_M\Data\BM012116\
Data File : BM004095.D
Acq On : 21 Jan 2016 08:59
Operator : SJ/UM
Sample : DFTPP42
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP42

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM012016.M
Title : SVOA CALIBRATION
Last Update : Thu Jan 21 11:40:38 2016

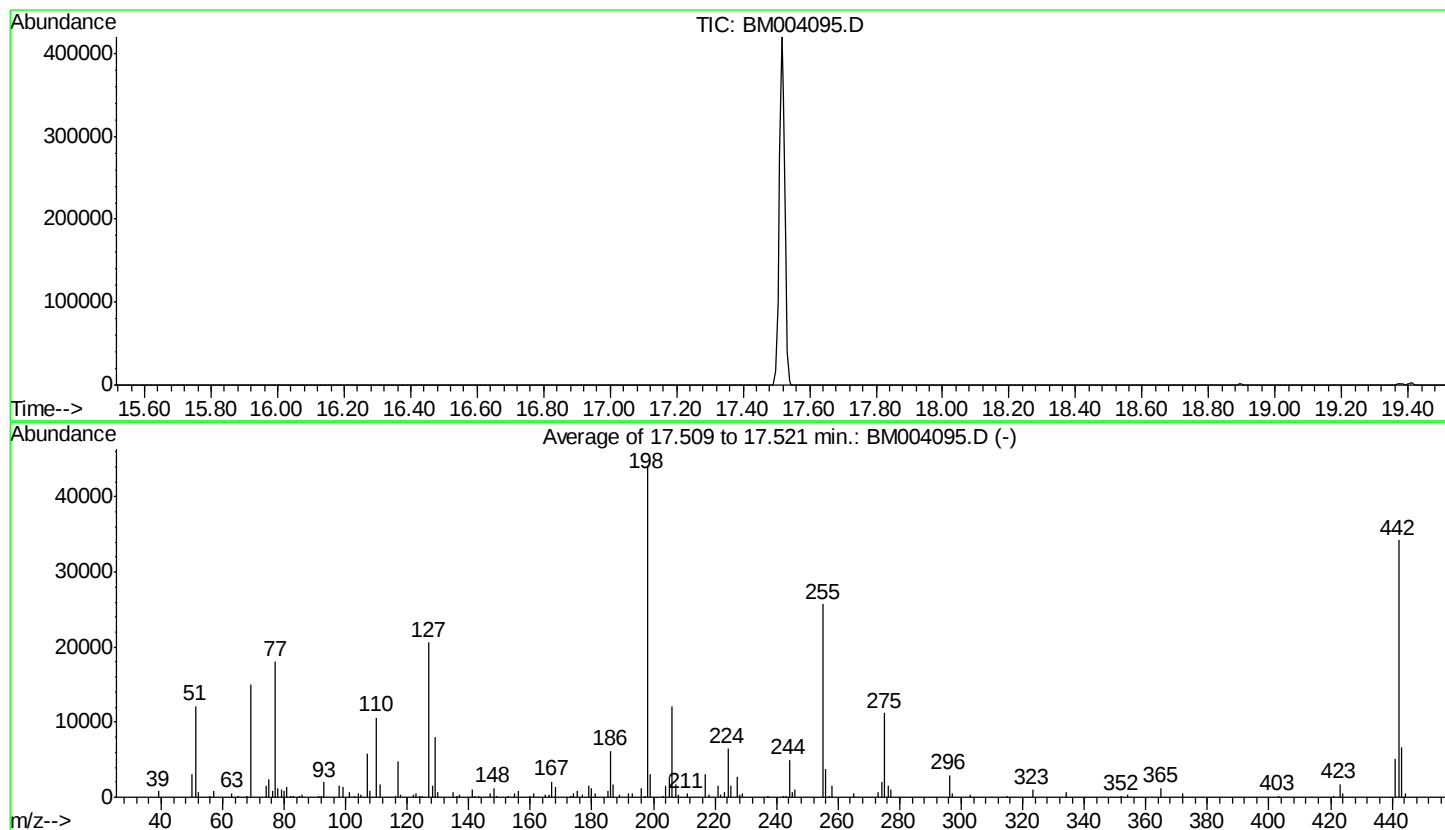

AutoFind: Scans 2452, 2453, 2454; Background Corrected with Scan 2447

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.6	12184	PASS
68	69	0.00	2	0.7	109	PASS
69	198	0.00	100	33.9	14981	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.6	20594	PASS
197	198	0.00	2	0.2	103	PASS
198	198	100	100	100.0	44162	PASS
199	198	5	9	6.9	3030	PASS
275	198	10	60	25.4	11227	PASS
365	198	1	100	2.7	1205	PASS
441	443	0.01	100	77.0	5108	PASS
442	198	50	100	77.6	34264	PASS
443	442	15	24	19.4	6634	PASS

m/z	Abundance
39.00	769.0
50.10	2893.0
51.10	11361.0
52.00	579.0
56.00	332.0
57.00	731.0
63.00	513.0
69.00	13784.0
74.00	1418.0
75.00	2271.0
76.10	796.0
77.10	16112.0
78.10	1176.0
79.00	1023.0
80.00	770.0
81.00	1199.0
86.00	327.0
93.00	1752.0
98.00	1399.0
99.00	1296.0
101.00	714.0
104.00	419.0
105.00	396.0
107.00	5066.0
108.00	793.0
110.00	9210.0
111.00	1516.0
117.00	4192.0
118.00	344.0
122.00	323.0
123.00	480.0
127.00	17792.0
128.00	1329.0
129.00	6771.0
130.00	612.0
135.00	627.0
137.00	322.0
141.00	859.0
147.00	480.0
148.00	992.0
155.00	525.0
156.00	757.0
161.00	441.0
165.00	370.0
167.00	1878.0
168.00	1198.0
174.00	347.0
175.00	685.0
176.90	341.0
179.00	1315.0
180.00	1110.0
181.10	421.0
185.10	671.0
186.00	4935.0
187.00	1514.0
189.00	343.0
192.10	447.0
193.10	530.0
196.00	1065.0
198.00	35856.0
199.00	2546.0
204.10	1184.0
205.10	2108.0
206.10	9504.0
207.10	1549.0
208.00	332.0
211.00	367.0
217.00	2384.0
218.00	309.0
221.10	1381.0
221.90	381.0
223.00	556.0
224.10	5102.0
225.00	1247.0
227.00	2088.0
228.00	328.0
229.00	446.0
244.10	3950.0
245.00	468.0
246.00	767.0
255.10	19680.0
256.10	3068.0
258.00	1108.0
265.00	430.0
273.00	521.0
274.10	1405.0
275.10	8185.0
276.10	1178.0
277.00	730.0
296.00	2140.0
297.00	340.0

Instrument :
BNA_M
ClientSampleId :
DFTPP42

323.10	664.0
334.10	479.0
365.00	855.0
372.10	324.0
423.10	959.0
424.10	467.0
441.10	2848.0
442.10	20488.0
443.20	4037.0
444.10	382.0

Instrument :
BNA_M
ClientSampleId :
DFTPP42

m/z	Abundance
39.10	1000.0
50.10	3714.0
51.10	14464.0
52.00	795.0
56.00	403.0
57.00	1035.0
63.00	691.0
65.00	373.0
68.10	329.0
69.00	17816.0
74.10	1849.0
75.00	2961.0
76.10	1021.0
77.10	21784.0
78.10	1518.0
79.00	1323.0
80.00	1012.0
81.00	1501.0
82.00	333.0
83.00	424.0
85.00	388.0
86.00	452.0
91.00	322.0
92.00	431.0
93.00	2505.0
98.00	1778.0
99.00	1588.0
101.00	877.0
103.00	304.0
104.00	544.0
105.00	469.0
107.00	6987.0
108.00	1033.0
110.00	12659.0
111.00	2133.0
116.00	367.0
117.00	5721.0
118.00	403.0
122.00	476.0
123.00	736.0
124.00	346.0
125.00	308.0
127.10	24520.0
128.00	1842.0
129.00	9676.0
130.00	735.0
135.00	763.0
136.00	337.0
137.10	468.0
141.00	1280.0
142.00	404.0
143.00	315.0
147.00	702.0
148.00	1412.0
149.00	341.0
153.00	408.0
155.00	695.0
156.00	1097.0
160.00	391.0
161.00	585.0
165.00	458.0
166.00	489.0
167.00	2461.0
168.00	1604.0
173.00	317.0
174.00	563.0
175.10	985.0
177.00	486.0
179.00	1853.0
180.00	1478.0
181.00	654.0
185.00	938.0
186.10	7273.0
187.10	2158.0
189.00	428.0
192.00	624.0
193.00	667.0
196.00	1547.0
197.10	310.0
198.00	52352.0
199.00	3621.0
203.00	397.0
204.00	1898.0
205.10	3318.0
206.10	14633.0
207.10	1995.0
208.00	475.0
211.00	571.0
217.00	3599.0
218.00	456.0
221.10	1868.0

Instrument :
BNA_M
ClientSampleId :
DFTPP42

221.80	588.0
223.10	822.0
224.10	7513.0
225.10	1949.0
227.10	3260.0
228.00	463.0
229.00	674.0
237.00	343.0
242.10	410.0
243.00	398.0
244.10	5773.0
245.00	827.0
246.00	1157.0
255.10	30440.0
256.10	4519.0
257.00	387.0
258.00	1679.0
265.00	626.0
273.10	868.0
274.10	2410.0
275.10	13448.0
276.10	1741.0
277.00	1175.0
296.10	3493.0
297.00	523.0
303.10	456.0
315.00	401.0
323.10	1154.0
334.10	687.0
352.10	350.0
354.10	383.0
365.00	1489.0
372.00	560.0
403.00	333.0
423.10	2084.0
424.10	675.0
441.10	6058.0
442.10	39776.0
443.10	7550.0
444.20	719.0

Instrument :
BNA_M
ClientSampleId :
DFTPP42

m/z	Abundance
39.00	705.0
50.10	2618.0
51.10	10727.0
52.00	526.0
57.00	710.0
63.00	477.0
69.00	13345.0
74.00	1341.0
75.00	2166.0
76.00	767.0
77.10	16096.0
78.10	1130.0
79.00	974.0
80.00	764.0
81.00	1154.0
85.00	332.0
86.00	332.0
93.00	1754.0
98.00	1511.0
99.00	1253.0
101.00	661.0
104.00	484.0
105.00	393.0
107.00	5322.0
108.00	826.0
110.00	9899.0
111.00	1448.0
116.00	369.0
117.10	4187.0
118.00	384.0
122.00	395.0
123.00	578.0
127.10	19472.0
128.10	1446.0
129.00	7540.0
130.00	584.0
135.00	665.0
137.00	371.0
141.00	1007.0
142.00	319.0
147.00	537.0
148.00	1234.0
152.90	365.0
155.00	572.0
156.00	919.0
159.90	314.0
161.00	495.0
165.00	325.0
166.00	339.0
167.00	2051.0
168.00	1142.0
174.00	451.0
175.10	833.0
177.00	381.0
179.00	1647.0
180.00	1225.0
181.00	580.0
185.00	814.0
186.10	6232.0
187.10	1687.0
189.00	401.0
192.00	583.0
193.00	605.0
196.10	1149.0
198.00	44280.0
199.00	2925.0
203.00	311.0
204.10	1605.0
205.10	2744.0
206.10	12060.0
207.10	1639.0
208.00	459.0
211.00	475.0
217.00	3072.0
218.00	412.0
221.10	1577.0
223.00	689.0
224.10	6663.0
225.10	1538.0
227.00	2693.0
228.00	429.0
229.00	652.0
242.00	356.0
243.10	369.0
244.10	5173.0
245.10	715.0
246.00	1097.0
255.10	27072.0
256.10	3819.0
257.00	364.0
258.00	1641.0

Instrument :
BNA_M
ClientSampleId :
DFTPP42

265.00	658.0
273.10	850.0
274.10	2111.0
275.10	12049.0
276.10	1613.0
277.00	1085.0
296.10	3244.0
297.00	502.0
303.10	375.0
315.10	321.0
323.10	1062.0
334.10	719.0
352.10	375.0
354.10	408.0
365.10	1271.0
372.10	554.0
403.00	380.0
421.10	319.0
423.10	2115.0
424.10	583.0
441.10	6420.0
442.10	42528.0
443.10	8315.0
444.10	685.0

Instrument :
BNA_M
ClientSampleId :
DFTPP42

m/z Abundance

Instrument :
BNA_M
ClientSampleId :
DFTPP42