

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM012117\
 Data File : BM008773.D
 Acq On : 21 Jan 2017 15:42
 Operator : UM/SJ
 Sample : PB96196BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK96

Quant Time: Jan 23 03:56:21 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM010617.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jan 23 03:51:57 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.96	152	50990	20.00	ng/ul	0.00
18) Naphthalene-d8	10.76	136	210697	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.59	164	166371	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.33	188	366875	20.00	ng/ul	0.00
75) Chrysene-d12	21.49	240	483579	20.00	ng/ul	0.00
83) Perylene-d12	23.85	264	403612	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.40	96	8811	7.98	ng/uL	0.00
5) Phenol-d5	7.10	99	161002	38.43	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.28	67	131540	46.27	ng/ul	0.00
9) 2-Chlorophenol-d4	7.49	132	106700	36.57	ng/ul	0.00
13) 4-Methylphenol-d8	8.65	113	123388	37.98	ng/ul	0.00
19) Nitrobenzene-d5	9.12	128	54409	41.85	ng/ul	0.00
22) 2-Nitrophenol-d4	9.84	143	60597	42.89	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.37	165	119805	36.82	ng/ul	0.00
29) 4-Chloroaniline-d4	10.89	131	80007	22.20	ng/ul	0.00
43) Dimethylphthalate-d6	13.99	166	447074	40.73	ng/ul	0.00
46) Acenaphthylene-d8	14.28	160	492310	38.04	ng/ul	0.00
51) 4-Nitrophenol-d4	14.76	143	61611	34.32	ng/ul	0.00
57) Fluorene-d10	15.57	176	396239	39.15	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.68	200	81239	42.96	ng/ul	0.00
70) Anthracene-d10	17.42	188	676816	42.82	ng/ul	0.00
76) Pyrene-d10	19.71	212	833522	39.12	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.70	264	661429	40.18	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
15) N-Nitroso-di-n-propylamine	8.65	70	6890	2.13	ng/ul#	1
21) Isophorone	9.84	82	16926	2.07	ng/ul#	71


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM012117\
Data File : BM008773.D
Acq On : 21 Jan 2017 15:42
Operator : UM/SJ
Sample : PB96196BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK96

Quant Time: Jan 23 03:56:21 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM010617.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jan 23 03:51:57 2017
Response via : Initial Calibration




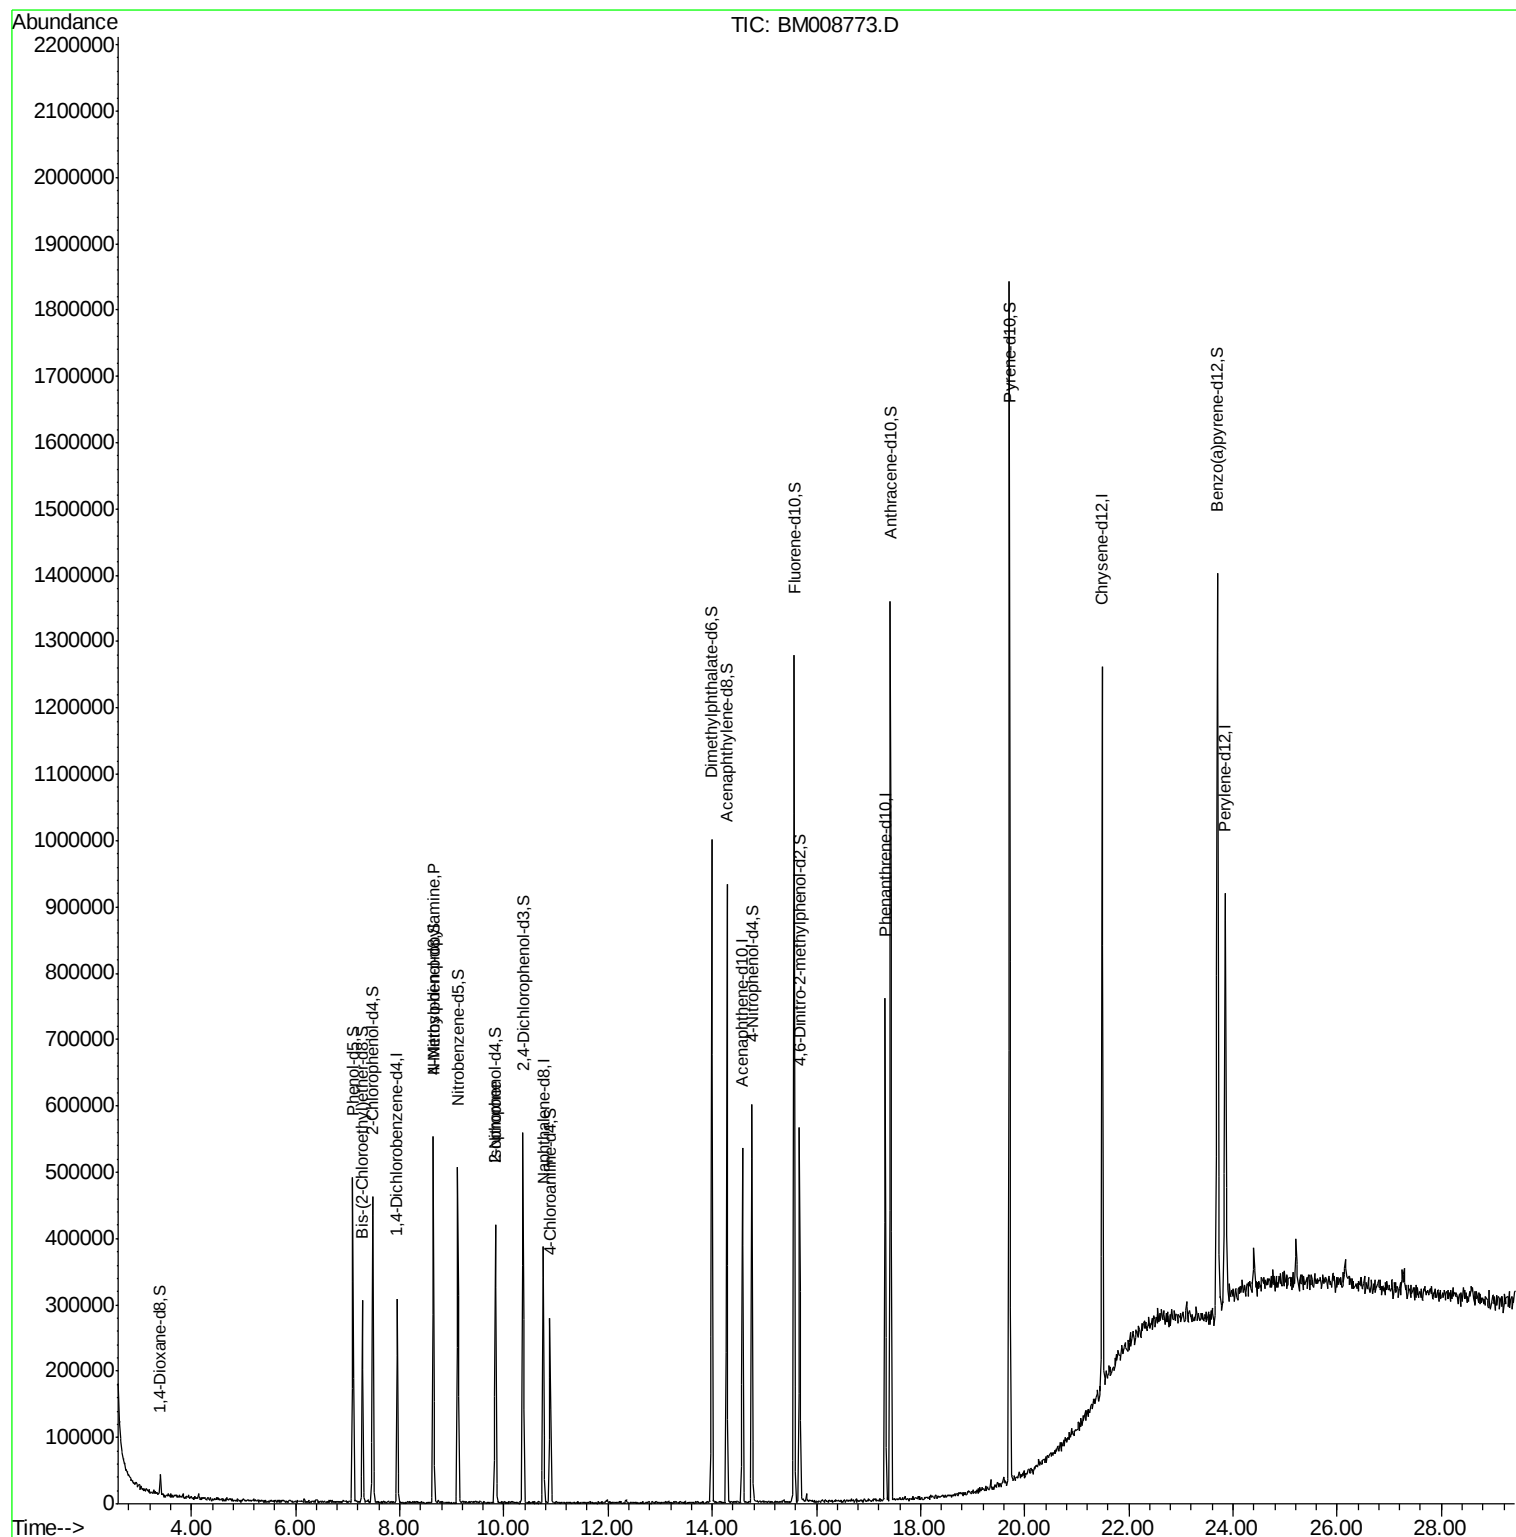


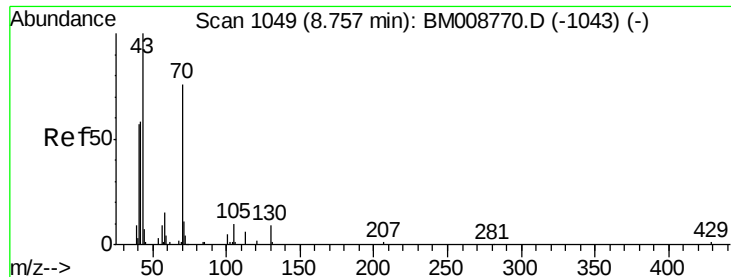

#15
N-Nitroso-di-n-propylamine
Concen: 2.13 ng/ul
RT: 8.65 min Scan# 1030
Delta R.T. -0.11 min
Lab File: BM008773.D
Acq: 21 Jan 2017 15:42

Instrument :
BNA_M
ClientSampleId :
SBLK96

Tgt Ion: 70 Resp: 6890
Ion Ratio Lower Upper
70 100
42 409.3 37.5 56.3#
101 0.0 7.8 11.8#
130 0.0 16.6 25.0#

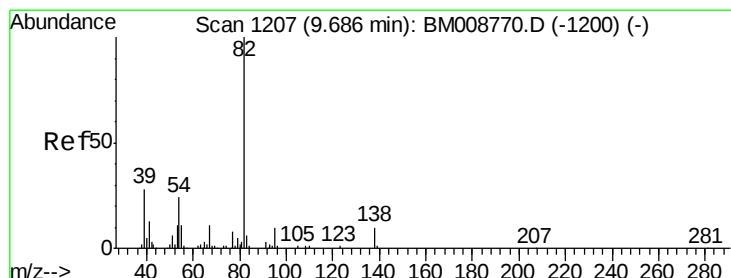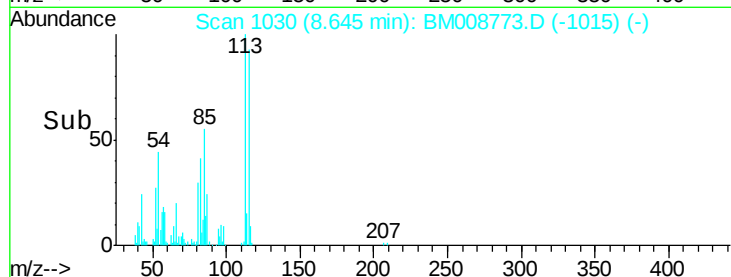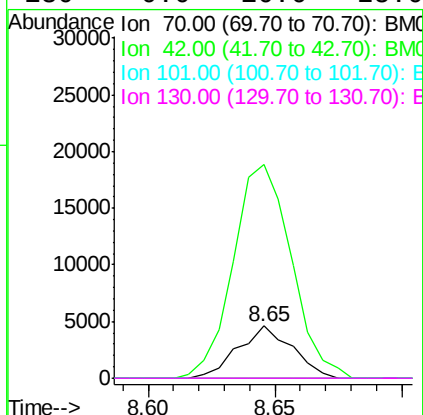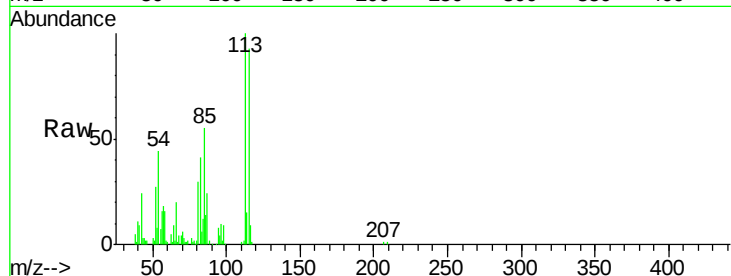

#21
Isophorone
Concen: 2.07 ng/ul
RT: 9.84 min Scan# 1233
Delta R.T. 0.15 min
Lab File: BM008773.D
Acq: 21 Jan 2017 15:42

Tgt Ion: 82 Resp: 16926
Ion Ratio Lower Upper
82 100
95 4.9 6.1 9.1#
138 0.0 13.4 20.2#

