

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM012117\
 Data File : BM008785.D
 Acq On : 21 Jan 2017 23:47
 Operator : UM/SJ
 Sample : I1323-20
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA9R2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM010617.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	7.098	762	767	776	rVB3	87749	138908	6.06%	0.654%
2	7.281	791	798	806	rBV	282909	435747	19.00%	2.051%
3	7.481	824	832	839	rBV	345074	538867	23.49%	2.536%
4	7.951	904	912	920	rBV2	365321	587197	25.60%	2.763%
5	8.645	1024	1030	1043	rVB2	220093	362035	15.78%	1.704%
6	9.116	1102	1110	1117	rBV	456036	760105	33.14%	3.577%
7	9.833	1225	1232	1239	rBV	405047	659307	28.74%	3.103%
8	10.363	1314	1322	1330	rBV	468322	785265	34.23%	3.695%
9	10.751	1381	1388	1395	rBV	408091	715294	31.18%	3.366%
10	13.986	1932	1938	1945	rBV	908247	1222661	53.30%	5.754%
11	14.274	1981	1987	1996	rVB	782986	1161387	50.63%	5.466%
12	14.580	2033	2039	2045	rBV	612826	874693	38.13%	4.116%
13	14.757	2064	2069	2077	rBV	85594	123980	5.40%	0.583%
14	15.574	2202	2208	2217	rVB	1085145	1552509	67.68%	7.306%
15	15.680	2221	2226	2235	rVV2	549456	741811	32.34%	3.491%
16	15.815	2243	2249	2254	rVB6	14308	24055	1.05%	0.113%
17	17.321	2500	2505	2511	rVB	762989	1122300	48.93%	5.282%
18	17.421	2514	2522	2529	rBV2	1340356	1873460	81.67%	8.817%
19	18.192	2649	2653	2657	rBV3	38114	43879	1.91%	0.206%
20	19.339	2844	2848	2852	rBV4	18822	25576	1.11%	0.120%
21	19.468	2866	2870	2875	rBV5	51002	57351	2.50%	0.270%
22	19.709	2905	2911	2916	rBV	1667585	2226563	97.07%	10.478%
23	21.486	3208	3213	3221	rBV	1160709	1503385	65.54%	7.075%
24	23.703	3583	3590	3597	rBV2	1179963	2293866	100.00%	10.795%
25	23.850	3609	3615	3623	rVB	732522	1419141	61.87%	6.679%


Sum of corrected areas: 21249342

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM012117\
Data File : BM008785.D
Acq On : 21 Jan 2017 23:47
Operator : UM/SJ
Sample : I1323-20
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA9R2

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM010617.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

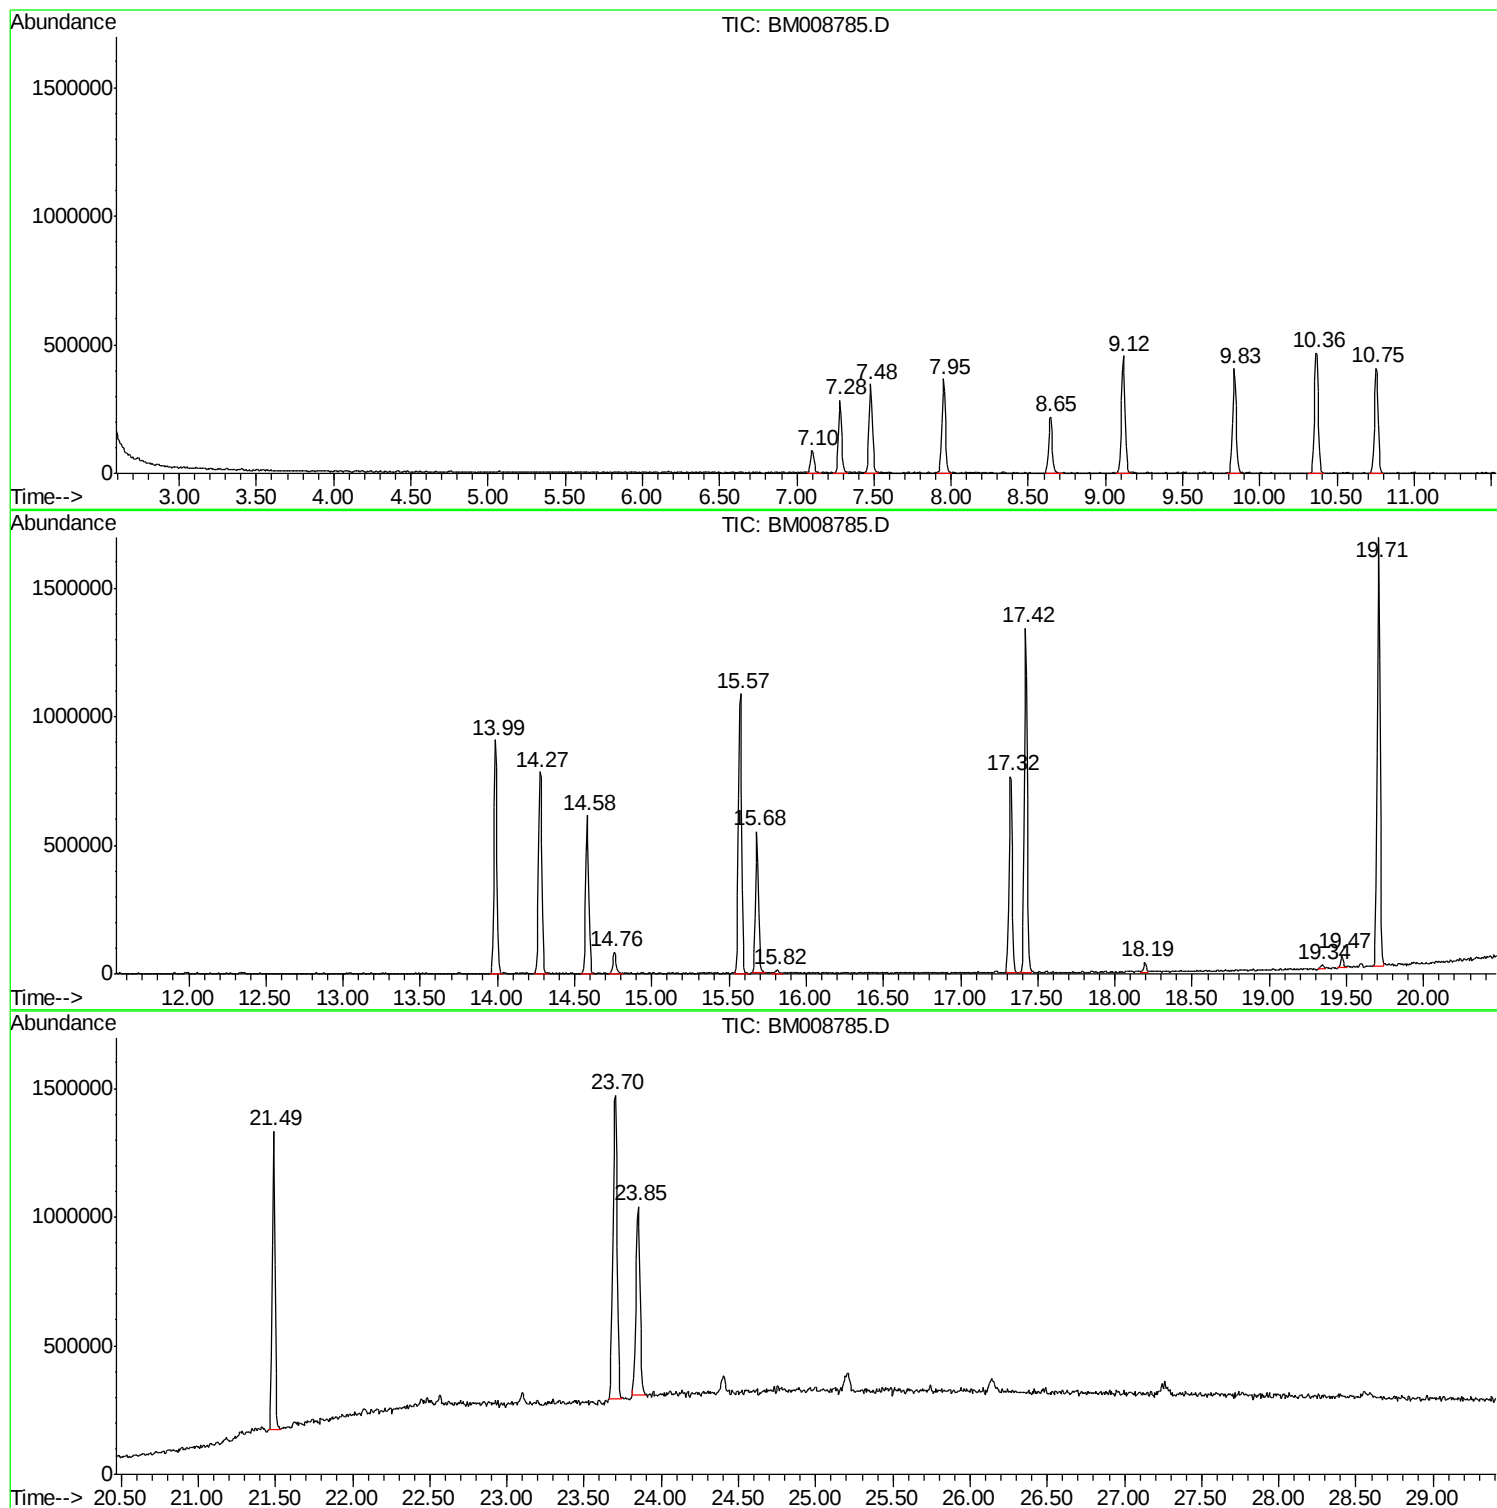

DbaaaPath::ZZ\NRPBMM1BBAAMMDAAAB0002217X\
 DbaaaFile::B0000885DD
 AcqQOn :221Jan2007 233447
 Operator::UMMSJ
 Sample::II333200
 Misc:::
 ASSVaal::166 SampleMultiplier:11

Instrument :
 BNA_M
 ClientSampleId :
 DA9R2

QqaabMebbdd::ZZ\NRPBMM1BBAAMMMEH00SS0000222EPAB0000067MM
 QqaabTitle::SU0AC6AIBRATION

TICLibrary::CC\DATA\BBS6EN0\$T11LL
 TICIntegratioonParameters:LS6CNTTP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
