
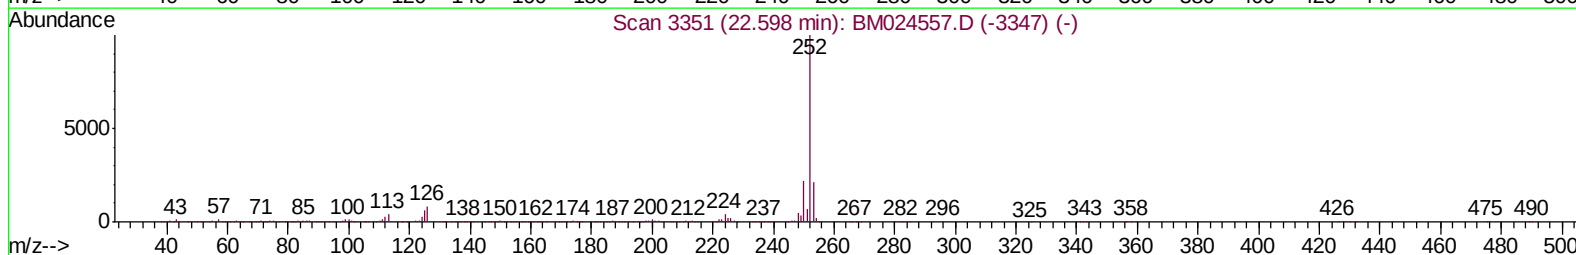
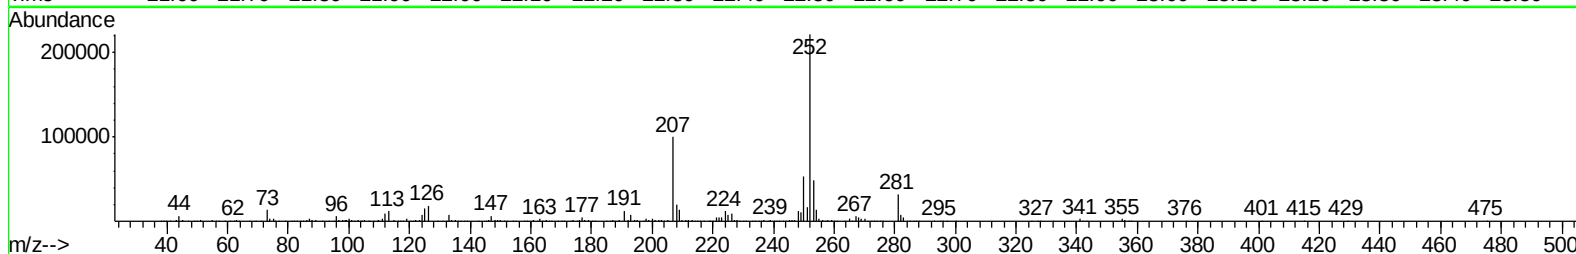


Data File : BM024567.D
Acq On : 21 Jan 2020 17:31
Operator : JU
Sample : L1109-10MEDL 10X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Quant Time: Jan 22 02:07:32 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM011520MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jan 22 02:05:31 2020
Response via : Initial Calibration

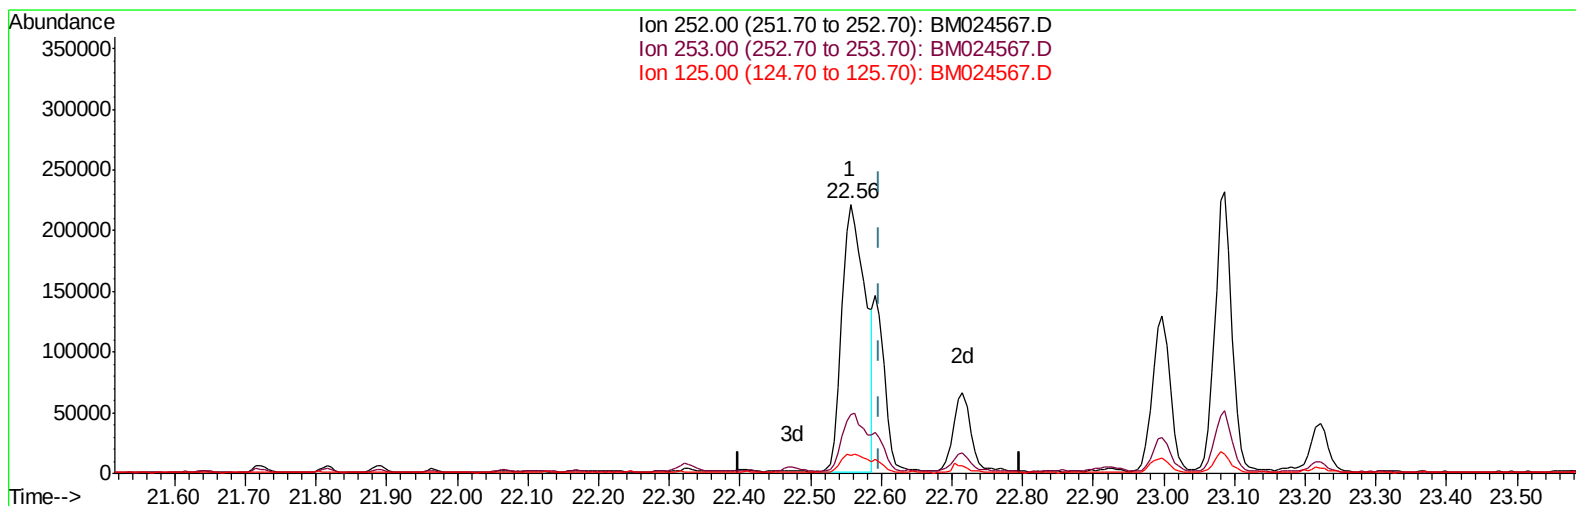

TIC: BM024567.D

(89) Benzo(k)fluoranthene
22.556min (-0.041) 5.68ng/ul
response 516550

Ion	Exp%	Act%
252.00	100	100
253.00	21.40	22.09
125.00	6.50	6.70
0.00	0.00	0.00