

Data File : BM024570.D

Acq On : 21 Jan 2020 19:19

Operator : JU

Sample : SSTDCCC020EC

Misc :

ALS Vial : 2 Sample Multiplier: 1




Quant Time: Jan 22 02:08:09 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM011520MA.M

Quant Title : SVOA CALIBRATION

QLast Update : Wed Jan 22 02:05:31 2020

Response via : Initial Calibration

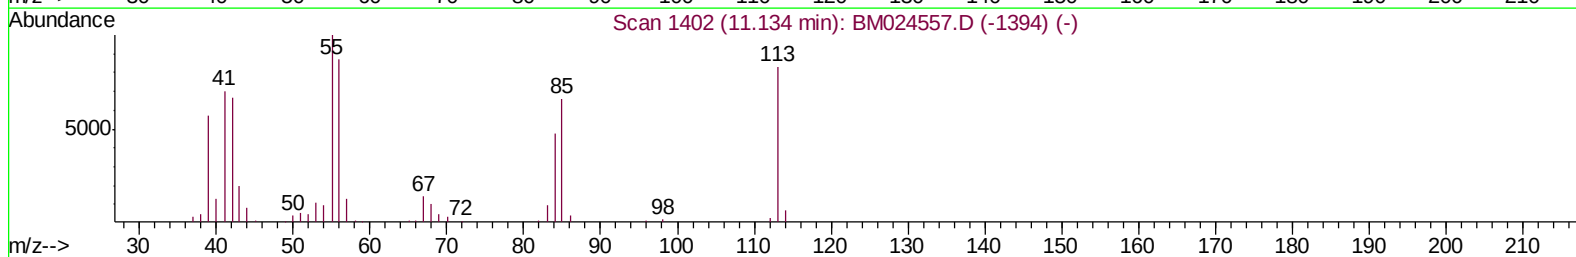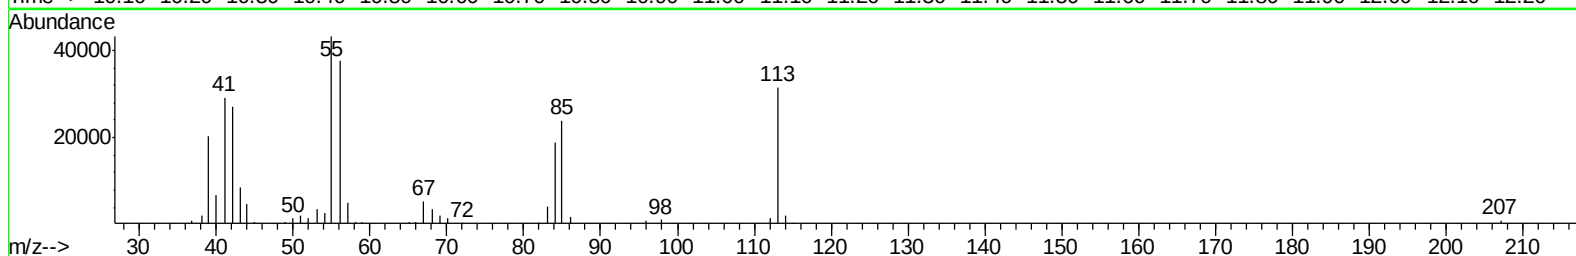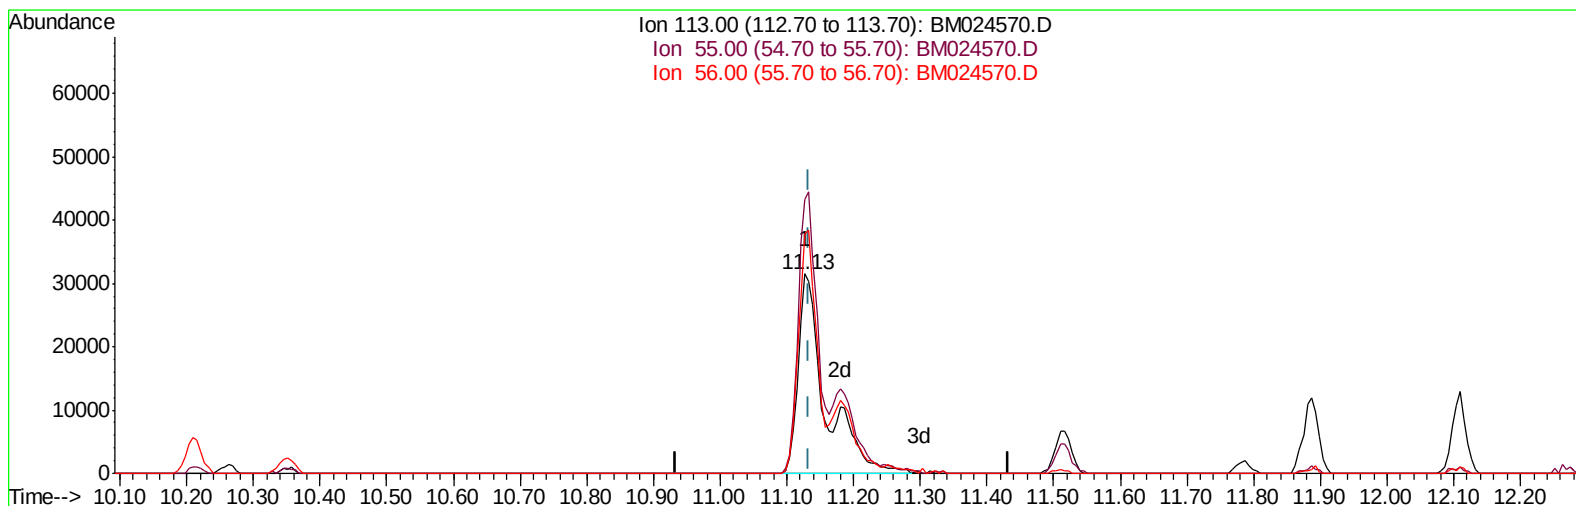

TIC: BM024570.D

(32) Caprolactam

11.127min (-0.006) 20.66ng/ul m

response 88270

Ion	Exp%	Act%
113.00	100	100
55.00	147.90	137.31
56.00	113.50	119.99
0.00	0.00	0.00