


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM012120\
Data File : BM024558.D
Acq On : 21 Jan 2020 12:08
Operator : JU
Sample : L1109-09ME
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GASG8ME

Manual Integrations
APPROVED

mohammad
1/23/2020 7:57:22 AM

Quant Time: Jan 21 14:41:10 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM011520MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jan 21 11:19:17 2020
Response via : Initial Calibration

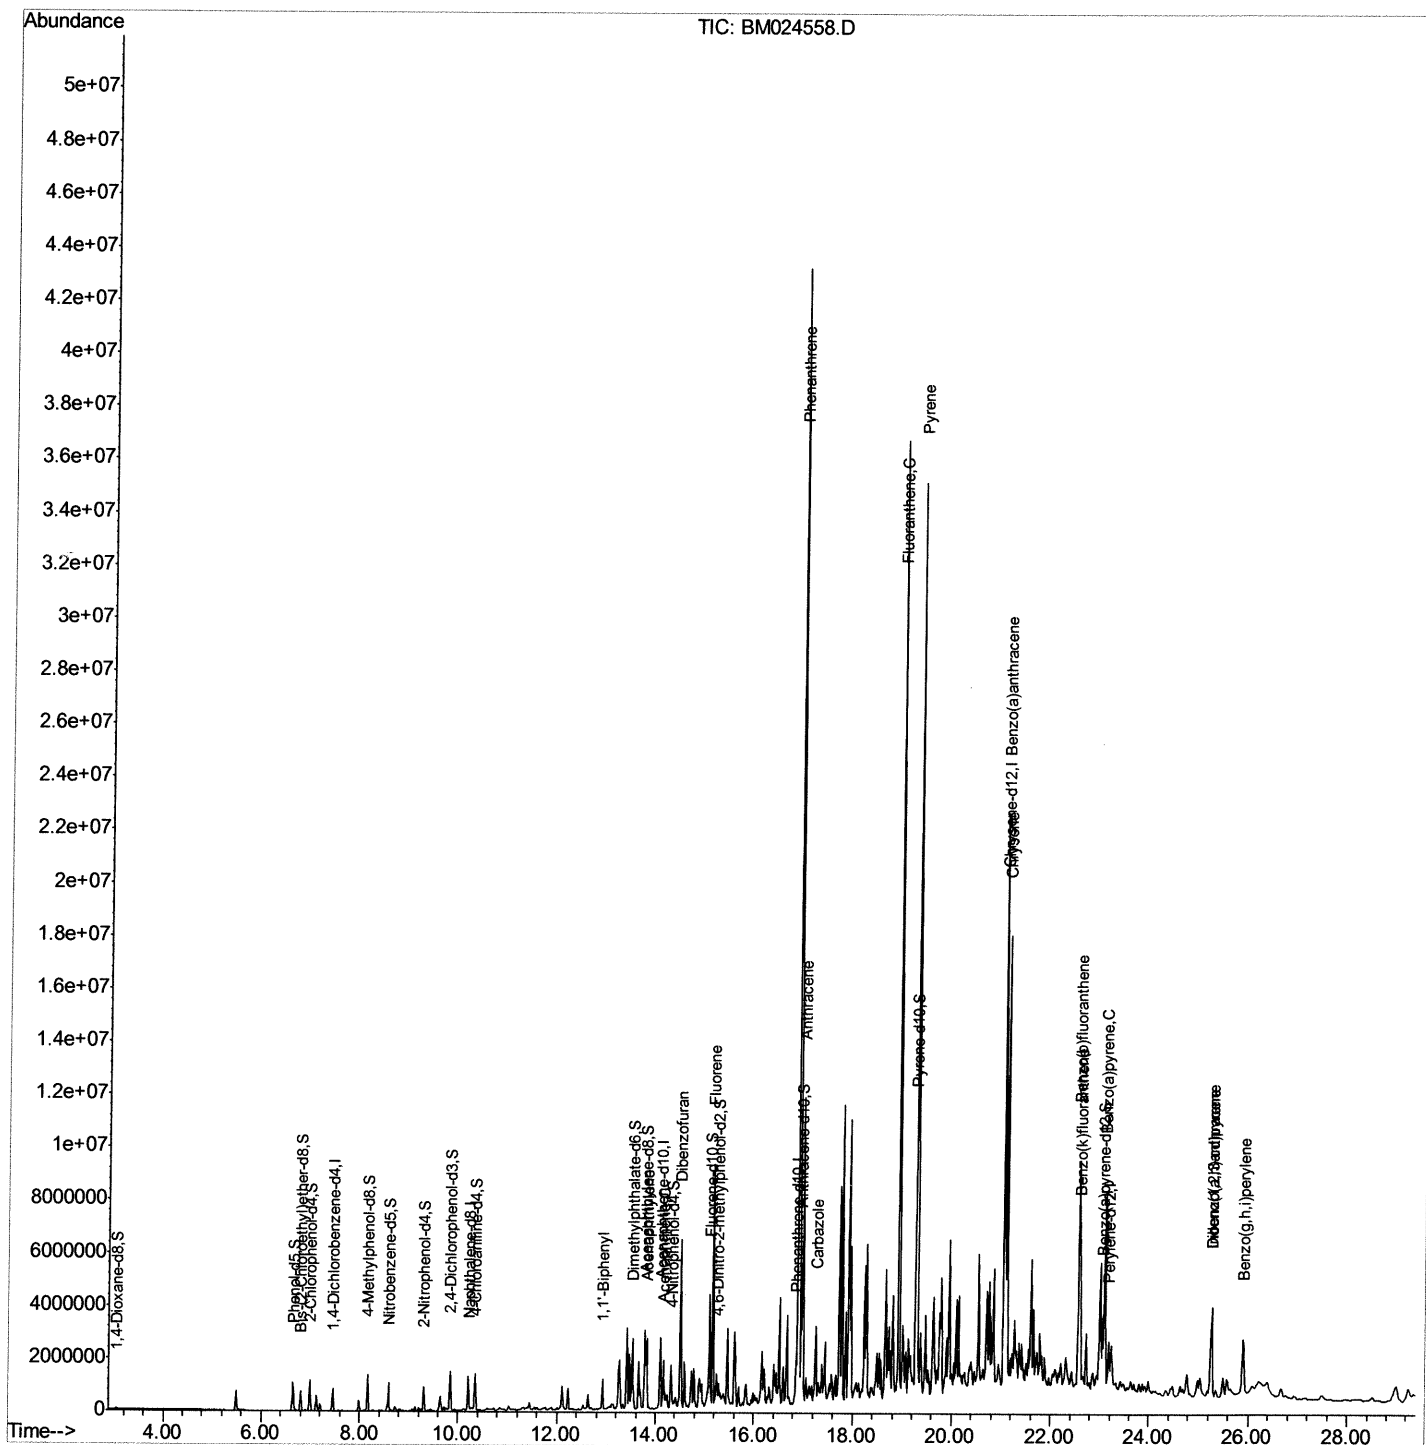

Quantitation Report (Qedit)


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM012120\
Data File : BM024558.D
Acq On : 21 Jan 2020 12:08
Operator : JU
Sample : L1109-09ME
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GASG8ME

Manual Integrations
APPROVED

mohammad
1/23/2020 7:57:22 AM

Quant Time: Jan 21 14:37:09 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM011520MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jan 21 11:19:17 2020
Response via : Initial Calibration

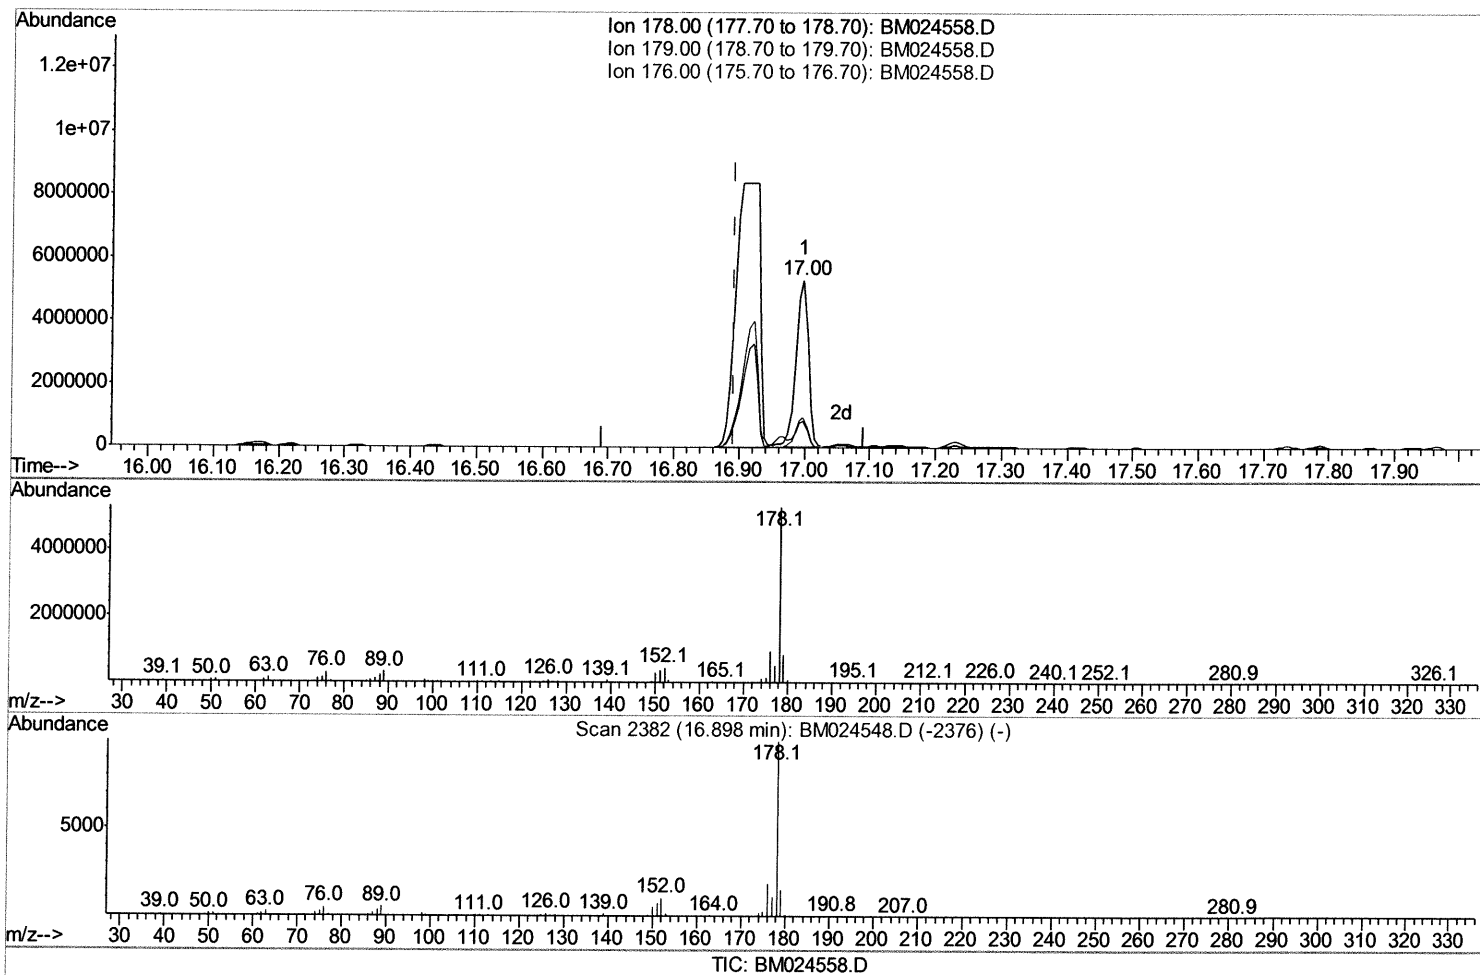

(70) Phenanthrene

16.998min (+0.106) 83.55ng/ul

response 6863881

Ion	Exp%	Act%
178.00	100	100
179.00	15.40	15.77
176.00	18.60	18.05
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM012120\
Data File : BM024558.D
Acq On : 21 Jan 2020 12:08
Operator : JU
Sample : L1109-09ME
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GASG8ME

Manual Integrations
APPROVED

mohammad
1/23/2020 7:57:22 AM

Quant Time: Jan 21 14:37:09 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM011520MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jan 21 11:19:17 2020
Response via : Initial Calibration

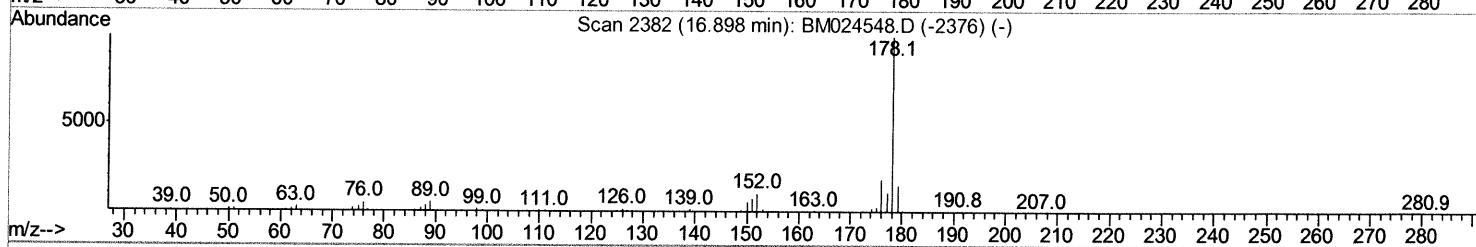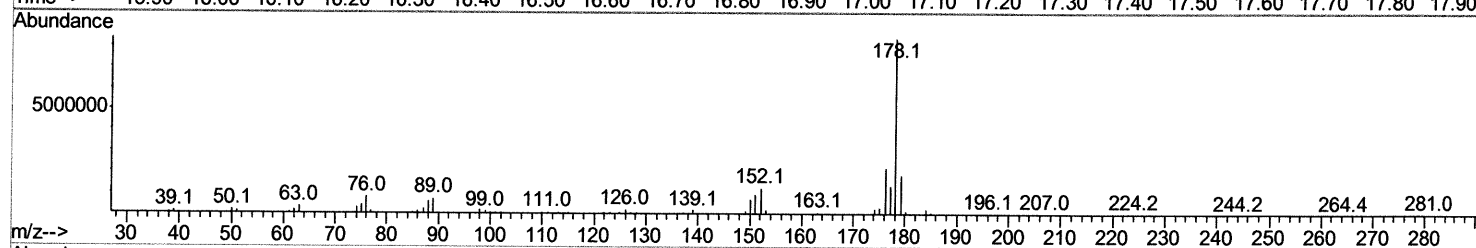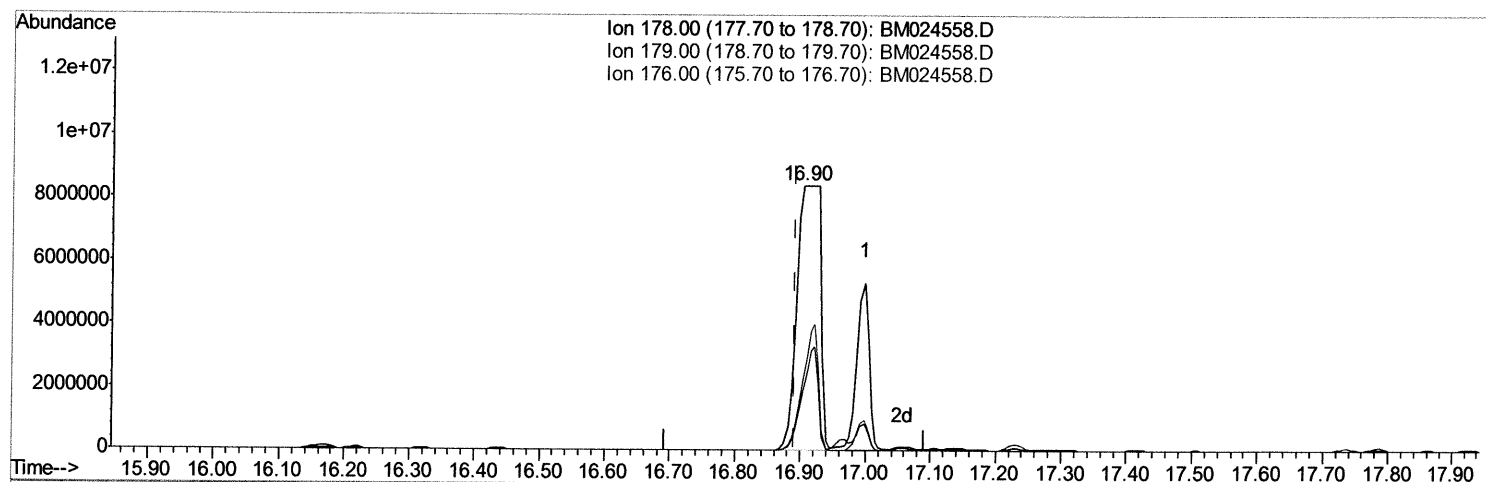

TIC: BM024558.D

(70) Phenanthrene

16.904min (+0.012) 257.44ng/ul m> SJ 1/22/20

response 21149008

Ion	Exp%	Act%
178.00	100	100
179.00	15.40	22.00#
176.00	18.60	25.80#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM012120\
Data File : BM024558.D
Acq On : 21 Jan 2020 12:08
Operator : JU
Sample : L1109-09ME
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GASG8ME

Manual Integrations
APPROVED

mohammad
1/23/2020 7:57:22 AM

Quant Time: Jan 21 14:37:09 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM011520MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jan 21 11:19:17 2020
Response via : Initial Calibration

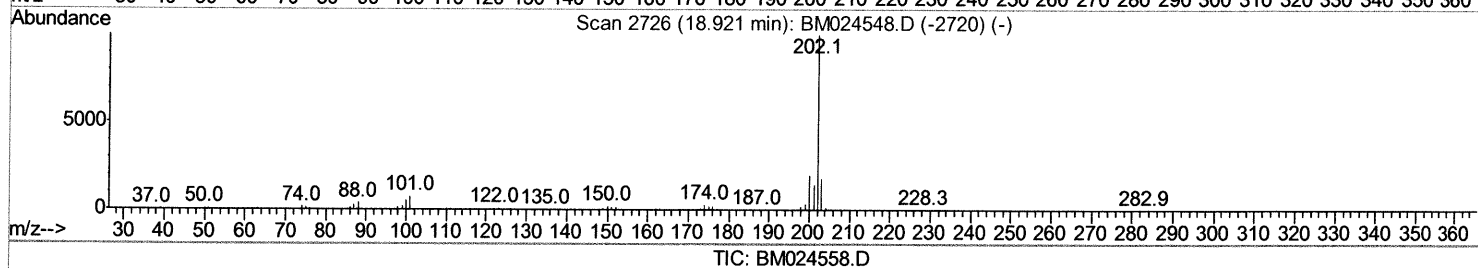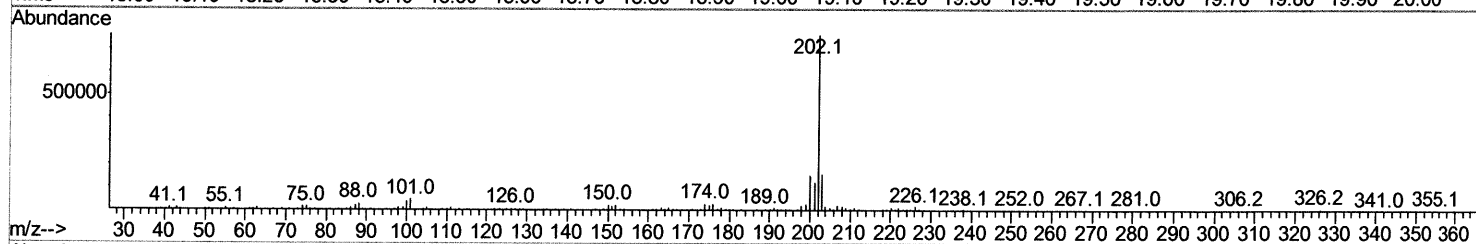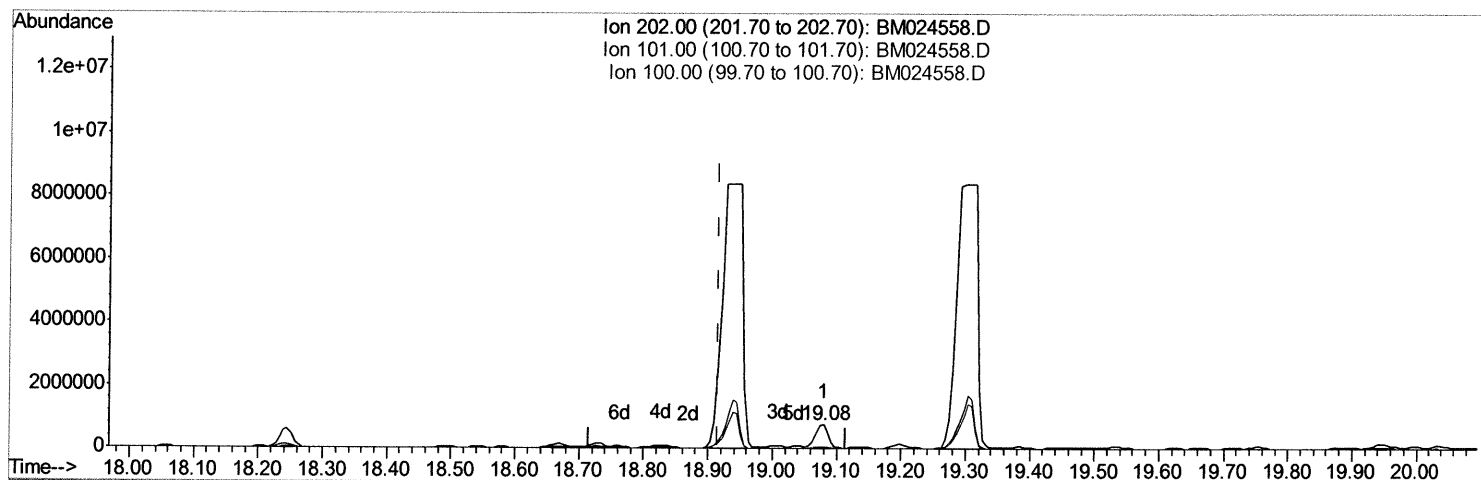

(77) Fluoranthene (C)

19.080min (+0.165) 8.80ng/ul

response 883874

Ion	Exp%	Act%
202.00	100	100
101.00	6.80	6.16
100.00	5.40	5.09
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM012120\
 Data File : BM024558.D
 Acq On : 21 Jan 2020 12:08
 Operator : JU
 Sample : L1109-09ME
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GASG8ME

Manual Integrations
 APPROVED

mohammad
 1/23/2020 7:57:22 AM

Quant Time: Jan 21 14:37:09 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM011520MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jan 21 11:19:17 2020
 Response via : Initial Calibration

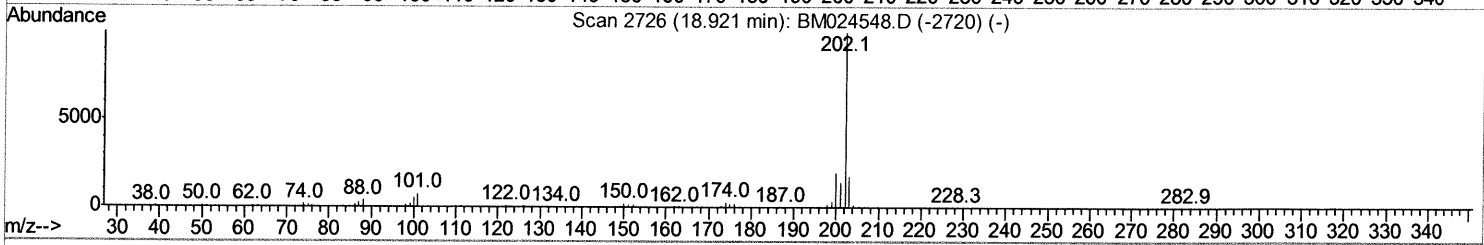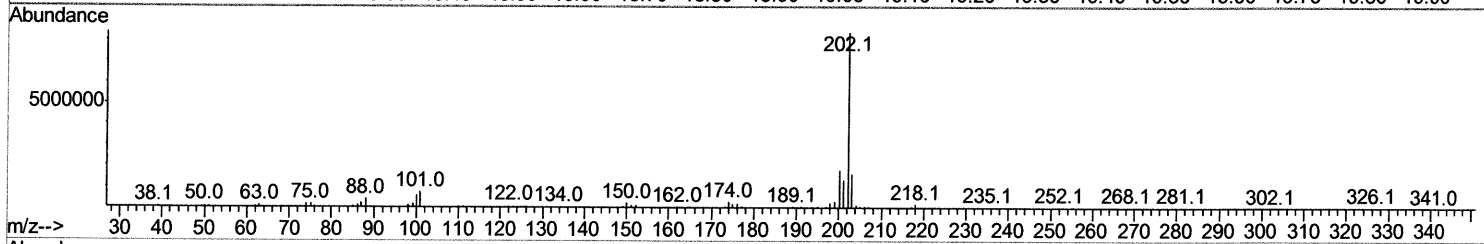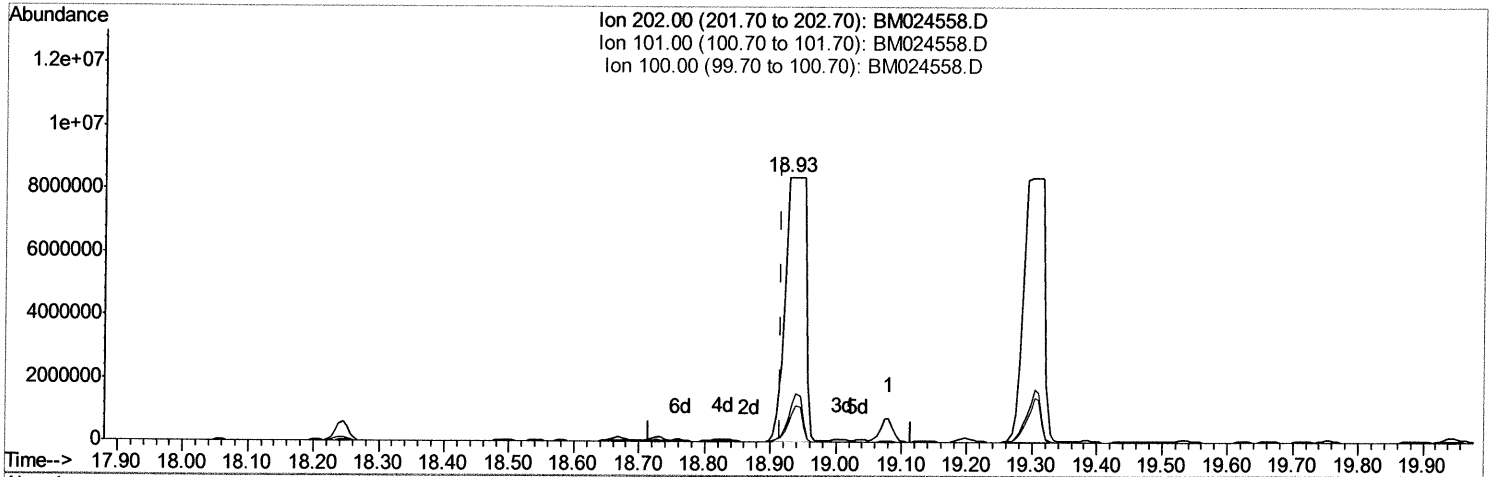

TIC: BM024558.D

(77) Fluoranthene (C)

18.927min (+0.012) 185.94ng/ul m> SJ 1/22/20

response 18669630

Ion	Exp%	Act%
202.00	100	100
101.00	6.80	8.86#
100.00	5.40	6.97#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM012120\
Data File : BM024558.D
Acq On : 21 Jan 2020 12:08
Operator : JU
Sample : L1109-09ME
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GASG8ME

Manual Integrations
APPROVED

mohammad
1/23/2020 7:57:22 AM

Quant Time: Jan 21 14:37:09 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM011520MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jan 21 11:19:17 2020
Response via : Initial Calibration

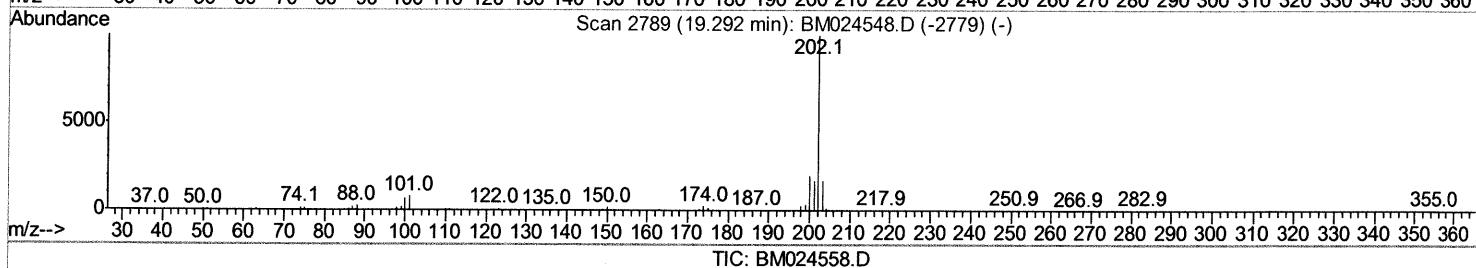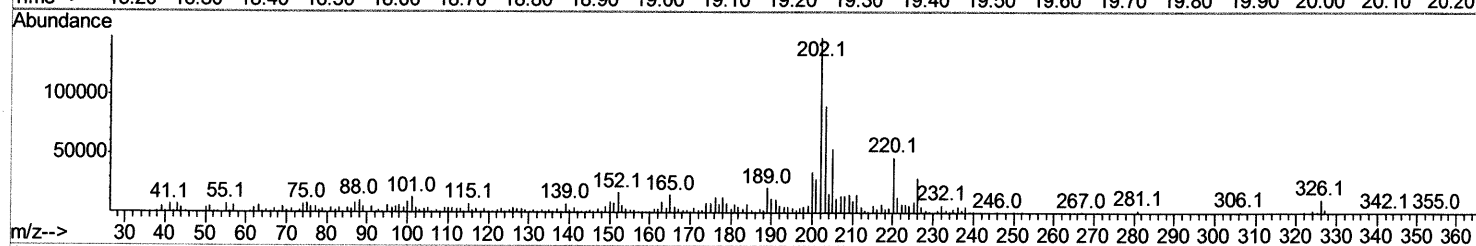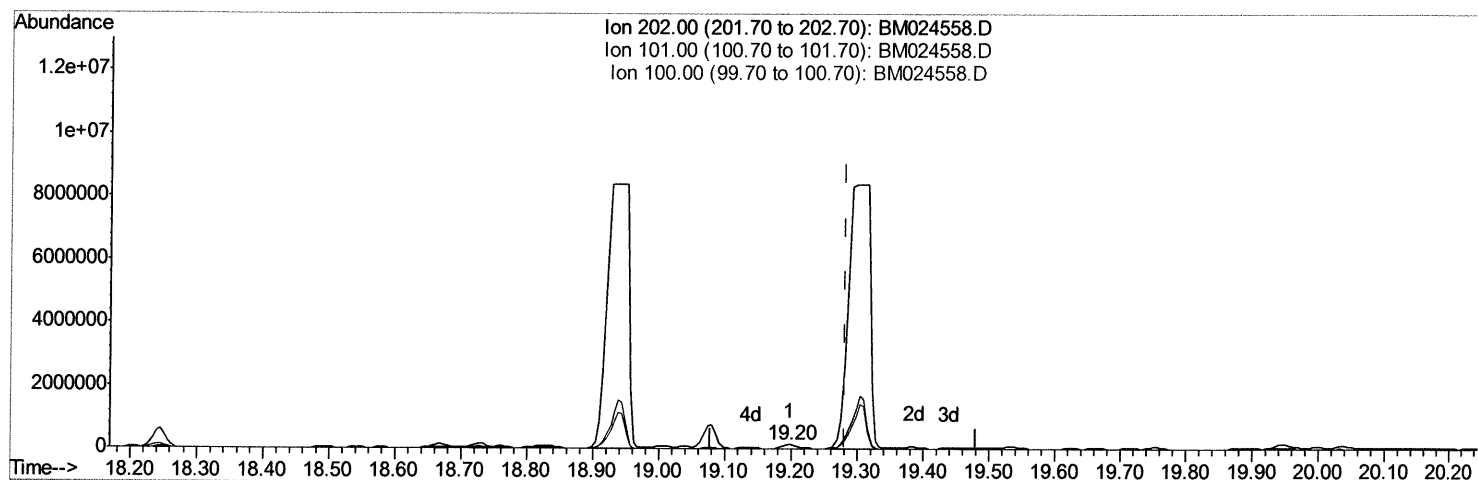

(80) Pyrene

19.198min (-0.082) 2.23ng/ul

response 216081

Ion	Exp%	Act%
202.00	100	100
101.00	8.10	8.87
100.00	6.30	6.36
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM012120\
Data File : BM024558.D
Acq On : 21 Jan 2020 12:08
Operator : JU
Sample : L1109-09ME
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GASG8ME

Manual Integrations
APPROVED

mohammad
1/23/2020 7:57:22 AM

Quant Time: Jan 21 14:37:09 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM011520MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jan 21 11:19:17 2020
Response via : Initial Calibration

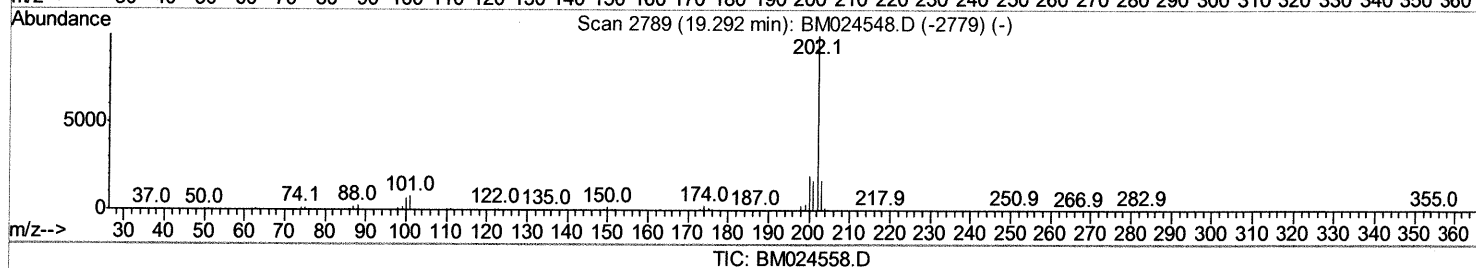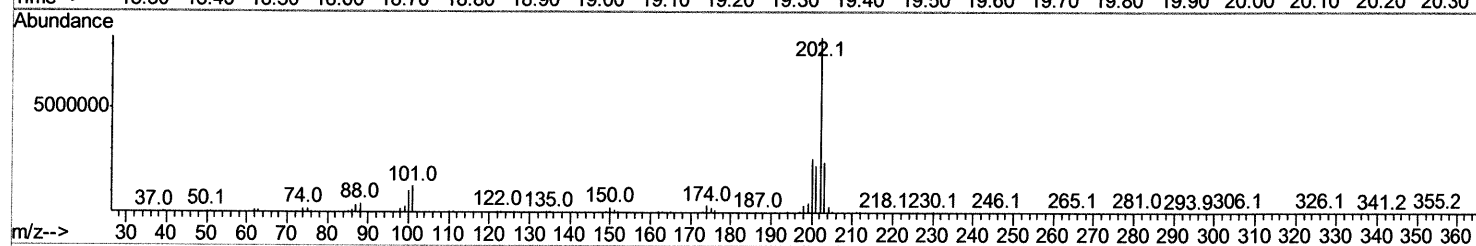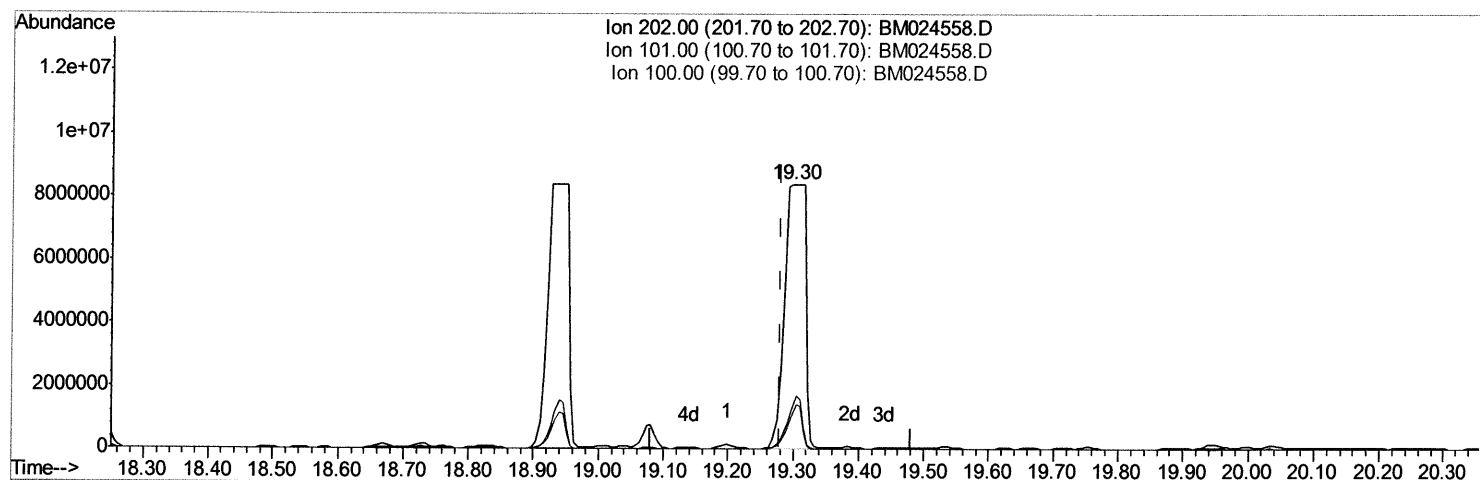

(80) Pyrene

19.298min (+0.018) 193.48ng/ul m> SJ 1/22/20

response 18776944

Ion	Exp%	Act%
202.00	100	100
101.00	8.10	14.95#
100.00	6.30	12.36#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM012120\
 Data File : BM024558.D
 Acq On : 21 Jan 2020 12:08
 Operator : JU
 Sample : L1109-09ME
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampleId :
 GASG8ME

Manual Integrations
APPROVED

mohammad
 1/23/2020 7:57:22 AM

Quant Time: Jan 21 14:37:09 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM011520MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jan 21 11:19:17 2020
 Response via : Initial Calibration

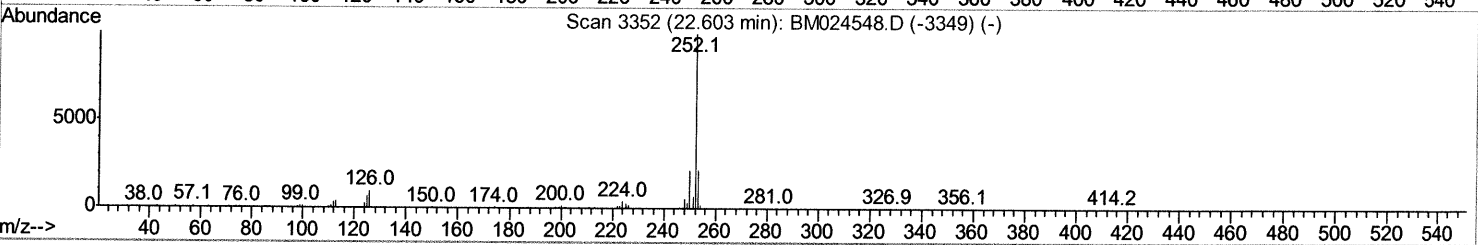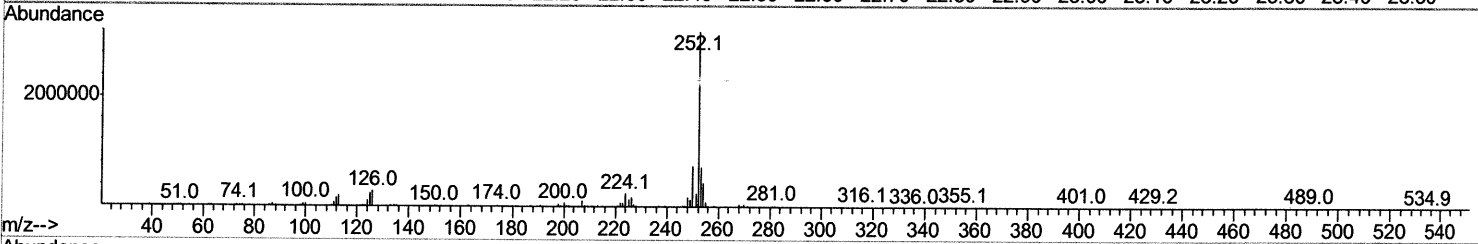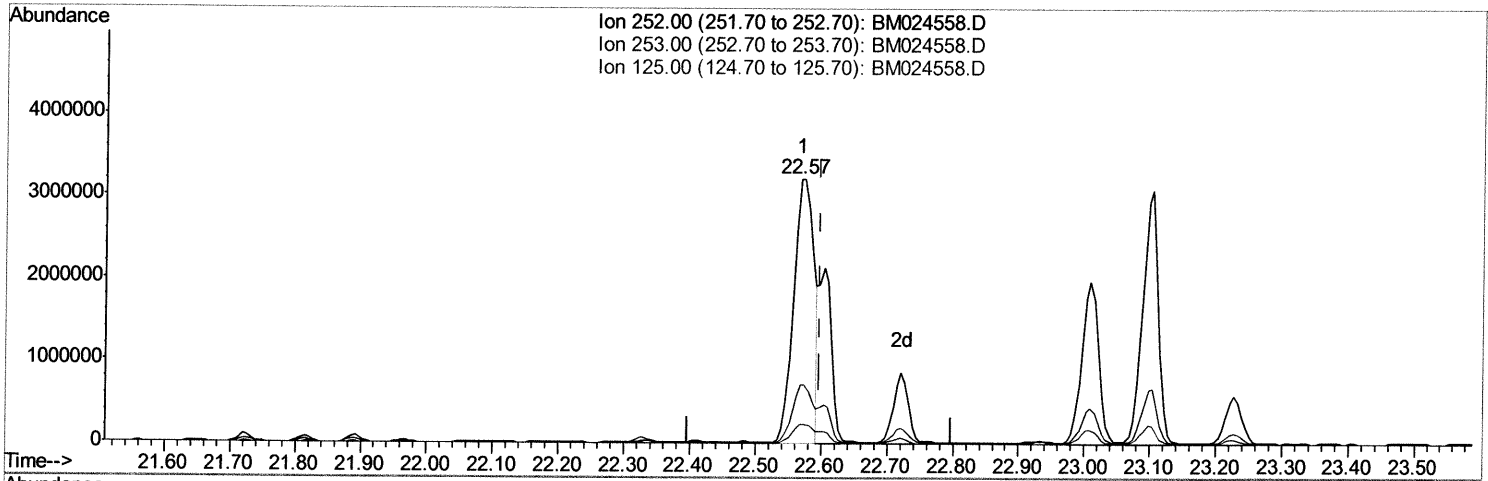

TIC: BM024558.D

(89) Benzo(k)fluoranthene
 22.568min (-0.030) 88.18ng/ul
 response 6907464

Ion	Exp%	Act%
252.00	100	100
253.00	21.40	22.34
125.00	6.50	7.25
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM012120\
Data File : BM024558.D
Acq On : 21 Jan 2020 12:08
Operator : JU
Sample : L1109-09ME
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GASG8ME

Manual Integrations
APPROVED

mohammad
1/23/2020 7:57:22 AM

Quant Time: Jan 21 14:37:09 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM011520MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jan 21 11:19:17 2020
Response via : Initial Calibration

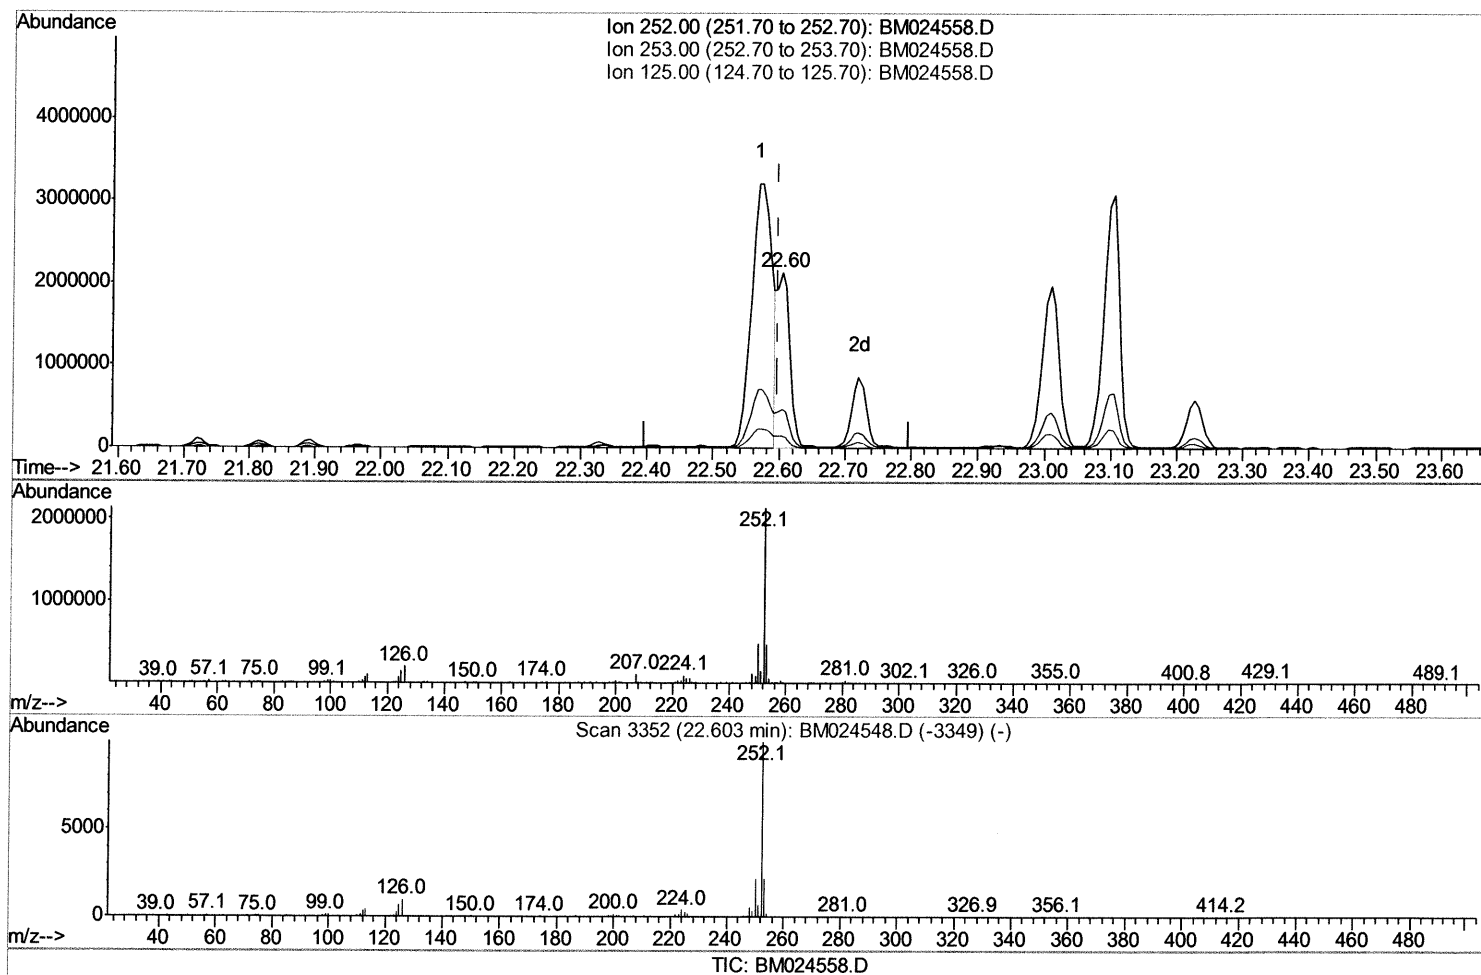

(89) Benzo(k)fluoranthene

22.603min (+0.006) 36.35ng/ul m> SJ 1/22/20

response 2847510

Ion	Exp%	Act%
252.00	100	100
253.00	21.40	22.24
125.00	6.50	7.10
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM012120\
Data File : BM024558.D
Acq On : 21 Jan 2020 12:08
Operator : JU
Sample : L1109-09ME
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GASG8ME

Manual Integrations
APPROVED

mohammad
1/23/2020 7:57:22 AM

Quant Time: Jan 21 14:37:09 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM011520MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jan 21 11:19:17 2020
Response via : Initial Calibration

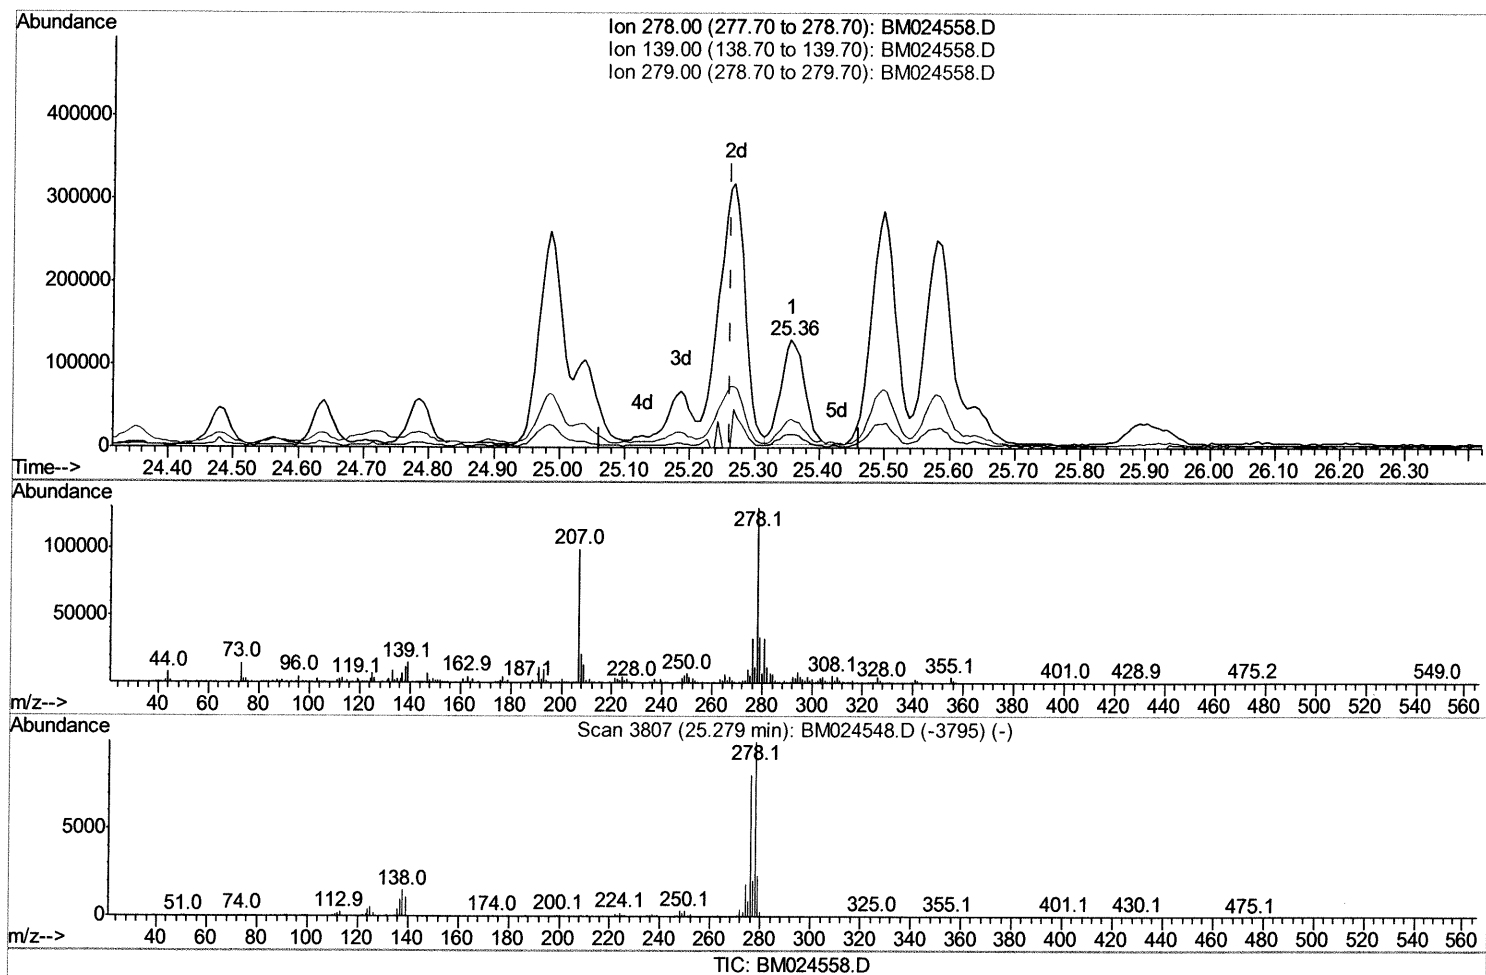

(93) Dibenzo(a,h)anthracene

25.356min (+0.094) 5.22ng/ul

response 320930

Ion	Exp%	Act%
278.00	100	100
139.00	10.90	11.83
279.00	23.20	26.39
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM012120\
Data File : BM024558.D
Acq On : 21 Jan 2020 12:08
Operator : JU
Sample : L1109-09ME
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GASG8ME

Manual Integrations
APPROVED

mohammad
1/23/2020 7:57:22 AM

Quant Time: Jan 21 14:37:09 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM011520MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jan 21 11:19:17 2020
Response via : Initial Calibration

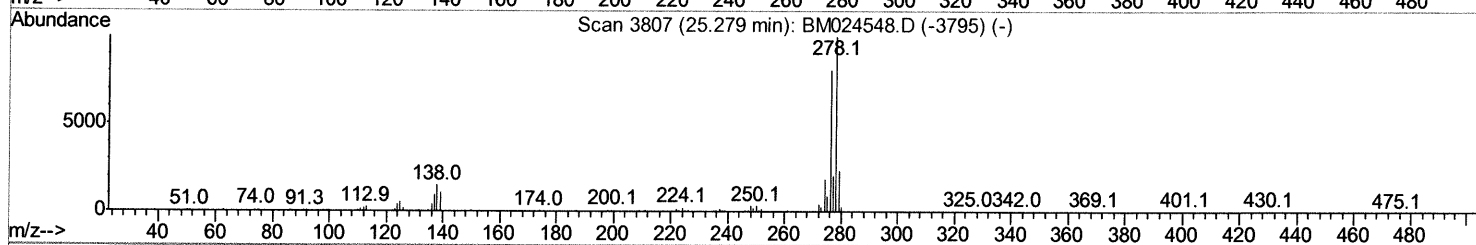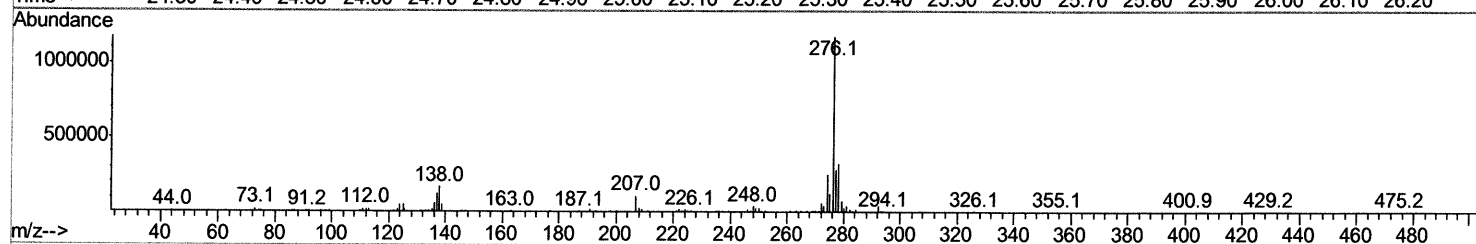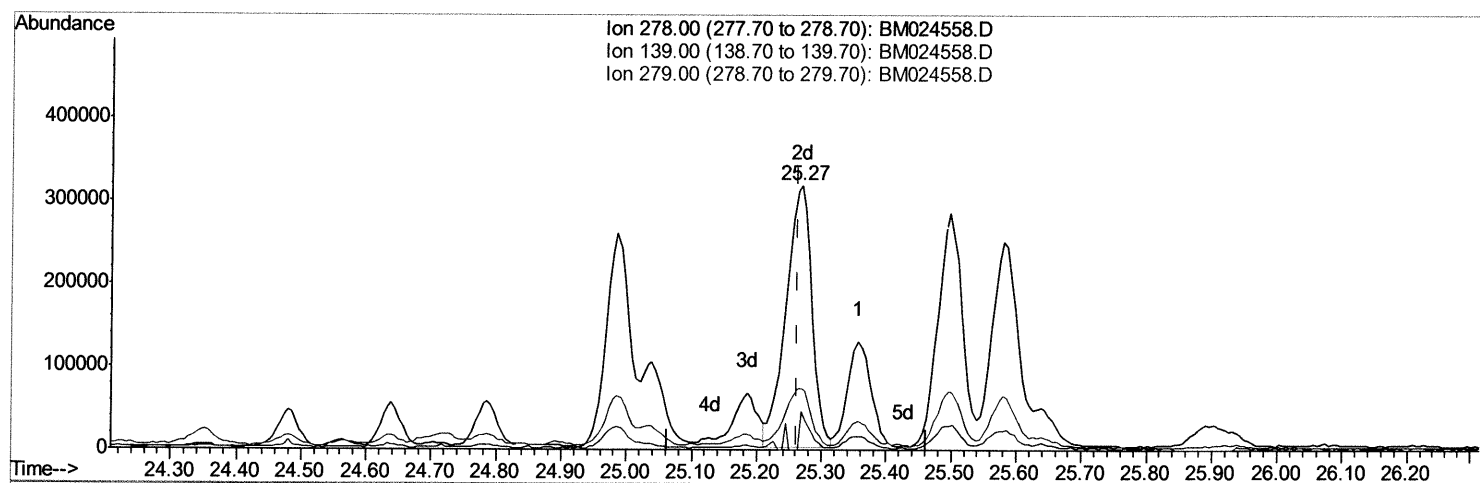

TIC: BM024558.D

(93) Dibenzo(a,h)anthracene

25.268min (+0.006) 14.40ng/ul m > 5] 1/22/20

response 885871

Ion	Exp%	Act%
278.00	100	100
139.00	10.90	14.59#
279.00	23.20	23.10
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM012120\
 Data File : BM024558.D
 Acq On : 21 Jan 2020 12:08
 Operator : JU
 Sample : L1109-09ME
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GASG8ME

Manual Integrations
 APPROVED

mohammad
 1/23/2020 7:57:22 AM

Quant Time: Jan 21 14:41:10 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM011520MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jan 21 11:19:17 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.46	152	231070	20.00	ng/ul	0.00
18) Naphthalene-d8	10.21	136	1003016	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.10	164	707554	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.86	188	1523327	20.00	ng/ul	0.00
78) Chrysene-d12	21.07	240	1417625	20.00	ng/ul	0.01
86) Perylene-d12	23.19	264	1205968	20.00	ng/ul	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.06	96	23044	4.87	ng/ul	0.00
5) Phenol-d5	6.65	99	546687	31.92	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.80	67	294106	30.91	ng/ul	0.00
9) 2-Chlorophenol-d4	6.99	132	484867	33.15	ng/ul	0.00
13) 4-Methylphenol-d8	8.16	113	476937	30.20	ng/ul	0.00
19) Nitrobenzene-d5	8.59	128	252170	35.78	ng/ul	0.00
22) 2-Nitrophenol-d4	9.31	143	295638	38.73	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.85	165	547297	31.86	ng/ul	0.00
29) 4-Chloroaniline-d4	10.35	131	694288	36.35	ng/ul	0.00
44) Dimethylphthalate-d6	13.53	166	1683037	30.36	ng/ul	0.00
47) Acenaphthylene-d8	13.79	160	1962526	30.76	ng/ul	0.00
52) 4-Nitrophenol-d4	14.32	143	287762	31.10	ng/ul	0.00
58) Fluorene-d10	15.10	176	1468580	30.09	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.24	200	241127	27.73	ng/ul	0.02
71) Anthracene-d10	16.96	188	2294278	32.39	ng/ul	0.01
79) Pyrene-d10	19.26	212	2685015	35.43	ng/ul	0.01
90) Benzo(a)pyrene-d12	23.06	264	2033408	32.51	ng/ul	0.01
Target Compounds						
					Ovalue	
41) 1,1'-Biphenyl	12.93	154	573941	11.173	ng/ul	98
48) Acenaphthylene	13.82	152	1440158	22.096	ng/ul	99
50) Acenaphthene	14.17	153	727239	16.486	ng/ul	99
54) Dibenzofuran	14.51	168	3345243	51.765	ng/ul	99
59) Fluorene	15.16	166	3553936	65.044	ng/ul	98
70) Phenanthrene	16.90	178	21149008m>	257.436	ng/ul	
72) Anthracene	17.00	178	6863881	81.932	ng/ul	99
75) Carbazole	17.26	167	1861197	26.404	ng/ul	99
77) Fluoranthene	18.93	202	18669630m>	185.941	ng/ul	
80) Pyrene	19.30	202	18776944m>	193.484	ng/ul	
83) Benzo(a)anthracene	21.06	228	10758403	111.405	ng/ul	95
85) Chrysene	21.11	228	9167544	98.518	ng/ul	98
88) Benzo(b)fluoranthene	22.57	252	6907464	86.659	ng/ul	99
89) Benzo(k)fluoranthene	22.60	252	2847510m>	36.350	ng/ul	
91) Benzo(a)pyrene	23.10	252	5090396	73.487	ng/ul	100
92) Indeno(1,2,3-cd)pyrene	25.26	276	3036903	41.901	ng/ul	99
93) Dibenzo(a,h)anthracene	25.27	278	885871m>	14.402	ng/ul	
94) Benzo(g,h,i)perylene	25.89	276	2517865	43.711	ng/ul	98

57 1/22/20

(#) = qualifier out of range (m) = manual integration (+) = signals summed