
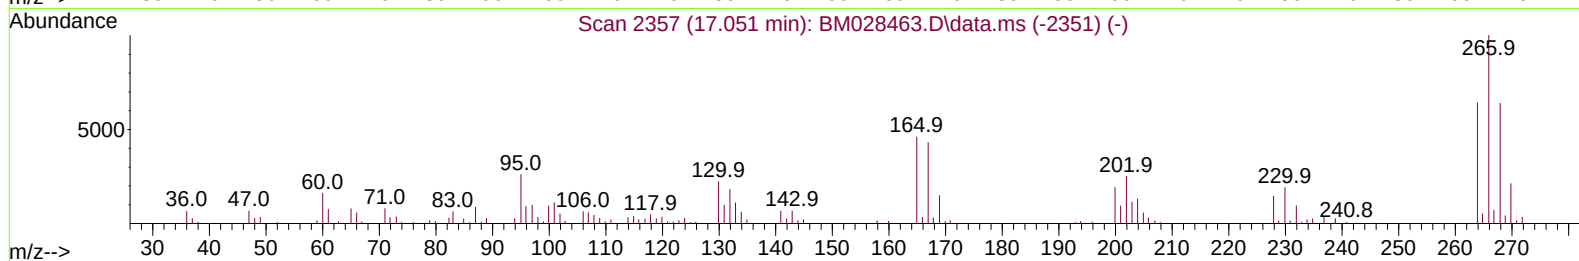
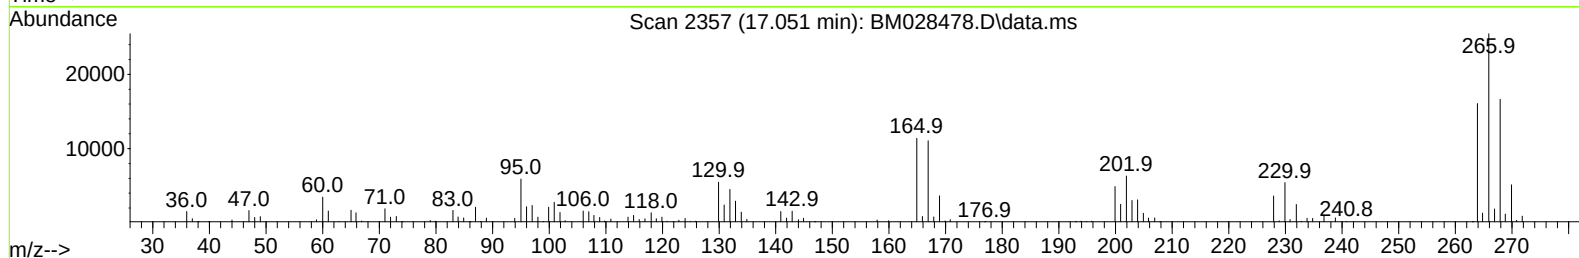


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012121\
Data File : BM028478.D
Acq On : 21 Jan 2021 08:18
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 22 01:31:56 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 20 14:45:01 2021
Response via : Initial Calibration

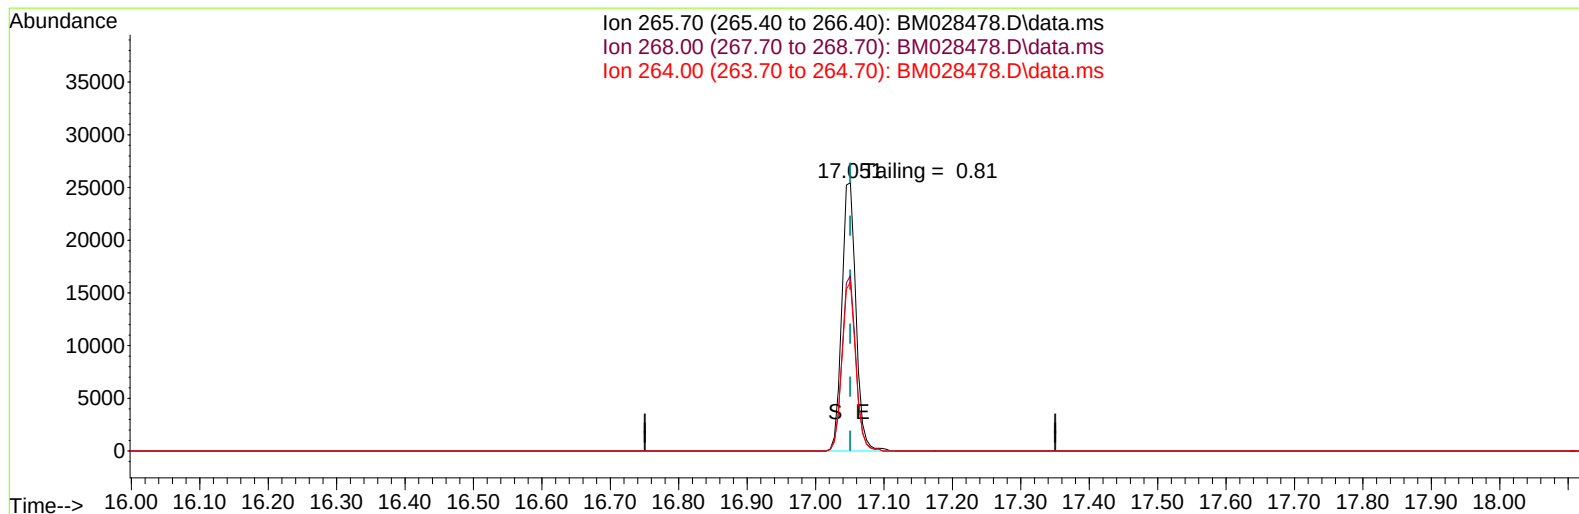

TIC: BM028478.D\data.ms

(70) Pentachlorophenol (C)




17.051min (+ 0.000) 0.00 ng

response 36519

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	65.28
264.00	63.30	63.08
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012121\
Data File : BM028478.D
Acq On : 21 Jan 2021 08:18
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 22 01:31:56 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 20 14:45:01 2021
Response via : Initial Calibration

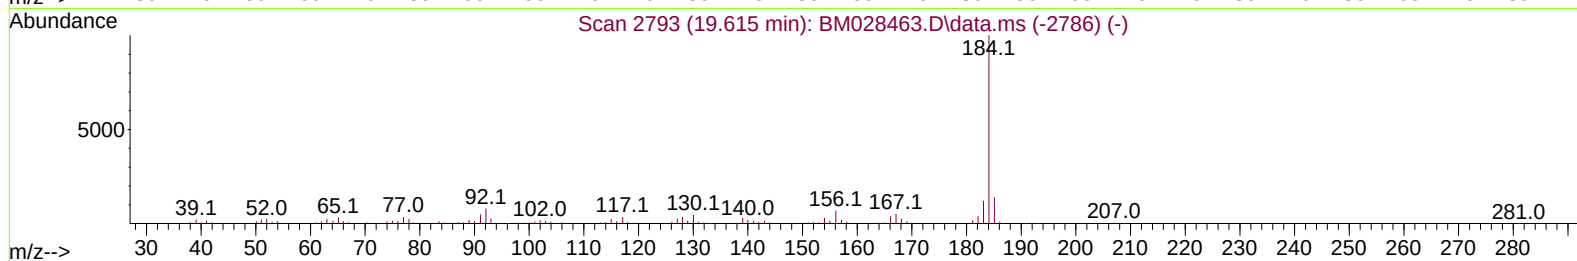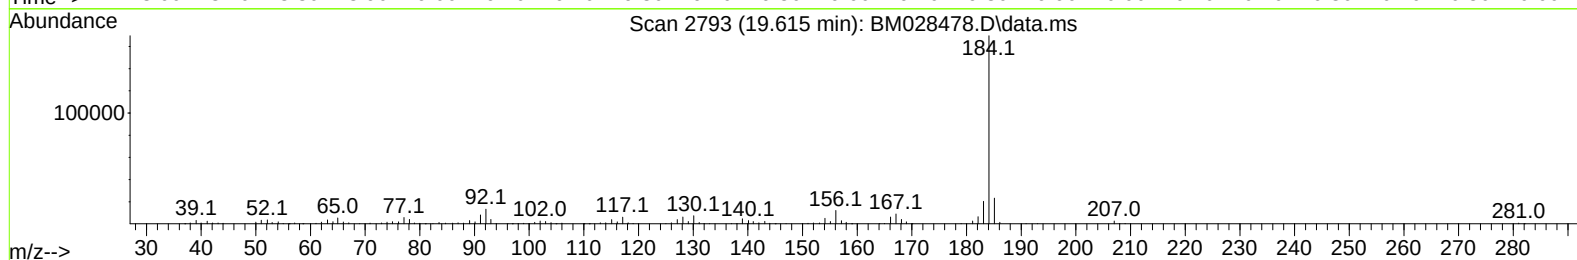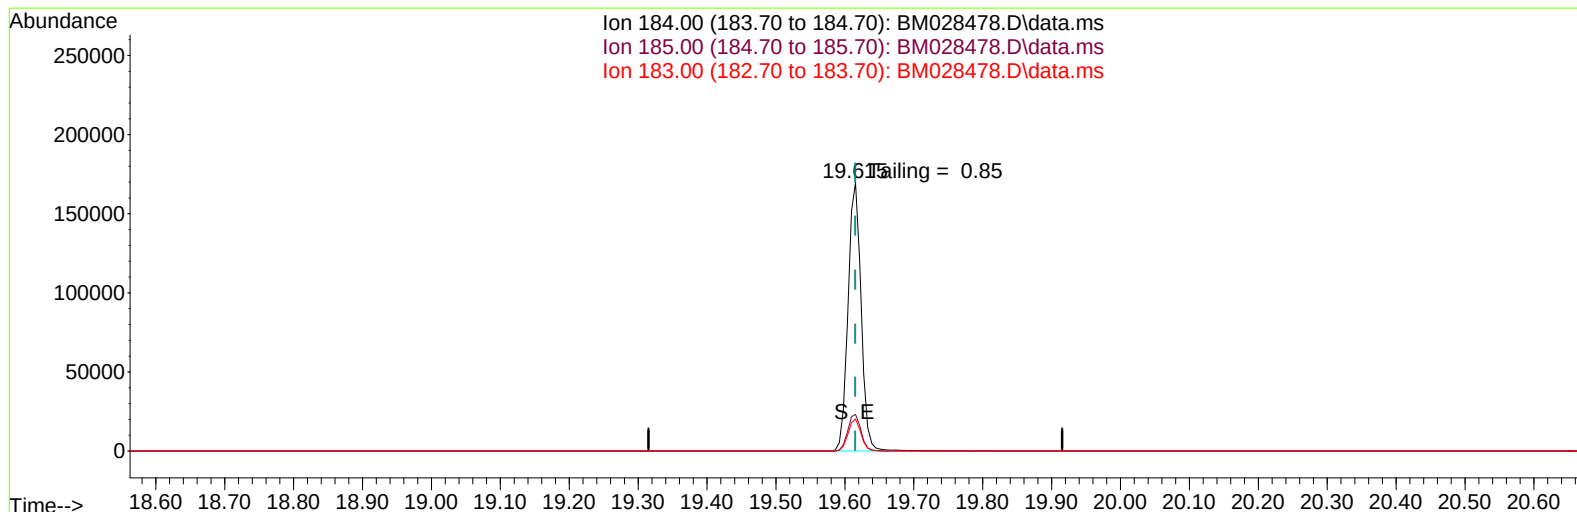

TIC: BM028478.D\data.ms

(77) Benzidine**19.615min (+ 0.000) 14936.94 ng****response 219677**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	13.68
183.00	12.10	11.96
0.00	0.00	0.00