

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012121\
 Data File : BM028480.D
 Acq On : 21 Jan 2021 09:30
 Operator : CG/JU
 Sample : PB134193BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB134193BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM028480.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.551	396	402	413	rBV	877822	1265163	56.17%	11.355%
2	7.193	673	681	692	rBV	844789	1318571	58.54%	11.834%
3	8.028	817	823	830	rVB	155974	236628	10.51%	2.124%
4	9.204	1016	1023	1033	rBV	500862	838973	37.25%	7.530%
5	10.845	1295	1302	1309	rBV	205975	332979	14.78%	2.988%
6	13.298	1712	1719	1725	rBV	1285304	1796067	79.74%	16.120%
7	14.669	1946	1952	1959	rVB	298830	430256	19.10%	3.862%
8	16.151	2198	2204	2218	rBV	1008842	1374383	61.02%	12.335%
9	17.398	2409	2416	2425	rBV	358326	493294	21.90%	4.427%
10	19.992	2851	2857	2862	rBV	1832024	2252390	100.00%	20.215%
11	21.527	3113	3118	3123	rBV	372344	441823	19.62%	3.965%
12	23.815	3501	3507	3515	rVB2	189644	361586	16.05%	3.245%




Sum of corrected areas: 11142113

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012121\
Data File : BM028480.D
Acq On : 21 Jan 2021 09:30
Operator : CG/JU
Sample : PB134193BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB134193BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

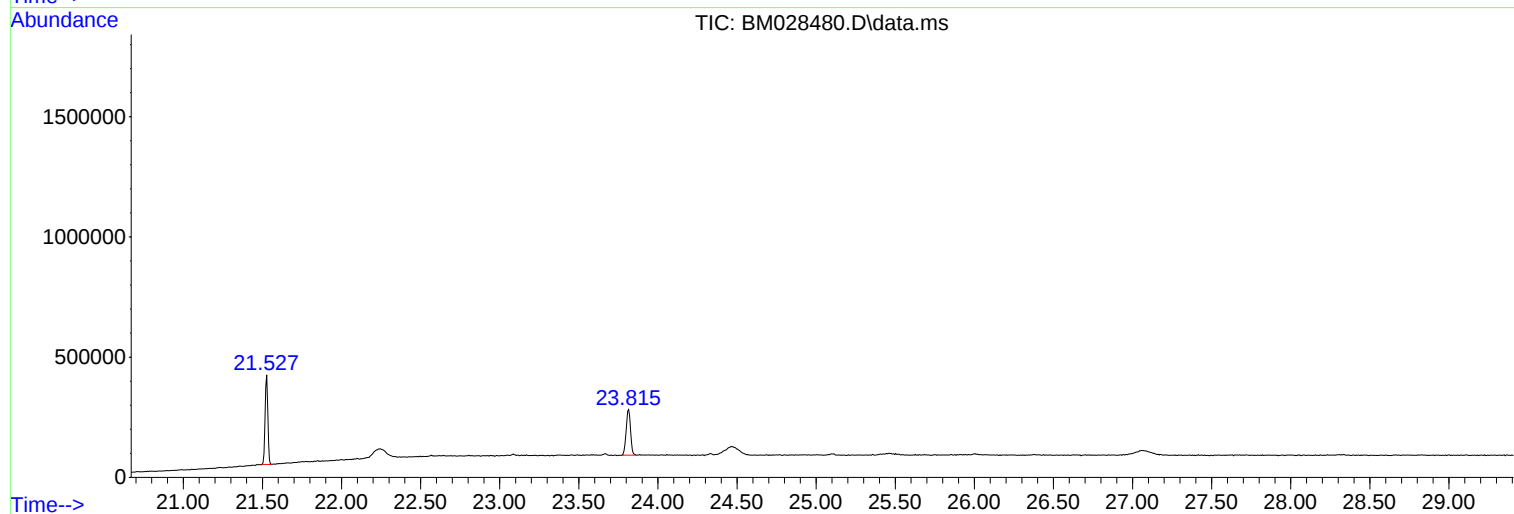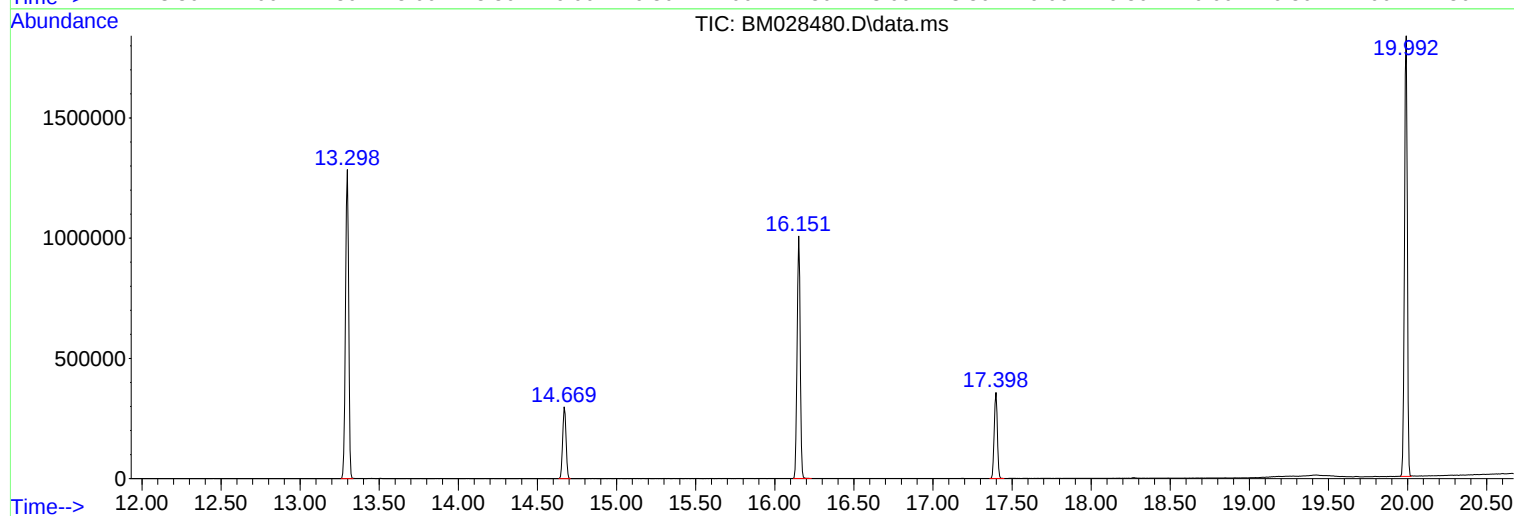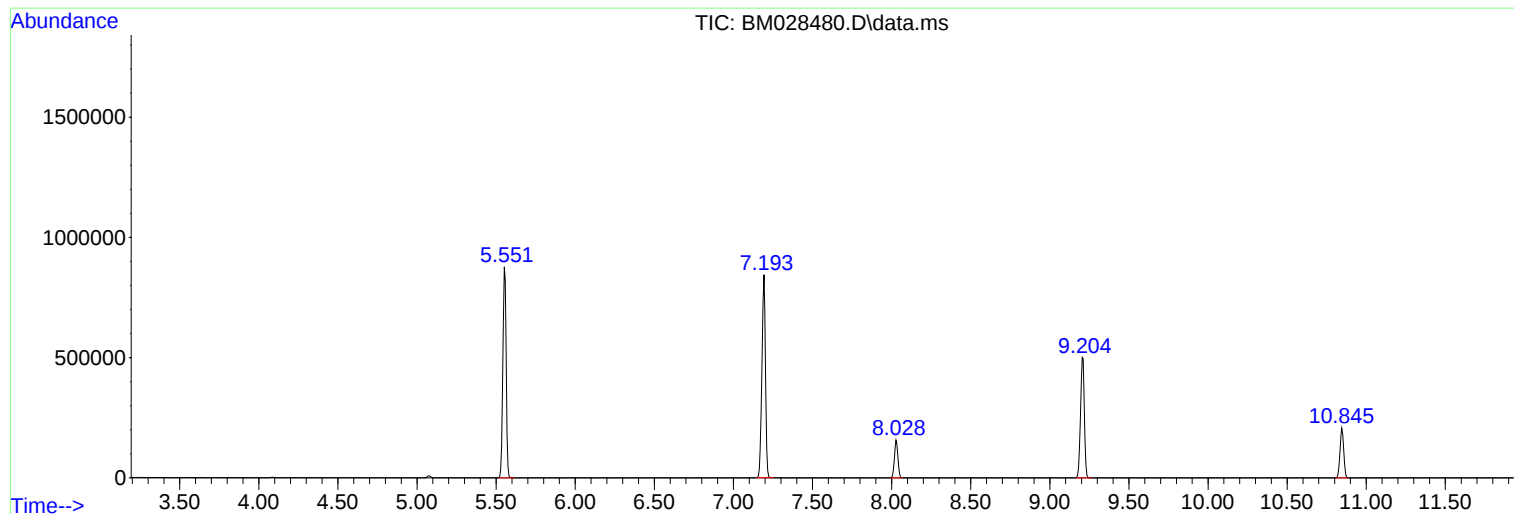

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012121\
Data File : BM028480.D
Acq On : 21 Jan 2021 09:30
Operator : CG/JU
Sample : PB134193BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB134193BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012121\
Data File : BM028480.D
Acq On : 21 Jan 2021 09:30
Operator : CG/JU
Sample : PB134193BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB134193BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------