

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012121\
 Data File : BM028485.D
 Acq On : 21 Jan 2021 12:41
 Operator : CG/JU
 Sample : M1100-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 TOPSOIL-RBF-DARK

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM028485.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.610	68	72	82	rBV	12788	21200	1.63%	0.189%
2	5.552	396	402	412	rBV	631384	913590	70.30%	8.156%
3	6.681	589	594	598	rVB	9787	13139	1.01%	0.117%
4	7.187	673	680	691	rBV	613634	1009325	77.67%	9.010%
5	7.451	720	725	731	rBV	10242	14978	1.15%	0.134%
6	7.622	749	754	762	rBV	46107	69899	5.38%	0.624%
7	8.028	816	823	829	rBB	121162	182021	14.01%	1.625%
8	9.204	1015	1023	1033	rBV	386602	630616	48.53%	5.630%
9	10.145	1173	1183	1192	rVB3	9437	18139	1.40%	0.162%
10	10.845	1295	1302	1310	rVB	154582	251906	19.38%	2.249%
11	13.292	1711	1718	1724	rBV	812491	1164879	89.64%	10.399%
12	13.404	1731	1737	1744	rBV	50321	74084	5.70%	0.661%
13	13.539	1755	1760	1772	rVB3	133259	221031	17.01%	1.973%
14	14.116	1853	1858	1866	rVB	96934	136962	10.54%	1.223%
15	14.498	1913	1923	1930	rBV3	10959	22091	1.70%	0.197%
16	14.669	1946	1952	1958	rVB	219009	314712	24.22%	2.810%
17	14.727	1958	1962	1969	rBV3	19150	29722	2.29%	0.265%
18	14.939	1988	1998	2002	rBV2	14842	24385	1.88%	0.218%
19	15.069	2014	2020	2025	rBV2	10614	15340	1.18%	0.137%
20	15.533	2095	2099	2105	rVB2	11349	13907	1.07%	0.124%
21	15.598	2105	2110	2115	rBV2	11038	15208	1.17%	0.136%
22	16.092	2188	2194	2197	rBV2	9817	15844	1.22%	0.141%
23	16.151	2197	2204	2210	rVB	612511	880476	67.75%	7.860%
24	16.427	2244	2251	2258	rBV	104502	136666	10.52%	1.220%
25	16.933	2333	2337	2344	rVB	9514	13743	1.06%	0.123%
26	17.392	2408	2415	2424	rBV	241738	365359	28.11%	3.262%
27	18.274	2559	2565	2579	rBV	421551	614068	47.25%	5.482%
28	18.457	2591	2596	2605	rVB	69444	93093	7.16%	0.831%
29	18.551	2608	2612	2618	rBV2	22908	30839	2.37%	0.275%
30	19.392	2751	2755	2757	rBV2	20452	26751	2.06%	0.239%
31	19.421	2757	2760	2767	rVB2	21667	45974	3.54%	0.410%
32	19.539	2774	2780	2796	rBV	324901	488223	37.57%	4.358%
33	19.986	2851	2856	2861	rVB	1063359	1299521	100.00%	11.601%
34	20.251	2898	2901	2904	rBV5	11329	15589	1.20%	0.139%
35	20.280	2904	2906	2909	rVB2	13856	13046	1.00%	0.116%
36	21.221	3062	3066	3072	rBV	246869	305117	23.48%	2.724%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012121\
 Data File : BM028485.D
 Acq On : 21 Jan 2021 12:41
 Operator : CG/JU
 Sample : M1100-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 TOPSOIL-RBF-DARK

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	21.521	3112	3117	3123	rBV	307831	402862	31.00%	3.596%
38	21.656	3138	3140	3147	rVB2	25939	31130	2.40%	0.278%
39	22.115	3211	3218	3228	rBV2	117066	225865	17.38%	2.016%
40	22.568	3291	3295	3299	rVB	48014	61476	4.73%	0.549%
41	22.803	3332	3335	3341	rVB3	40227	51990	4.00%	0.464%
42	23.080	3378	3382	3387	rBV	97073	146581	11.28%	1.309%
43	23.133	3388	3391	3398	rVB2	50848	82570	6.35%	0.737%
44	23.809	3500	3506	3514	rVB2	194696	376565	28.98%	3.362%
45	23.986	3533	3536	3544	rVB	47727	83748	6.44%	0.748%
46	24.327	3590	3594	3601	rVB2	55225	99202	7.63%	0.886%
47	24.421	3606	3610	3619	rVB2	62040	138266	10.64%	1.234%




Sum of corrected areas: 11201698

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012121\
Data File : BM028485.D
Acq On : 21 Jan 2021 12:41
Operator : CG/JU
Sample : M1100-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
TOPSOIL-RBF-DARK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

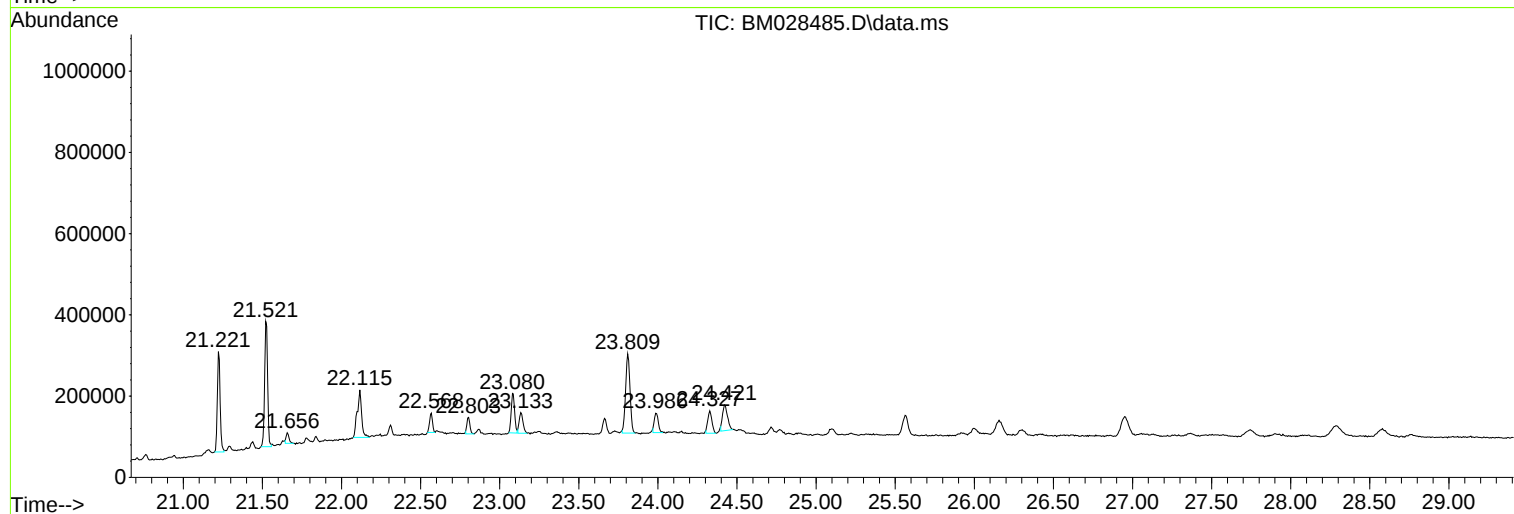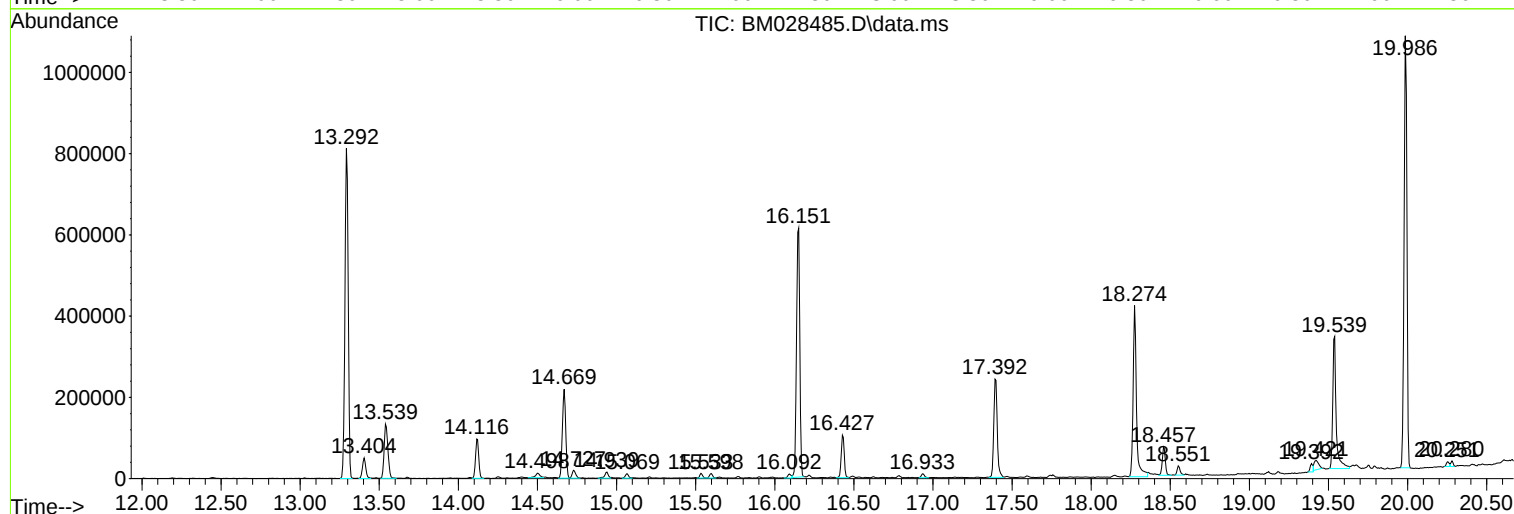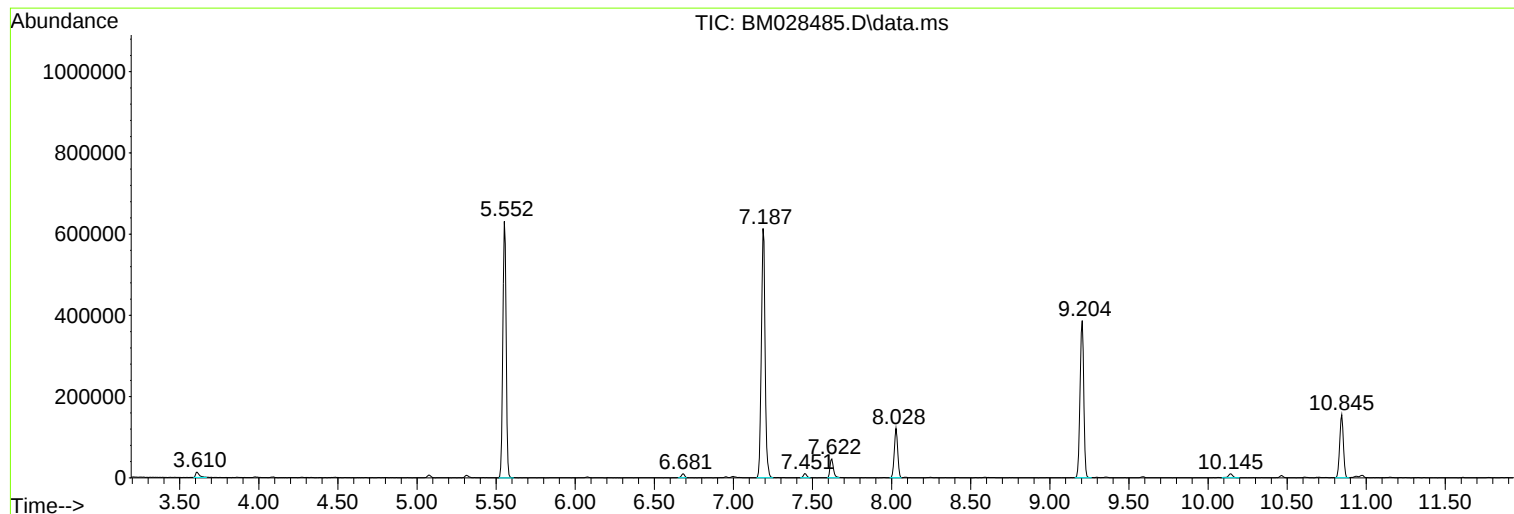

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012121\
Data File : BM028485.D
Acq On : 21 Jan 2021 12:41
Operator : CG/JU
Sample : M1100-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
TOPSOIL-RBF-DARK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012121\
Data File : BM028485.D
Acq On : 21 Jan 2021 12:41
Operator : CG/JU
Sample : M1100-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
TOPSOIL-RBF-DARK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------