

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012121\
 Data File : BM028487.D
 Acq On : 21 Jan 2021 13:54
 Operator : CG/JU
 Sample : M1082-02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BACKFILL-ASHCROFT-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM028487.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.075	315	321	326	rBV	10476	15147	1.28%	0.194%
2	5.552	395	402	413	rBV	504440	719119	61.00%	9.189%
3	7.187	673	680	691	rBV	481650	761035	64.55%	9.724%
4	7.622	748	754	763	rBV	8567	13973	1.19%	0.179%
5	8.028	816	823	829	rVB	126611	192203	16.30%	2.456%
6	9.204	1015	1023	1033	rBV	292148	483767	41.04%	6.182%
7	10.845	1295	1302	1309	rVB	158407	262023	22.23%	3.348%
8	13.292	1711	1718	1725	rBV	666513	945480	80.20%	12.081%
9	13.557	1756	1763	1772	rBV	258805	383041	32.49%	4.894%
10	14.116	1852	1858	1864	rBV	36276	47981	4.07%	0.613%
11	14.669	1946	1952	1960	rVB	220133	321890	27.30%	4.113%
12	15.769	2133	2139	2148	rBV	98804	131728	11.17%	1.683%
13	16.145	2197	2203	2218	rVB	494734	698977	59.29%	8.931%
14	17.398	2410	2416	2421	rBV	243614	350247	29.71%	4.475%
15	17.680	2458	2464	2472	rBV3	14052	23145	1.96%	0.296%
16	18.263	2559	2563	2569	rBV	50457	73171	6.21%	0.935%
17	19.021	2687	2692	2698	rBV	33255	42233	3.58%	0.540%
18	19.110	2703	2707	2715	rVV3	12543	20256	1.72%	0.259%
19	19.433	2758	2762	2766	rVB	41341	49149	4.17%	0.628%
20	19.527	2774	2778	2784	rBV2	20430	32793	2.78%	0.419%
21	19.651	2796	2799	2802	rBV	10640	12355	1.05%	0.158%
22	19.792	2819	2823	2830	rVB2	13371	16980	1.44%	0.217%
23	19.986	2850	2856	2861	rBV	1001895	1178900	100.00%	15.064%
24	20.651	2966	2969	2975	rVB	14202	17789	1.51%	0.227%
25	20.856	3000	3004	3008	rBV	49968	53649	4.55%	0.686%
26	21.221	3062	3066	3074	rBV	157985	196014	16.63%	2.505%
27	21.521	3113	3117	3126	rVB	294929	388589	32.96%	4.965%
28	23.809	3501	3506	3518	rVB2	205624	394376	33.45%	5.039%




Sum of corrected areas: 7826010

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012121\
Data File : BM028487.D
Acq On : 21 Jan 2021 13:54
Operator : CG/JU
Sample : M1082-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BACKFILL-ASHCROFT-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

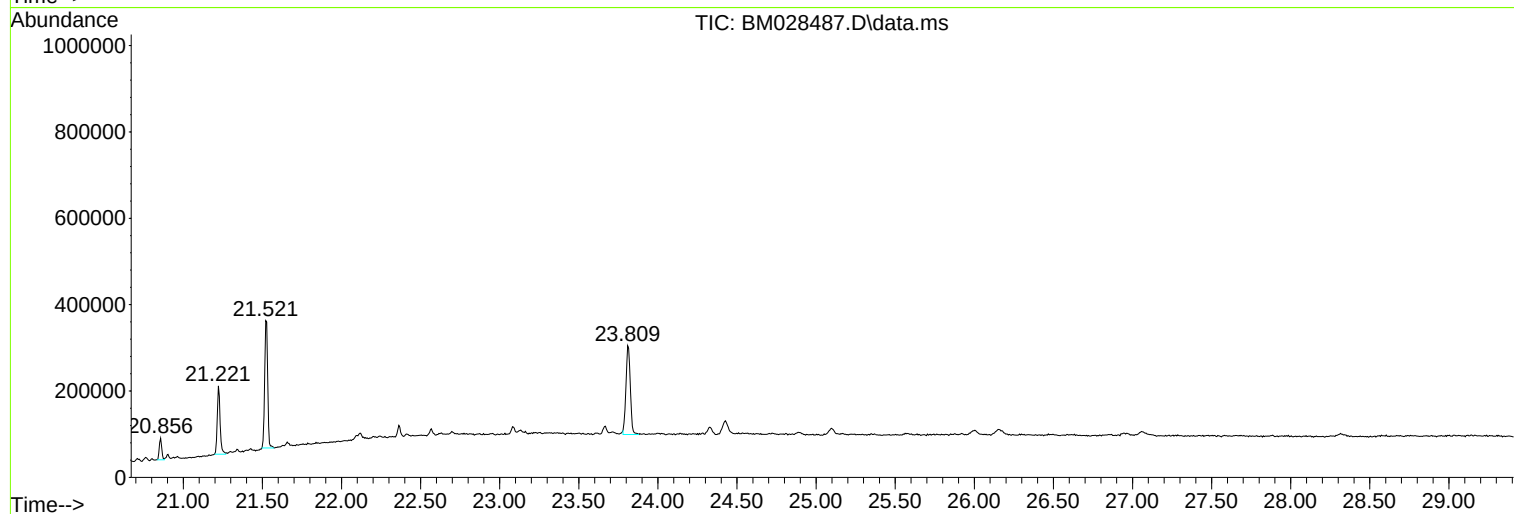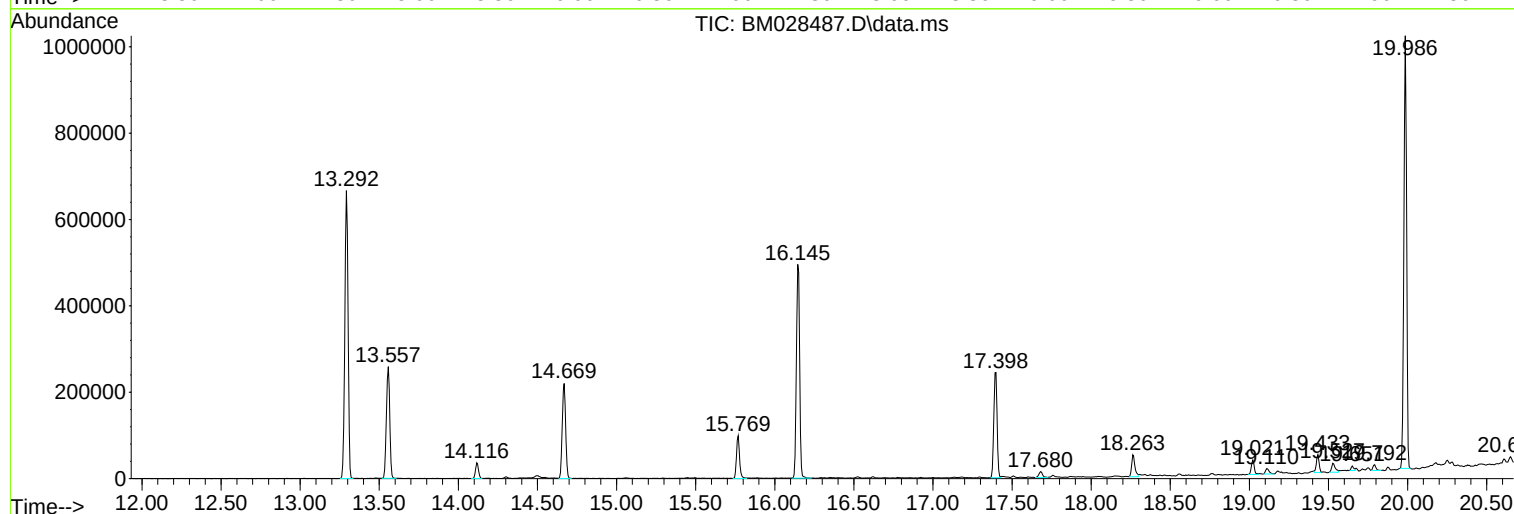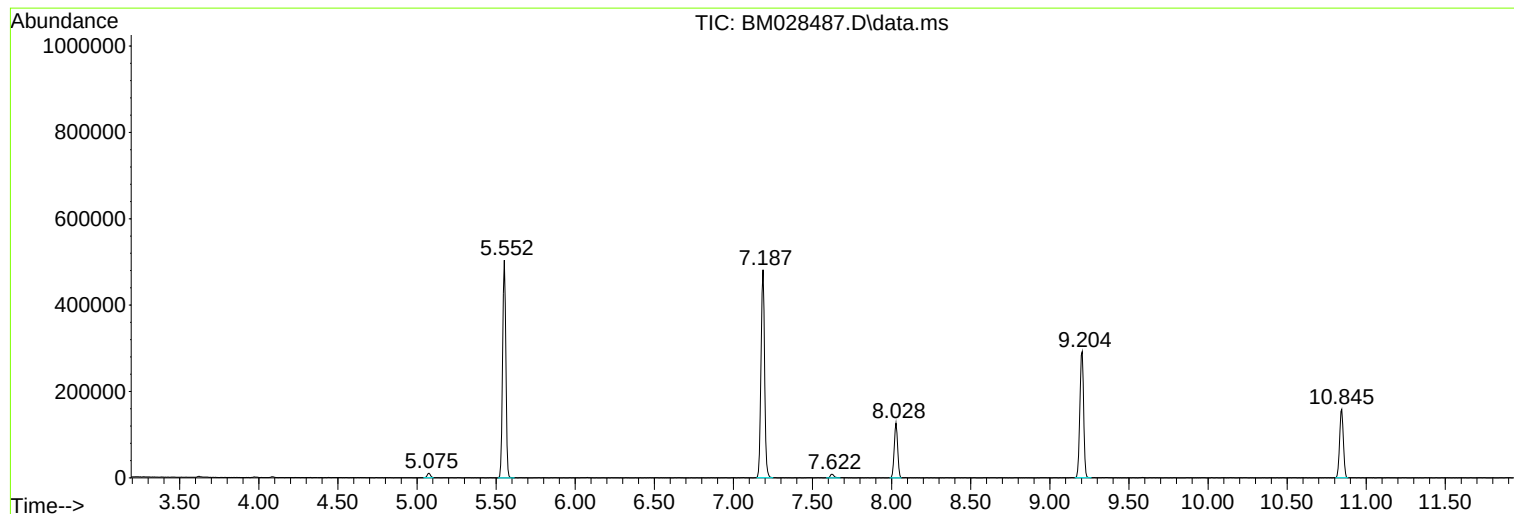

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012121\
Data File : BM028487.D
Acq On : 21 Jan 2021 13:54
Operator : CG/JU
Sample : M1082-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BACKFILL-ASHCROFT-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012121\
Data File : BM028487.D
Acq On : 21 Jan 2021 13:54
Operator : CG/JU
Sample : M1082-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BACKFILL-ASHCROFT-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------