

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012121\
 Data File : BM028488.D
 Acq On : 21 Jan 2021 14:30
 Operator : CG/JU
 Sample : M1082-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BACKFILL-ASHCROFT-02

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM028488.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.552	396	402	415	rVB	515959	748702	60.56%	10.010%
2	7.187	673	680	694	rVB	510687	799049	64.63%	10.683%
3	7.622	750	754	761	rBV	9883	14499	1.17%	0.194%
4	8.028	815	823	830	rBV	125871	192517	15.57%	2.574%
5	9.204	1013	1023	1030	rBV	312650	509828	41.24%	6.816%
6	10.845	1295	1302	1309	rVB	165925	269968	21.84%	3.609%
7	13.292	1711	1718	1724	rBV	736356	1012842	81.92%	13.541%
8	14.116	1853	1858	1865	rVB	46720	61477	4.97%	0.822%
9	14.669	1945	1952	1958	rVB	236888	330449	26.73%	4.418%
10	16.145	2197	2203	2213	rVB	541973	745758	60.32%	9.971%
11	16.474	2255	2259	2263	rBV	14039	17602	1.42%	0.235%
12	16.533	2263	2269	2275	rVV2	12020	24204	1.96%	0.324%
13	16.592	2275	2279	2282	rVV2	14029	19215	1.55%	0.257%
14	16.633	2282	2286	2291	rVB3	8213	14038	1.14%	0.188%
15	16.792	2308	2313	2319	rVB4	12009	21257	1.72%	0.284%
16	16.857	2319	2324	2329	rBV	14583	20261	1.64%	0.271%
17	17.398	2409	2416	2421	rBV	252224	354924	28.71%	4.745%
18	18.268	2558	2564	2574	rBV	52923	84320	6.82%	1.127%
19	19.527	2774	2778	2789	rBV4	18412	31940	2.58%	0.427%
20	19.798	2819	2824	2828	rBV2	26356	35771	2.89%	0.478%
21	19.986	2851	2856	2861	rBV	1056623	1236376	100.00%	16.530%
22	21.221	3062	3066	3075	rBV	129312	166777	13.49%	2.230%
23	21.527	3113	3118	3122	rBV	309807	388469	31.42%	5.194%
24	23.815	3501	3507	3514	rVB2	200674	379319	30.68%	5.071%




Sum of corrected areas: 7479562

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012121\
Data File : BM028488.D
Acq On : 21 Jan 2021 14:30
Operator : CG/JU
Sample : M1082-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BACKFILL-ASHCROFT-02

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

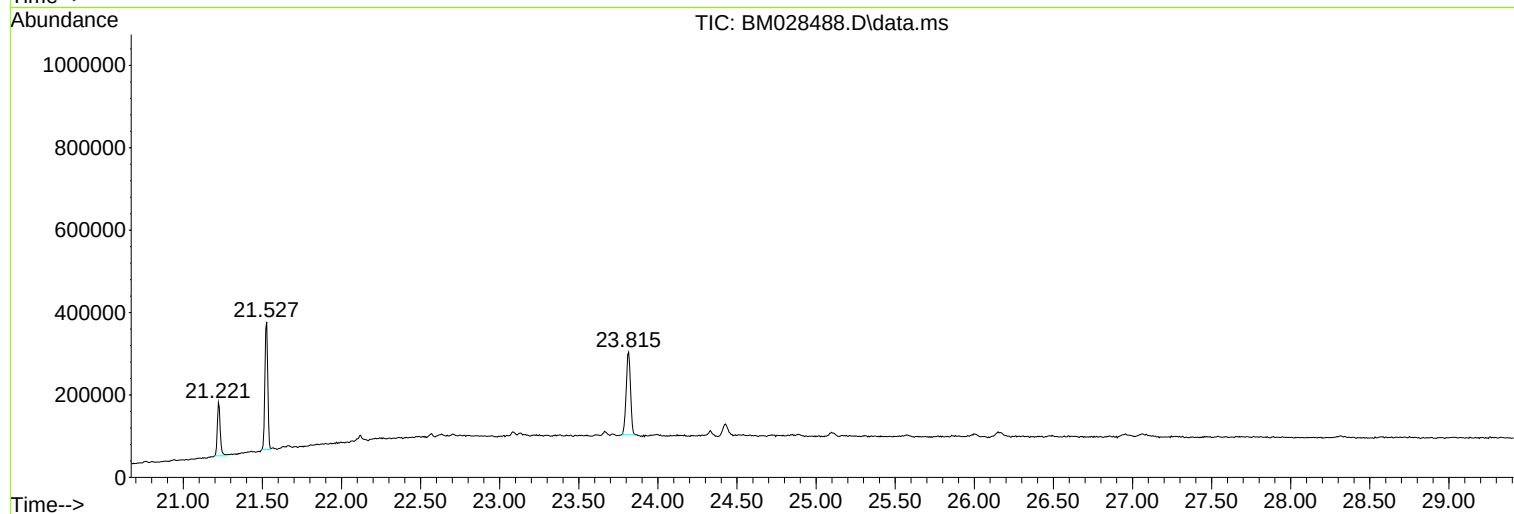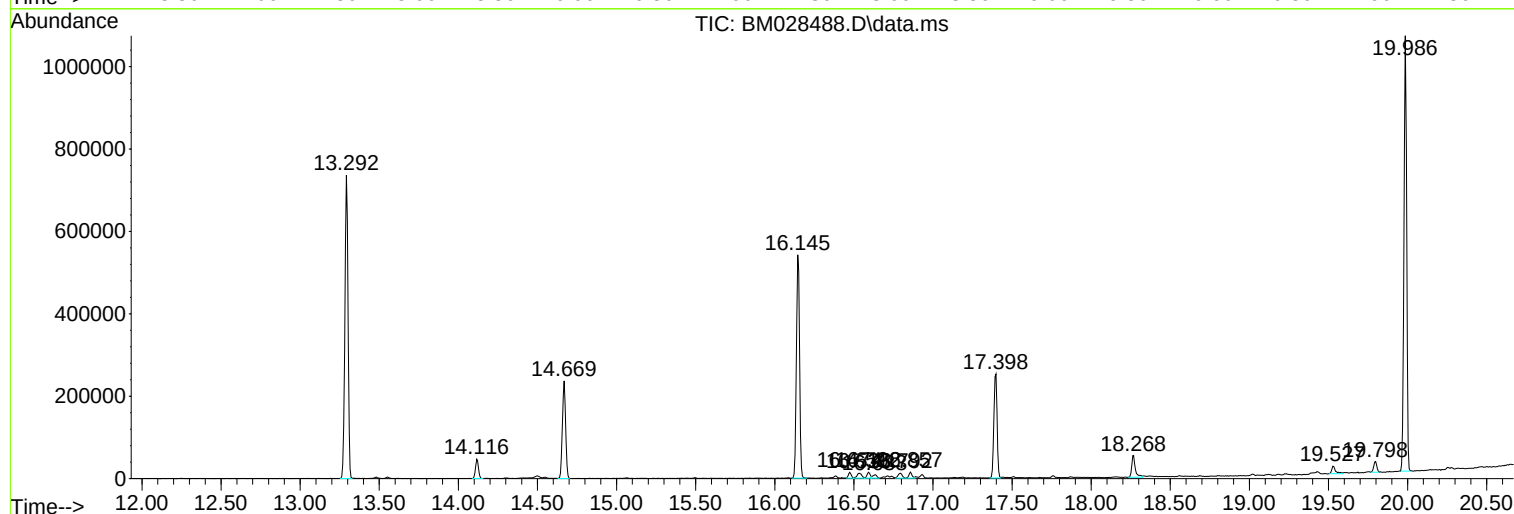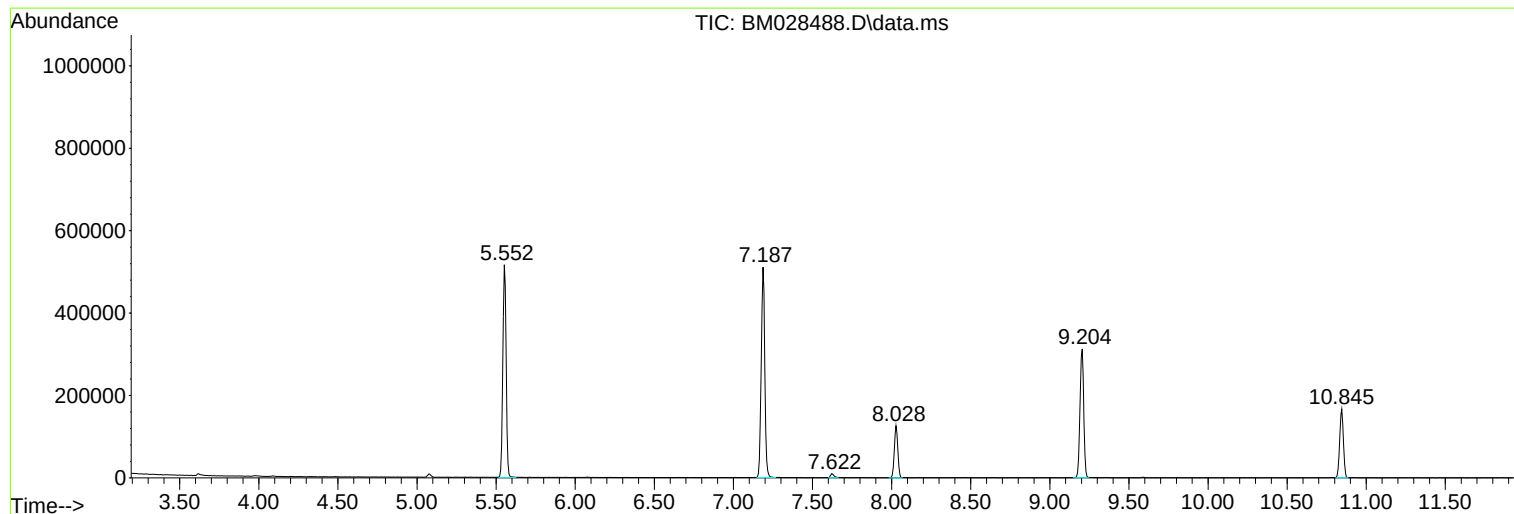

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012121\
Data File : BM028488.D
Acq On : 21 Jan 2021 14:30
Operator : CG/JU
Sample : M1082-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BACKFILL-ASHCROFT-02

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012121\
Data File : BM028488.D
Acq On : 21 Jan 2021 14:30
Operator : CG/JU
Sample : M1082-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BACKFILL-ASHCROFT-02

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------