


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012121\
 Data File : BM028478.D
 Acq On : 21 Jan 2021 08:18
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 22 10:45:04 2021

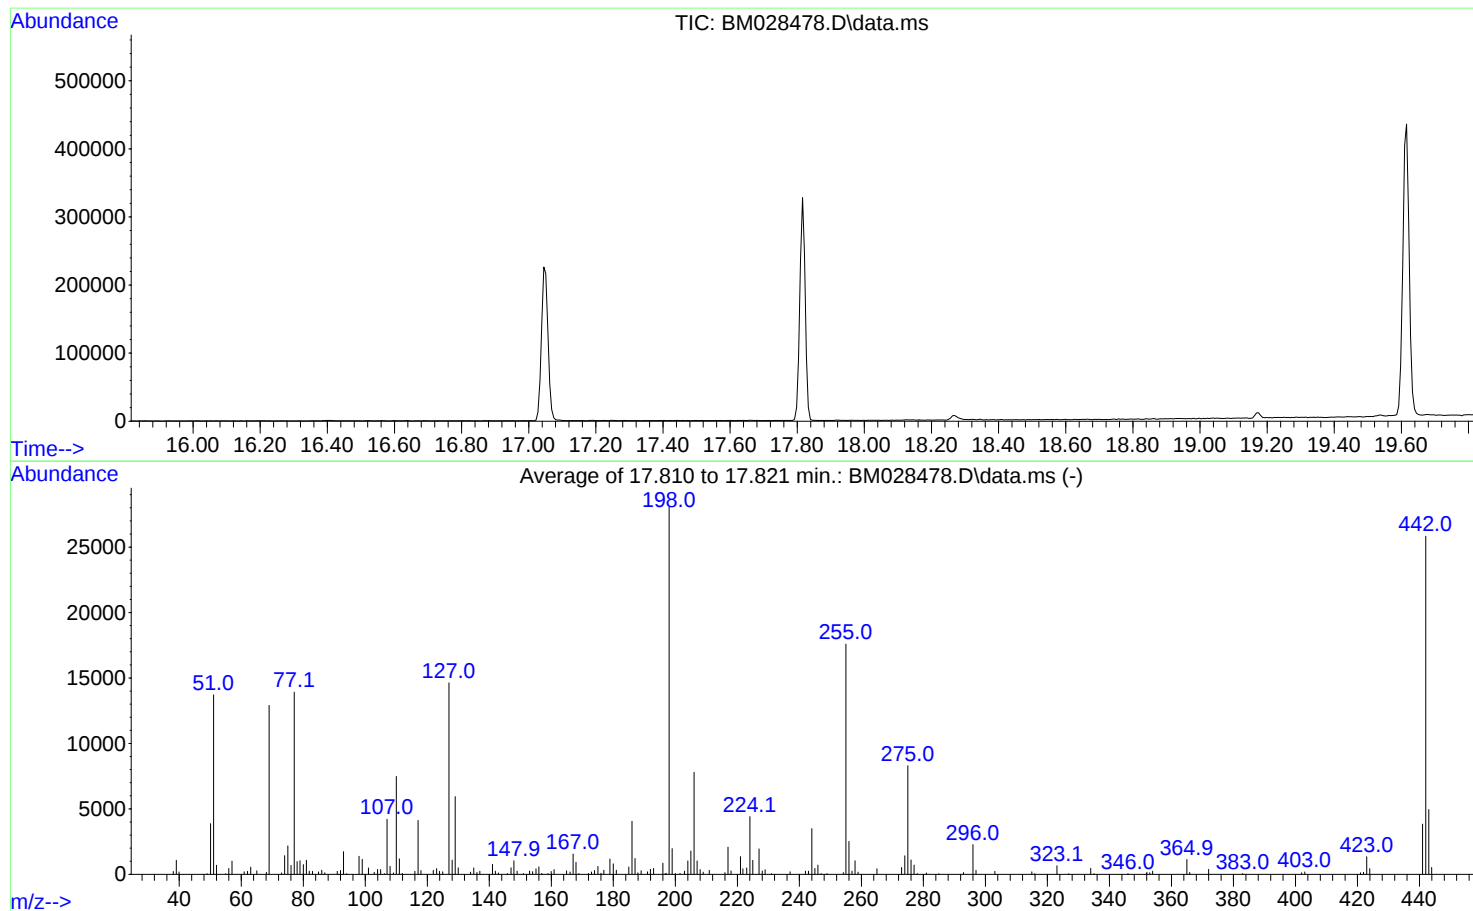

AutoFind: Scans 2486, 2487, 2488; Background Corrected with Scan 2480

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.8	13710	PASS
68	69	0.00	2	1.3	165	PASS
69	198	0.00	100	45.9	12907	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.1	14635	PASS
197	198	0.00	2	0.3	88	PASS
198	198	100	100	100.0	28099	PASS
199	198	5	9	7.0	1966	PASS
275	198	10	60	29.5	8302	PASS
365	198	1	100	4.0	1134	PASS
441	198	0.01	100	13.7	3844	PASS
442	198	50	100	91.9	25829	PASS
443	442	15	24	19.2	4947	PASS