


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012121\
 Data File : BM028490.D
 Acq On : 21 Jan 2021 16:13
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 22 10:45:04 2021

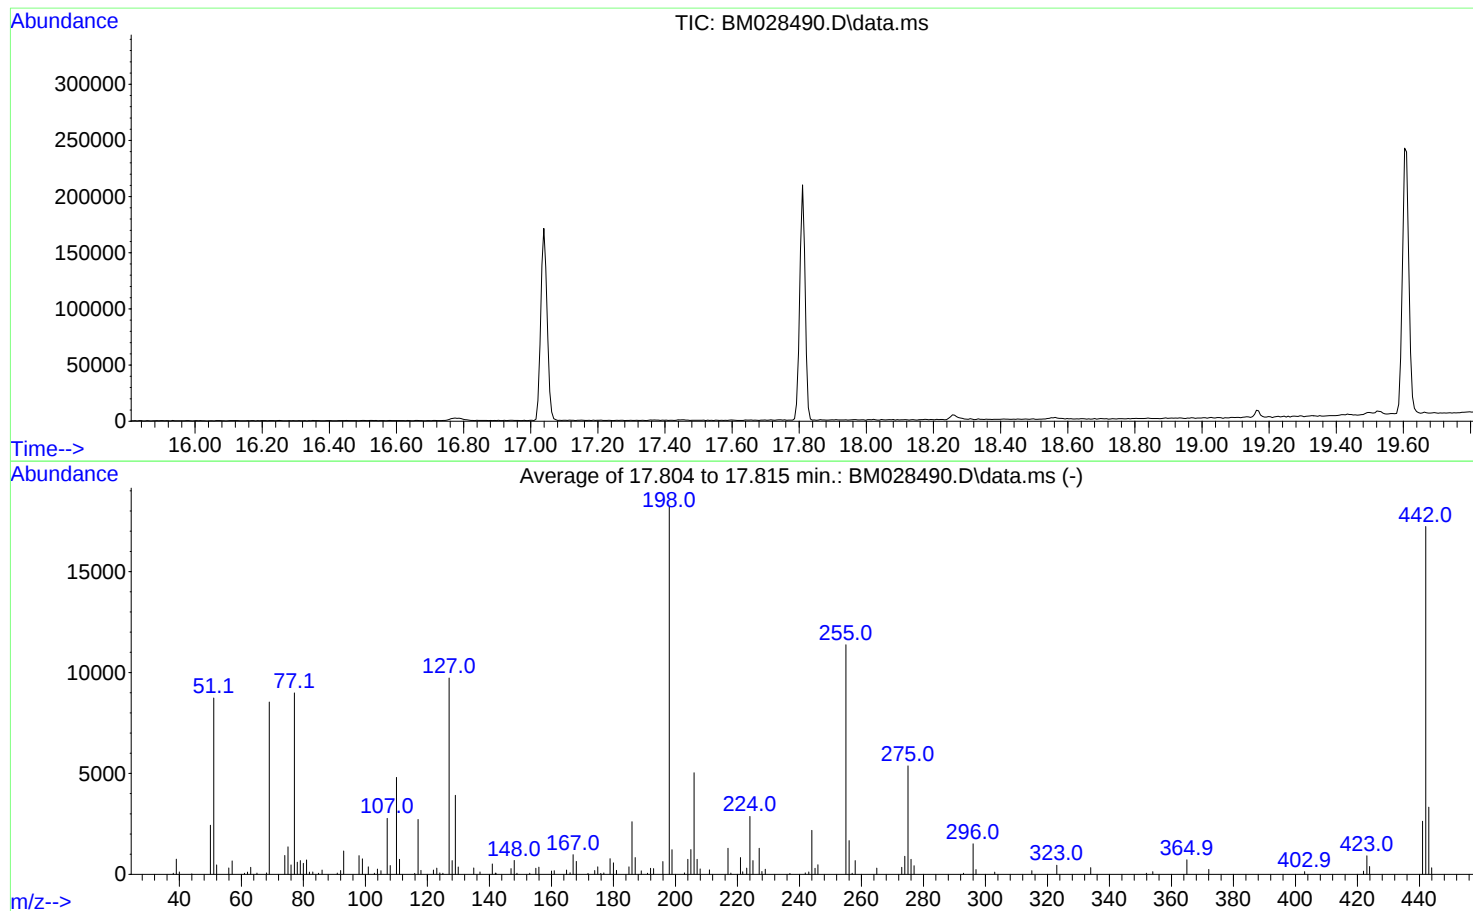

AutoFind: Scans 2485, 2486, 2487; Background Corrected with Scan 2479

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.9	8732	PASS
68	69	0.00	2	0.8	72	PASS
69	198	0.00	100	46.8	8536	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.4	9729	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	18225	PASS
199	198	5	9	6.7	1222	PASS
275	198	10	60	29.5	5371	PASS
365	198	1	100	4.0	723	PASS
441	198	0.01	100	14.4	2629	PASS
442	198	50	100	94.6	17234	PASS
443	442	15	24	19.3	3332	PASS