

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012125\
 Data File : BM049360.D
 Acq On : 21 Jan 2025 11:12
 Operator : RC/JU
 Sample : PB166143BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK143

Quant Time: Jan 21 22:48:23 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM011725.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 17 15:40:55 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.527	152	4965	0.400	ng/ul	0.00
4) Naphthalene-d8	10.282	136	13540	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.164	164	6858	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.010	188	1060319	0.400	ng/ul	0.09
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.13
23) Perylene-d12	23.267	264	18184	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.126	96	34312	5.938	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.904	152	5312	0.308	ng/ul	0.01
18) Fluoranthene-d10	18.956	212	10175	0.000	ng/ul	0.00
Target Compounds						
						Qvalue
12) Fluorene	15.164	166	2001	0.096	ng/ul#	16
26) Benzo(a)pyrene	23.130	252	4114	0.076	ng/ul#	76


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012125\
Data File : BM049360.D
Acq On : 21 Jan 2025 11:12
Operator : RC/JU
Sample : PB166143BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK143

Quant Time: Jan 21 22:48:23 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM011725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 17 15:40:55 2025
Response via : Initial Calibration

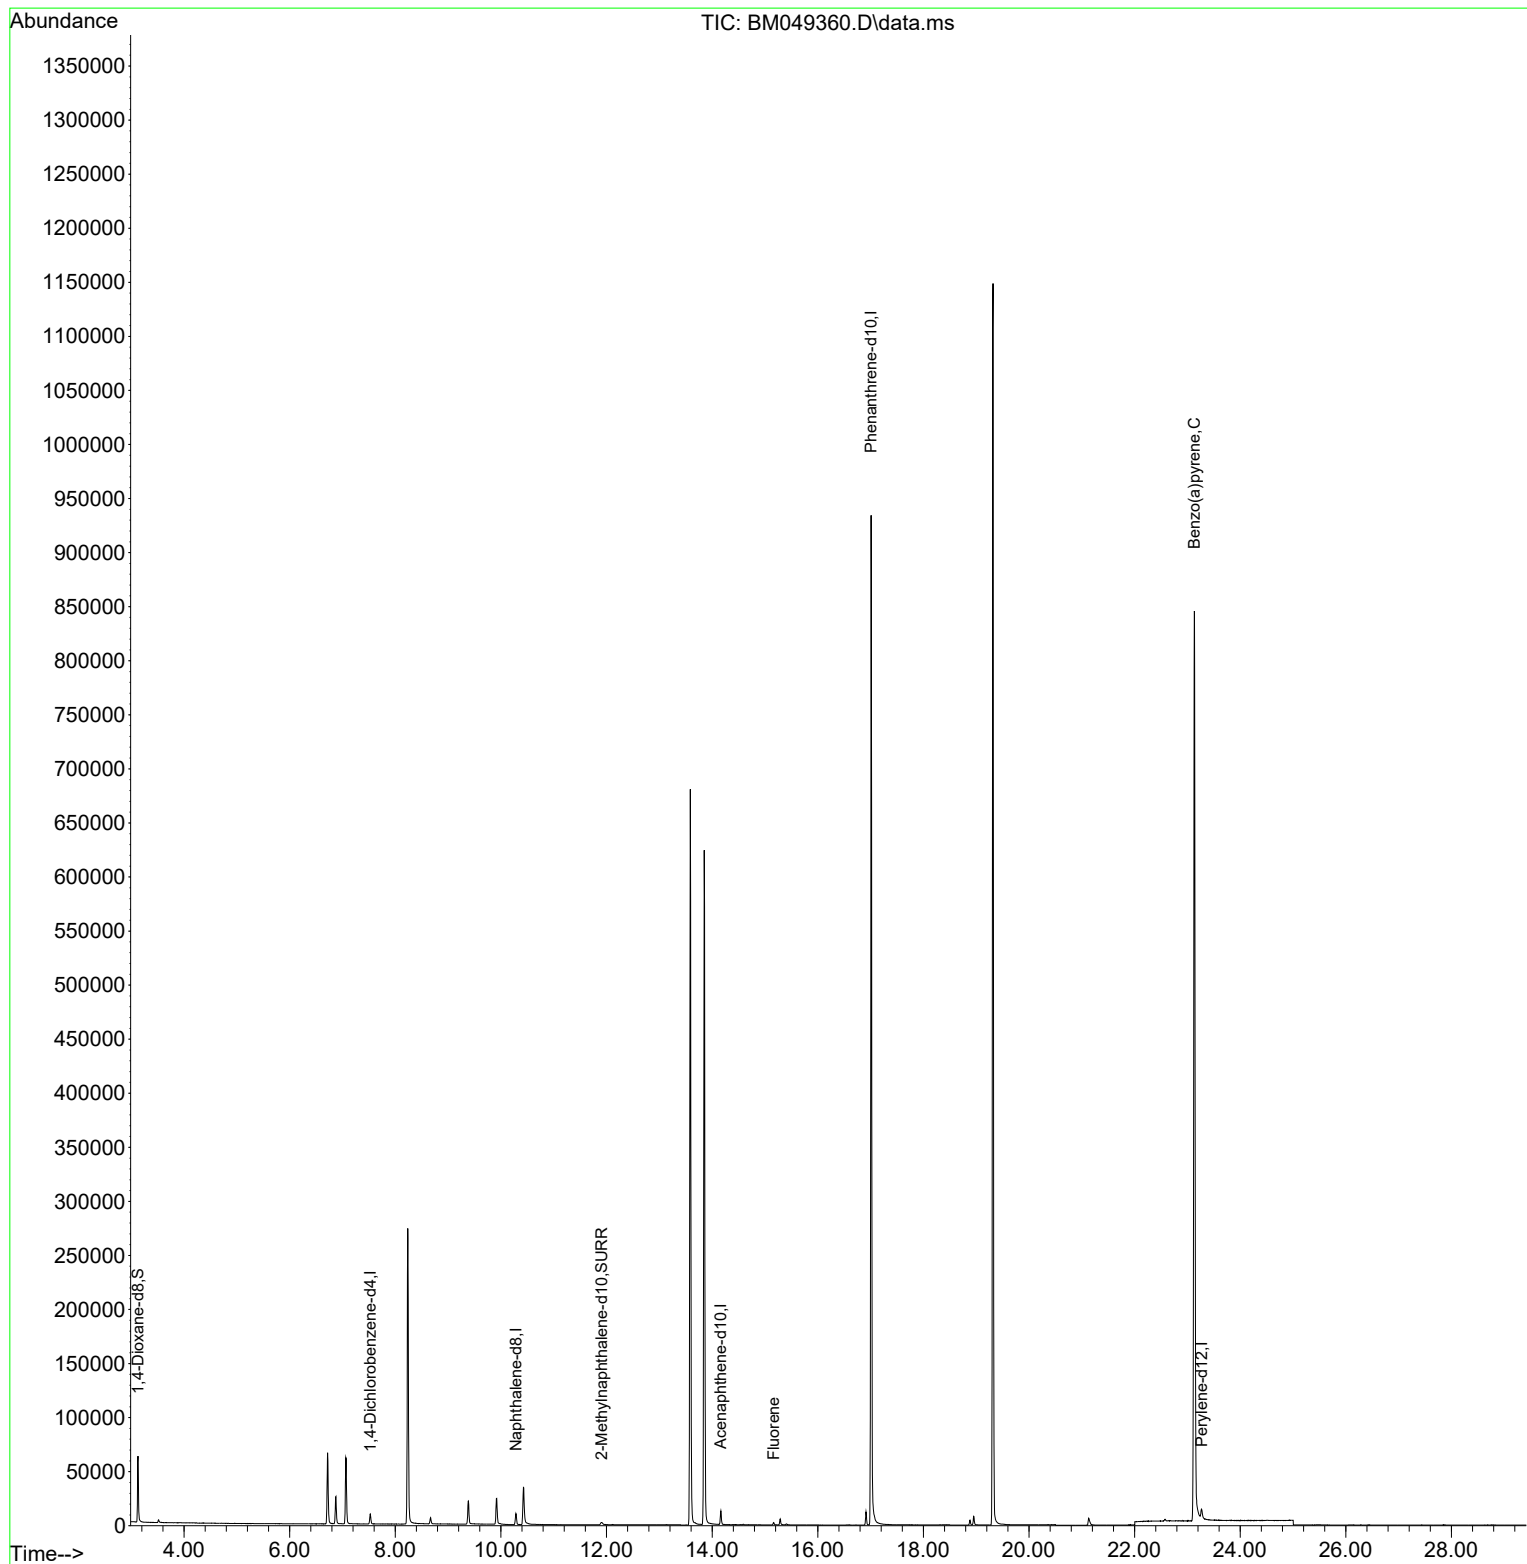

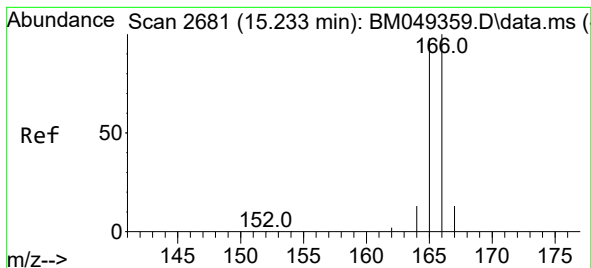

#12

Fluorene

Concen: 0.096 ng/ul

RT: 15.164 min Scan# 2

Delta R.T. -0.068 min

Lab File: BM049360.D

Acq: 21 Jan 2025 11:12

Instrument :

BNA_M

ClientSampleId :

SBLK143





Tgt Ion:166 Resp: 2001

Ion Ratio Lower Upper

166 100

165 10.0 79.2 118.8#

167 32.2 11.2 16.8#

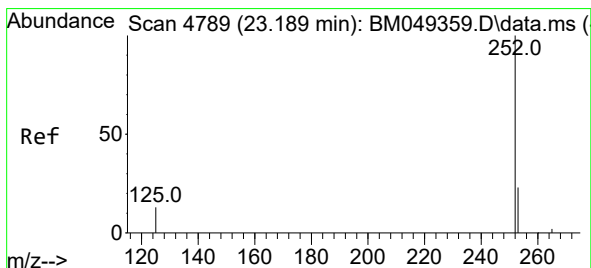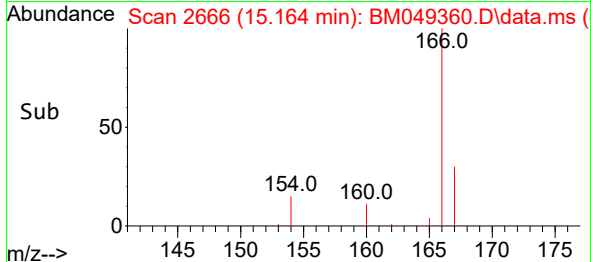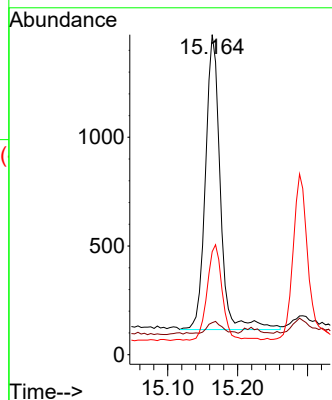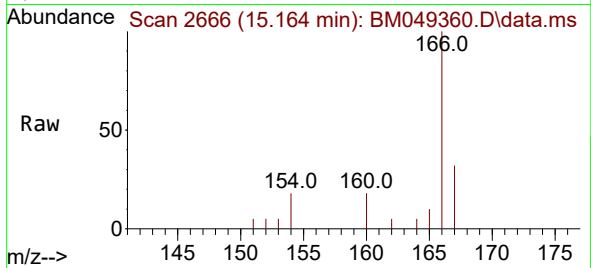

#26

Benzo(a)pyrene

Concen: 0.076 ng/ul

RT: 23.130 min Scan# 4769

Delta R.T. -0.056 min

Lab File: BM049360.D

Acq: 21 Jan 2025 11:12

Tgt Ion:252 Resp: 4114

Ion Ratio Lower Upper

252 100

253 44.4 24.8 37.2#

125 31.0 16.1 24.1#

