

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012125\
 Data File : BM049361.D
 Acq On : 21 Jan 2025 11:48
 Operator : RC/JU
 Sample : Q1126-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AF2

Quant Time: Jan 21 22:48:30 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM011725.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 17 15:40:55 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.527	152	5386	0.400	ng/ul	0.00
4) Naphthalene-d8	10.282	136	15635	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.164	164	8362	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.010	188	1485720	0.400	ng/ul	0.09
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.13
23) Perylene-d12	23.264	264	17740	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.126	96	32051	5.113	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.888	152	7034	0.354	ng/ul	0.00
18) Fluoranthene-d10	18.951	212	15899	0.000	ng/ul	0.00
Target Compounds						
					Qvalue	
26) Benzo(a)pyrene	23.130	252	3779	0.072	ng/ul#	70


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012125\
Data File : BM049361.D
Acq On : 21 Jan 2025 11:48
Operator : RC/JU
Sample : Q1126-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF2


Quant Time: Jan 21 22:48:30 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM011725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 17 15:40:55 2025
Response via : Initial Calibration

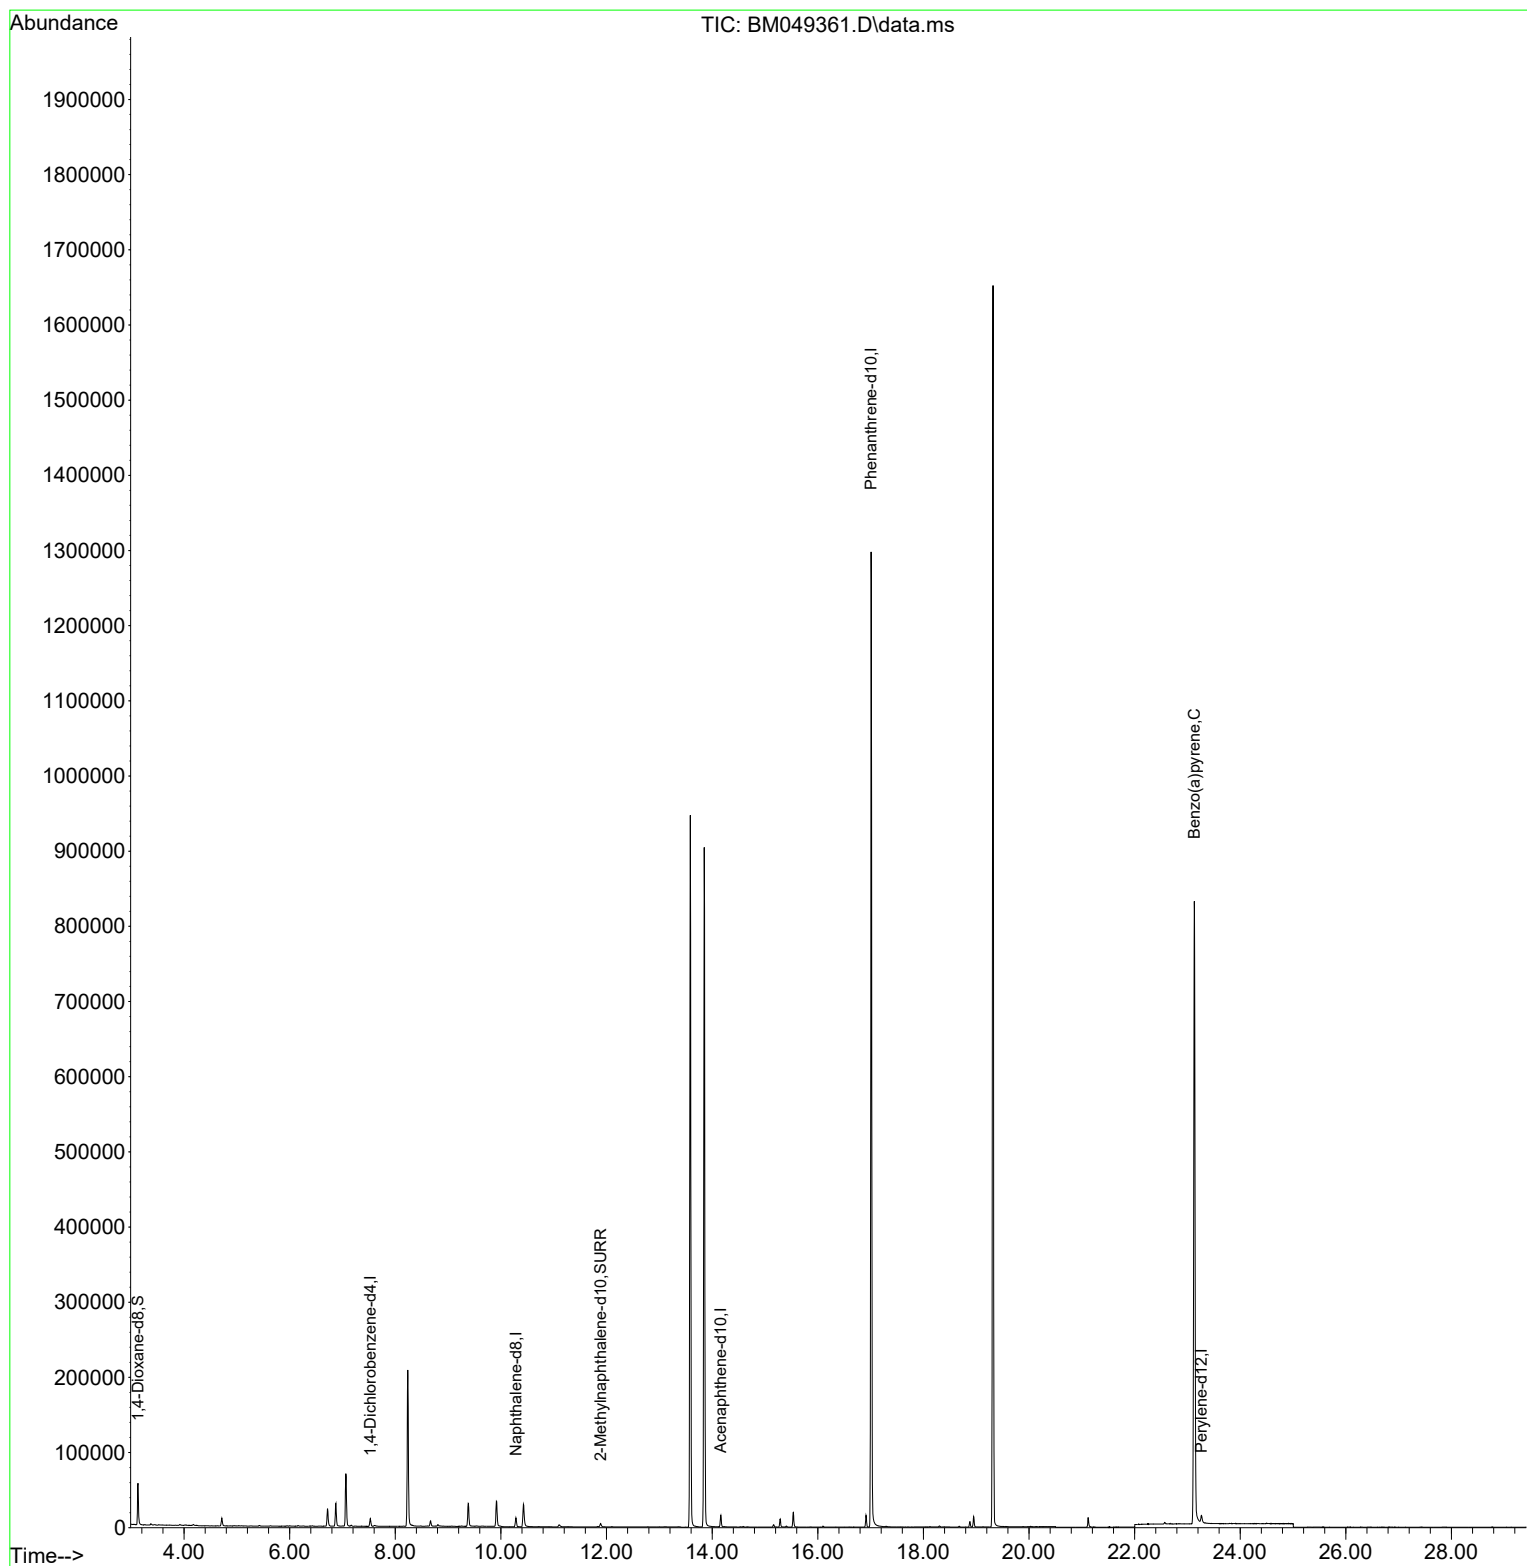

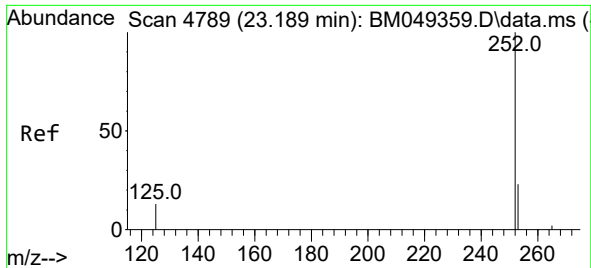

#26
Benzo(a)pyrene
Concen: 0.072 ng/ul
RT: 23.130 min Scan# 41
Delta R.T. -0.056 min
Lab File: BM049361.D
Acq: 21 Jan 2025 11:48

Instrument :
BNA_M
ClientSampleId :
C0AF2

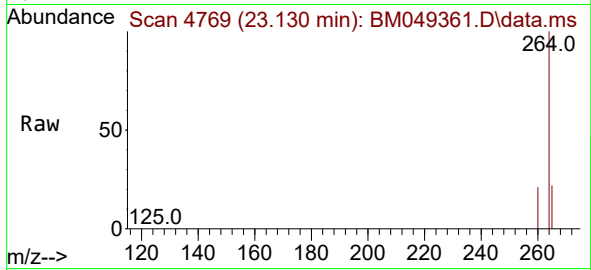

Tgt Ion:252 Resp: 3779
Ion Ratio Lower Upper
252 100
253 47.4 24.8 37.2#
125 34.6 16.1 24.1#

