

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012125\
 Data File : BM049362.D
 Acq On : 21 Jan 2025 12:23
 Operator : RC/JU
 Sample : Q1126-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AF3

Quant Time: Jan 21 22:48:36 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM011725.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 17 15:40:55 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.527	152	6018	0.400	ng/ul	0.00
4) Naphthalene-d8	10.282	136	17601	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.164	164	9144	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.010	188	1502446	0.400	ng/ul	0.09
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.13
23) Perylene-d12	23.265	264	18710	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.126	96	34993	4.996	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.888	152	7768	0.347	ng/ul	0.00
18) Fluoranthene-d10	18.951	212	16140	0.000	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.160	88	18741	2.377	ng/ul#	86
26) Benzo(a)pyrene	23.130	252	4659	0.084	ng/ul#	77


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012125\
Data File : BM049362.D
Acq On : 21 Jan 2025 12:23
Operator : RC/JU
Sample : Q1126-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF3

Quant Time: Jan 21 22:48:36 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM011725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 17 15:40:55 2025
Response via : Initial Calibration




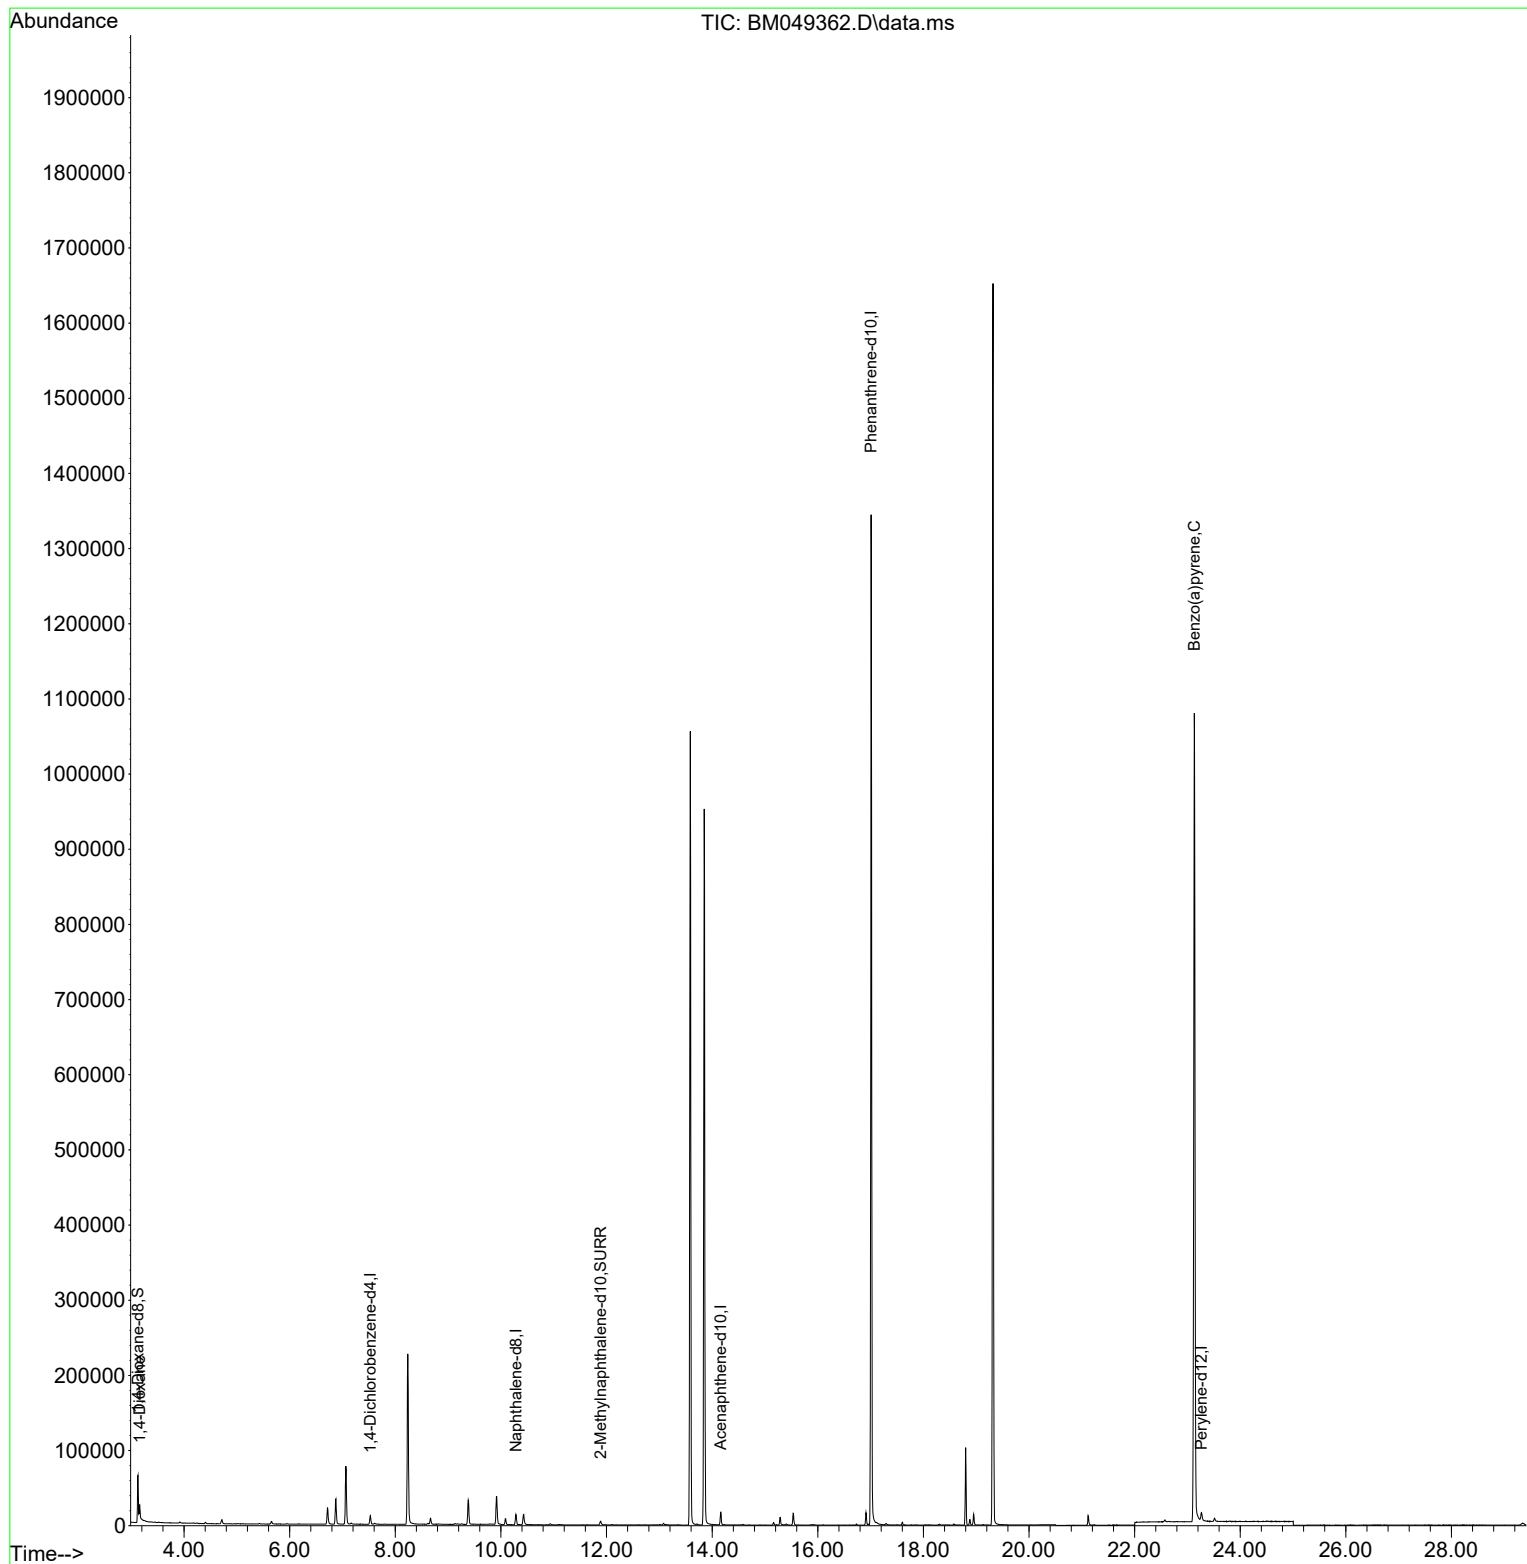


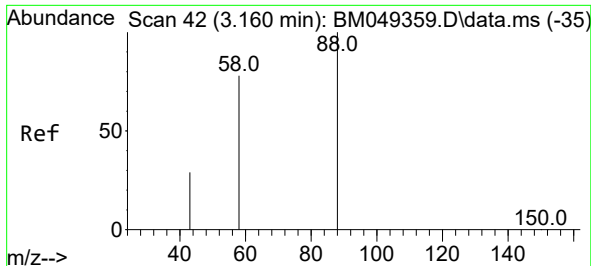

#2
1,4-Dioxane
Concen: 2.377 ng/ul
RT: 3.160 min Scan# 41
Delta R.T. -0.000 min
Lab File: BM049362.D
Acq: 21 Jan 2025 12:23

Instrument :
BNA_M
ClientSampleId :
C0AF3

Tgt Ion: 88 Resp: 18741
Ion Ratio Lower Upper
88 100
43 30.5 26.2 39.2
58 65.9 41.4 62.0#

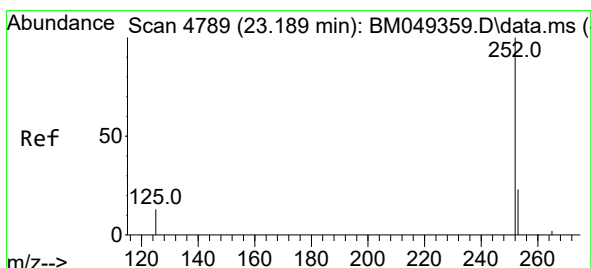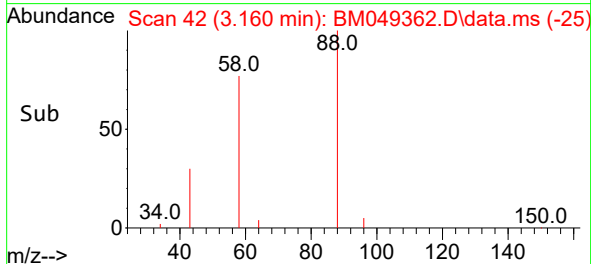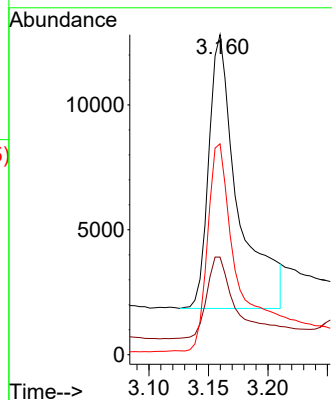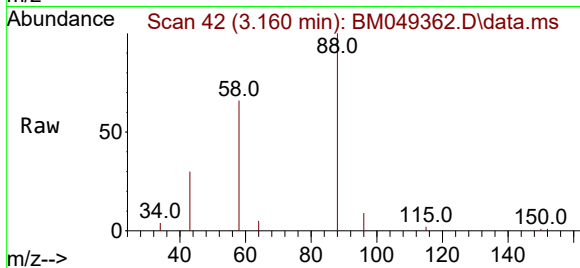

#26
Benzo(a)pyrene
Concen: 0.084 ng/ul
RT: 23.130 min Scan# 4769
Delta R.T. -0.056 min
Lab File: BM049362.D
Acq: 21 Jan 2025 12:23

Tgt Ion: 252 Resp: 4659
Ion Ratio Lower Upper
252 100
253 43.9 24.8 37.2#
125 30.0 16.1 24.1#

