

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012125\
 Data File : BM049363.D
 Acq On : 21 Jan 2025 12:59
 Operator : RC/JU
 Sample : Q1126-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AF4

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 01/22/2025
 Supervised By :mohammad ahmed 01/22/2025

Quant Time: Jan 21 22:48:43 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM011725.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 17 15:40:55 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.527	152	4857	0.400	ng/u1	0.00
4) Naphthalene-d8	10.282	136	14073	0.400	ng/u1	0.00
9) Acenaphthene-d10	14.164	164	7753	0.400	ng/u1	0.00
13) Phenanthrene-d10	16.913	188	16673m	0.400	ng/u1	-0.01
17) Chrysene-d12	21.119	240	13111m	0.400	ng/u1	0.00
23) Perylene-d12	23.267	264	11097m	0.400	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.126	96	29821	5.276	ng/u1	0.00
6) 2-Methylnaphthalene-d10	11.882	152	7076	0.395	ng/u1	0.00
18) Fluoranthene-d10	18.951	212	16577m	0.370	ng/u1	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.159	88	5548m	0.872	ng/u1	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012125\
Data File : BM049363.D
Acq On : 21 Jan 2025 12:59
Operator : RC/JU
Sample : Q1126-03
Misc :
ALS Vial : 6 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
C0AF4

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/22/2025
Supervised By :mohammad ahmed 01/22/2025


Quant Time: Jan 21 22:48:43 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM011725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 17 15:40:55 2025
Response via : Initial Calibration

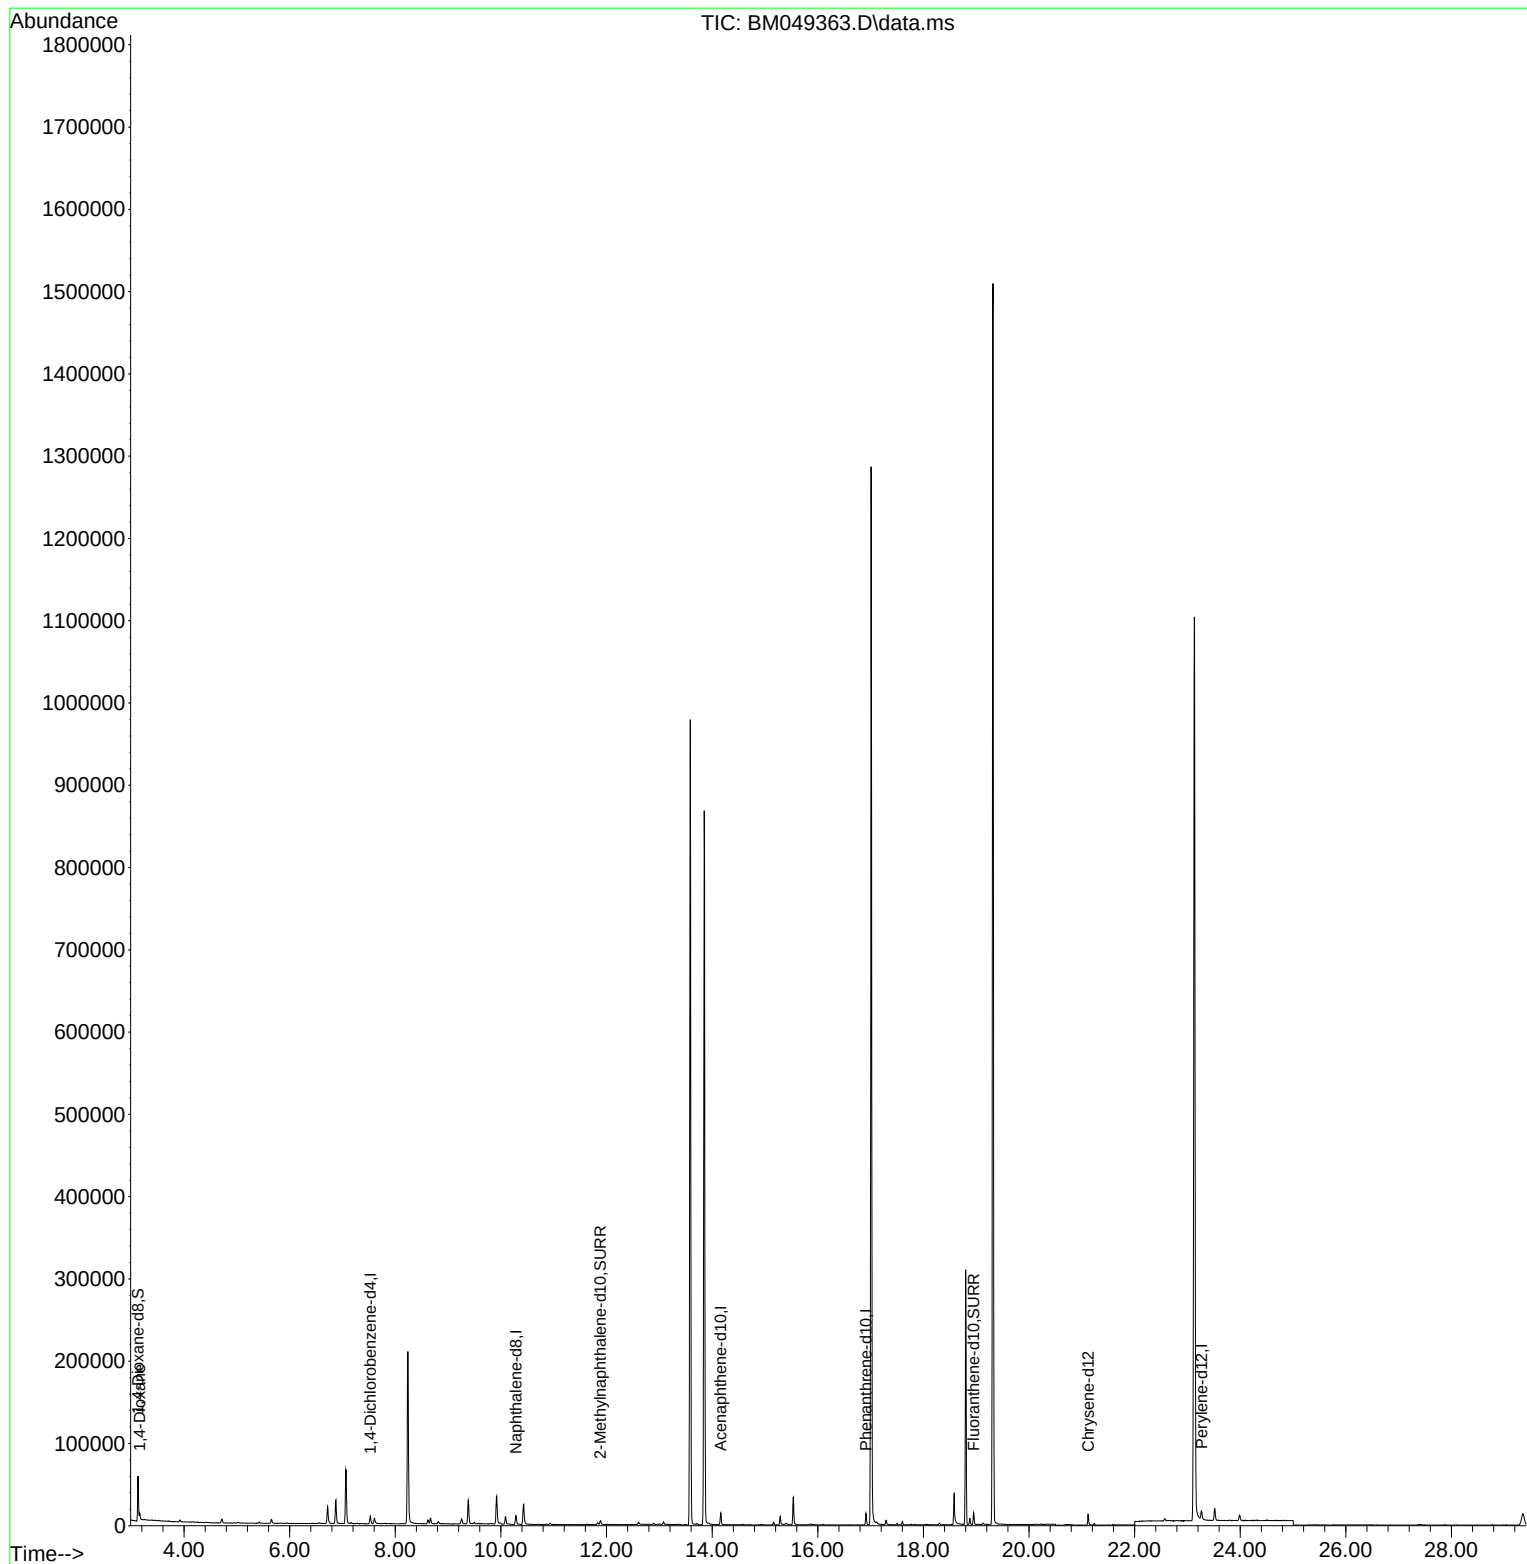

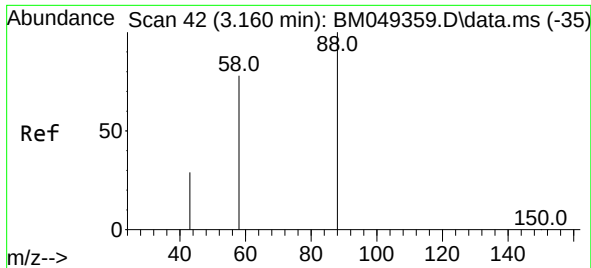

#2
 1,4-Dioxane
 Concen: 0.872 ng/ul m
 RT: 3.159 min Scan# 43
 Delta R.T. -0.000 min
 Lab File: BM049363.D
 Acq: 21 Jan 2025 12:59

Instrument :
 BNA_M
 ClientSampleId :
 C0AF4

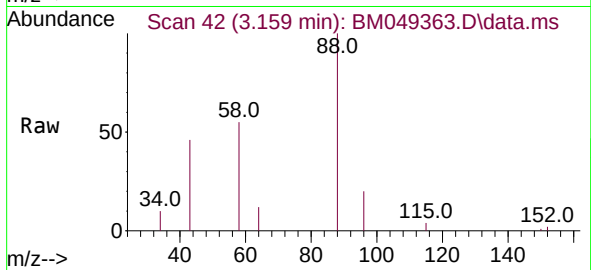

Tgt Ion: 88 Resp: 5548
 Ion Ratio Lower Upper
 88 100
 43 46.0 26.2 39.2
 58 55.5 41.4 62.0

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 01/22/2025
 Supervised By :mohammad ahmed 01/22/2025

