
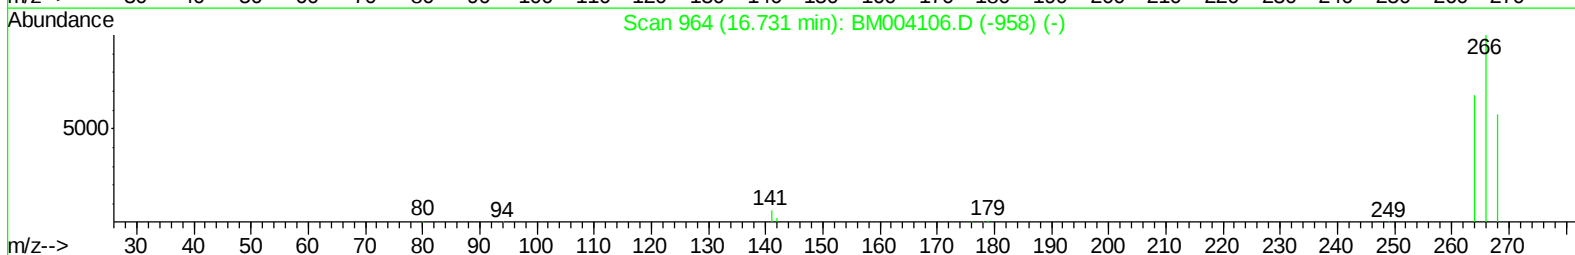
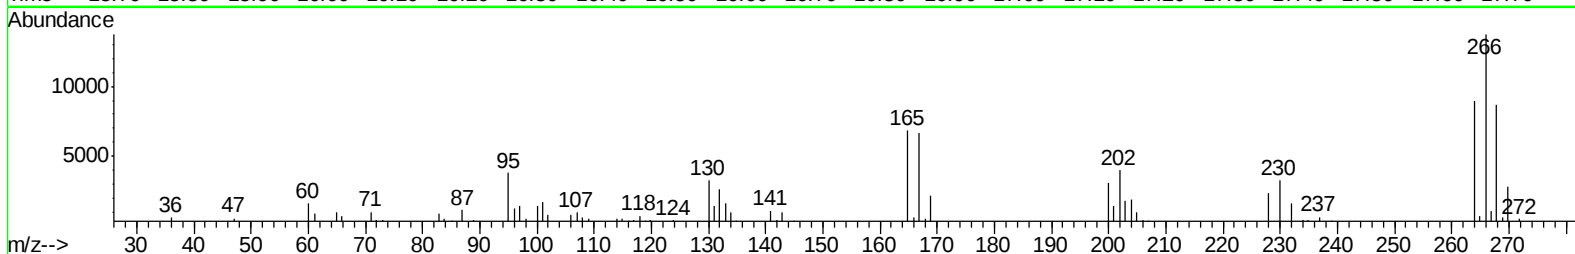


Data Path : Z:\HPCHEM1\BNA M\DATA\BM012216\
Data File : BM004101.D
Acq On : 22 Jan 2016 09:17
Operator : SJ/UM
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 22 09:52:44 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-SIM-BM010216.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 04 13:33:21 2016
Response via : Initial Calibration

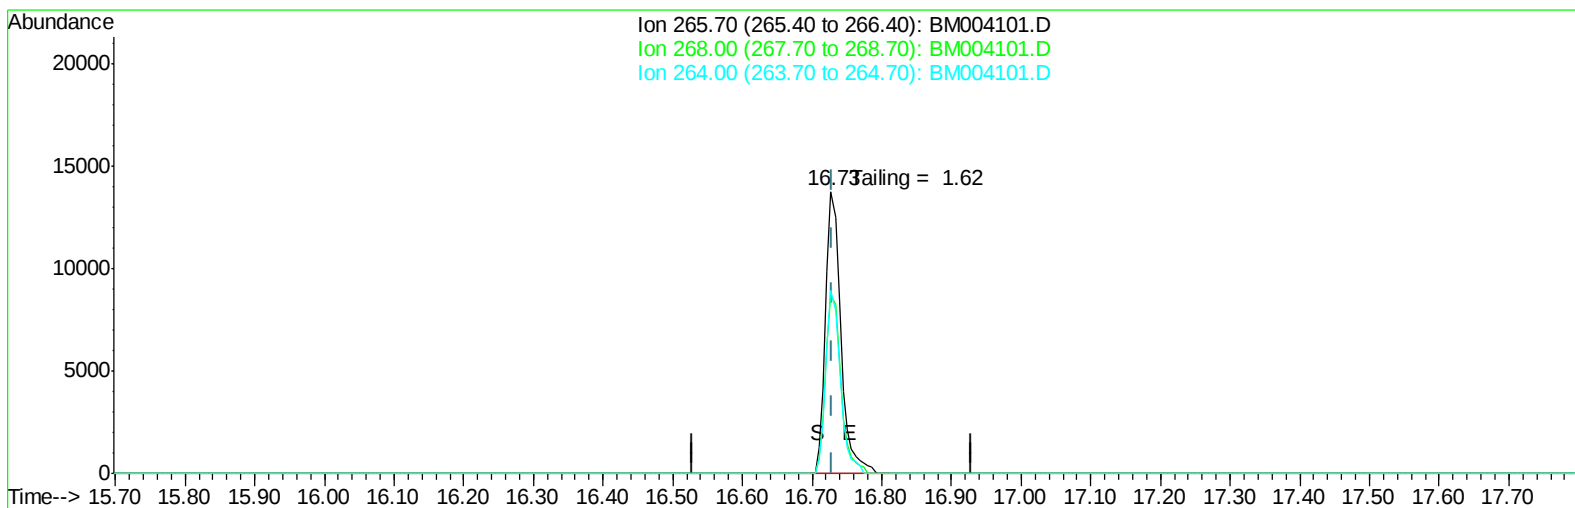

TIC: BM004101.D

(22) Pentachlorophenol




16.727min (-0.003) 0.00ng

response 21117

Ion	Exp%	Act%
265.70	100	100
268.00	78.40	63.35
264.00	57.10	65.16
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA M\DATA\BM012216\
Data File : BM004101.D
Acq On : 22 Jan 2016 09:17
Operator : SJ/UM
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 22 09:52:44 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-SIM-BM010216.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 04 13:33:21 2016
Response via : Initial Calibration

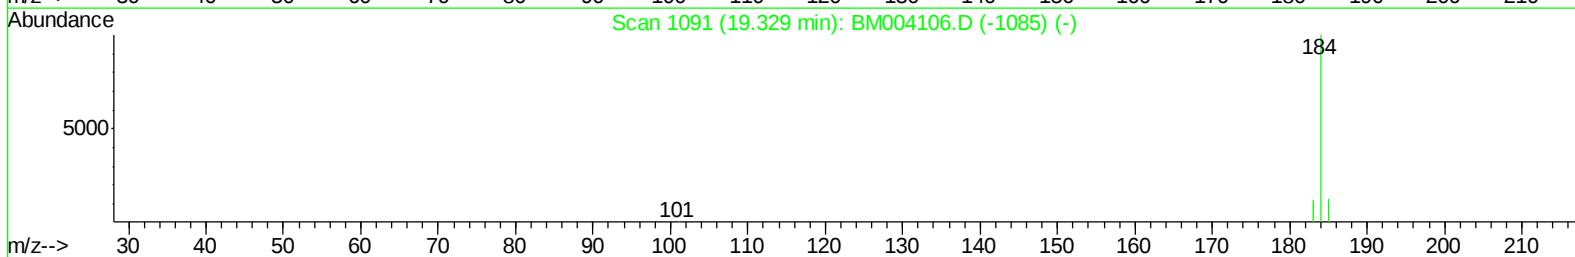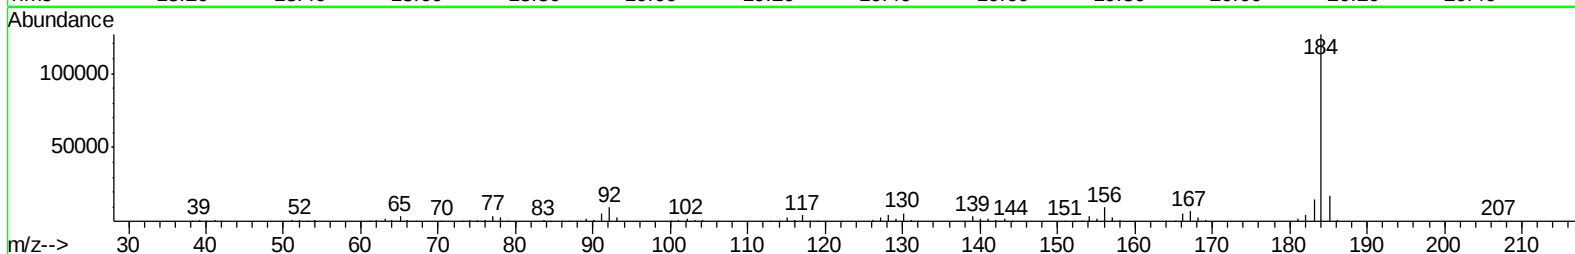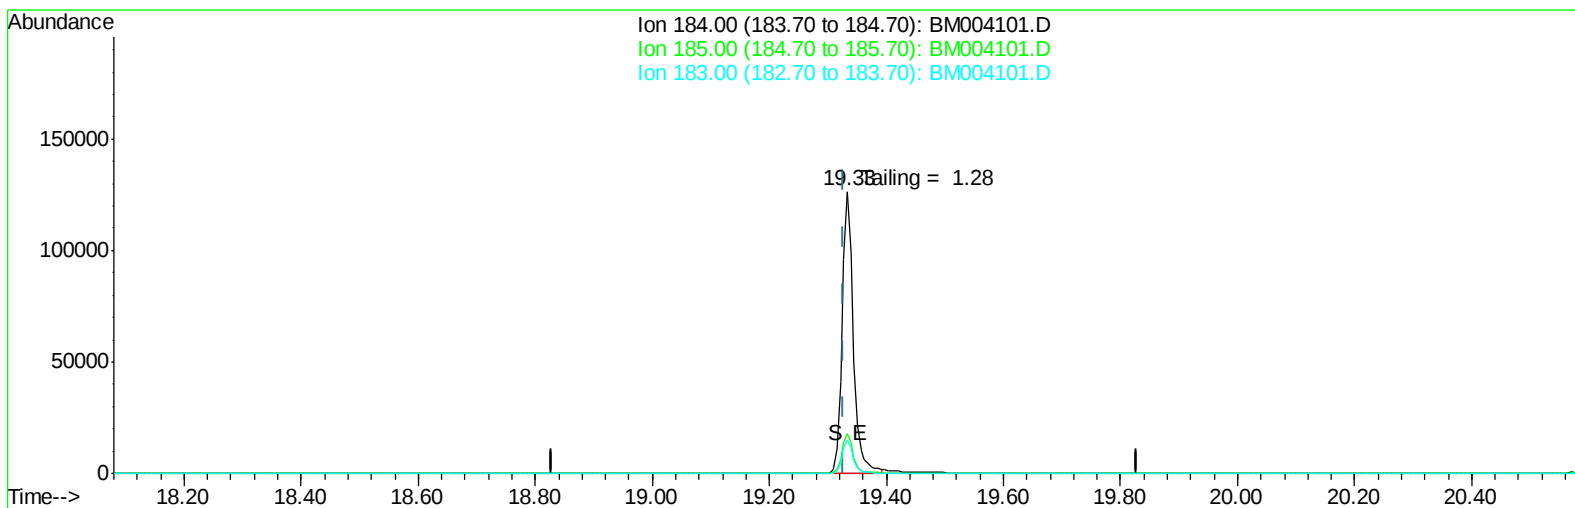

TIC: BM004101.D

(27) Benzidine

19.333min (+0.005) 0.00ng

response 173255

Ion	Exp%	Act%
184.00	100	100
185.00	16.50	14.04
183.00	11.30	11.66
0.00	0.00	0.00