
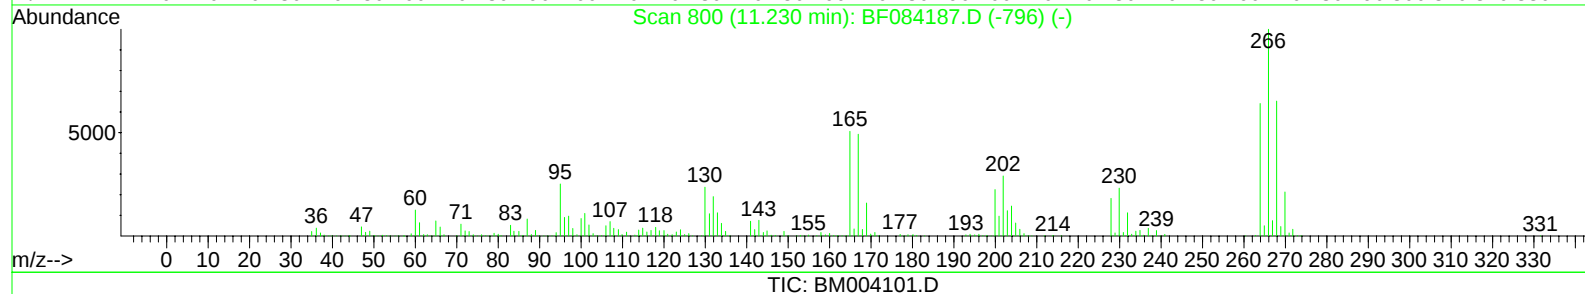
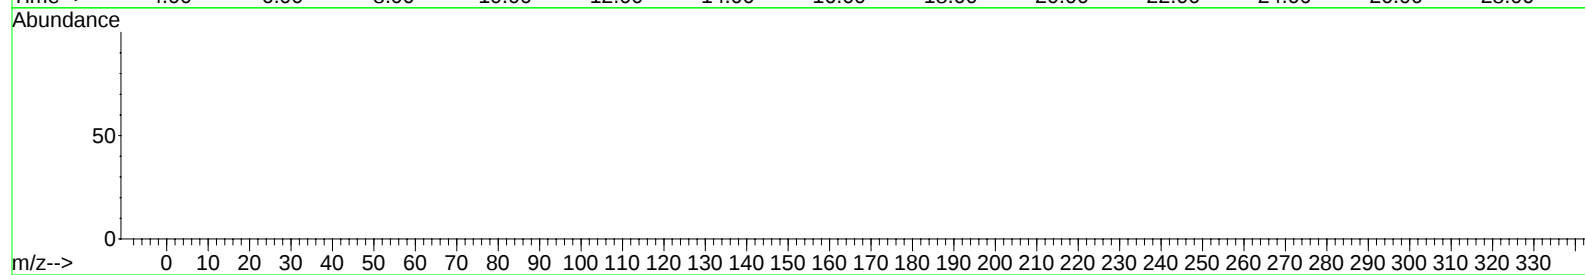


Data Path : Z:\HPCHEM1\BNA M\Data\BM012216\
Data File : BM004101.D
Acq On : 21 Jan 2016 14:52
Operator : SJ/UM
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 22 06:12:49 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF123115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 14 14:15:52 2016
Response via : Initial Calibration

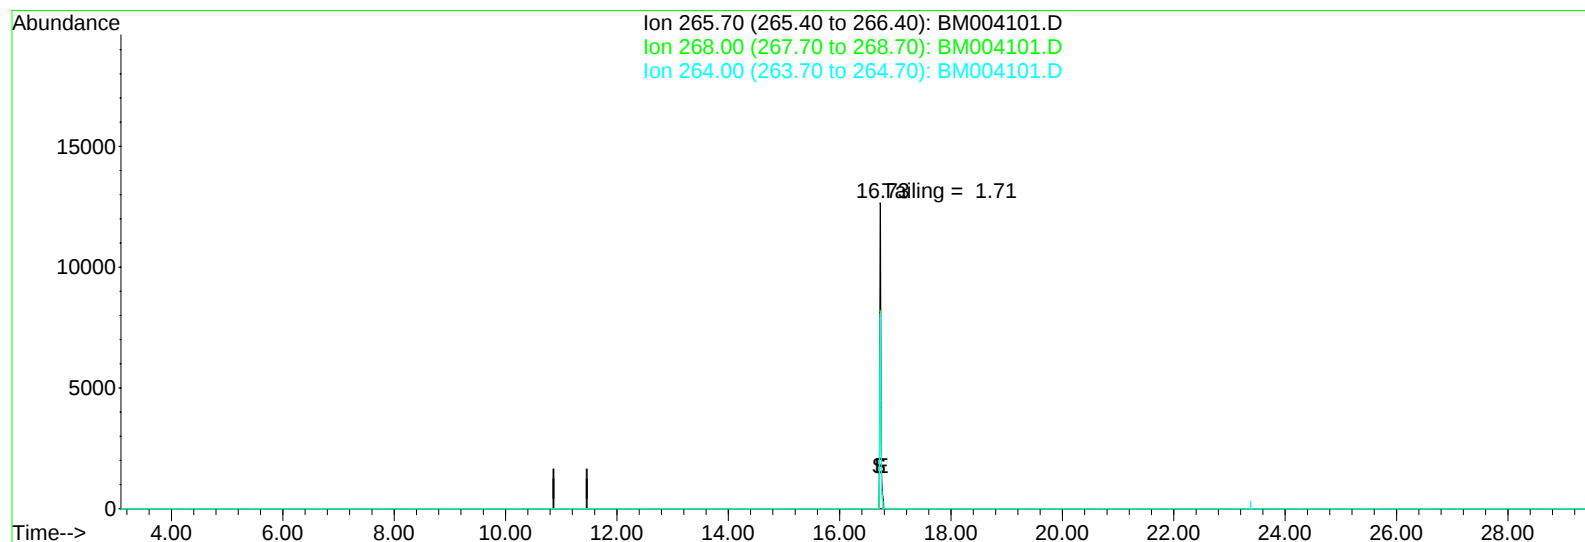

(69) Pentachlorophenol (C)




11.162min (-11.162) 0.00ng

response 0

Ion	Exp%	Act%
265.70	100	0.00
268.00	65.50	0.00#
264.00	62.70	0.00#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA M\Data\BM012216\
Data File : BM004101.D
Acq On : 21 Jan 2016 14:52
Operator : SJ/UM
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 22 06:12:49 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF123115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 14 14:15:52 2016
Response via : Initial Calibration

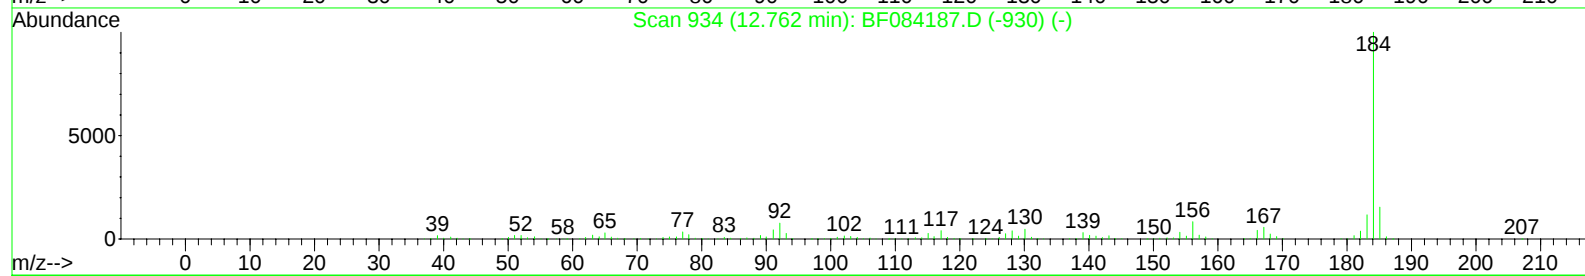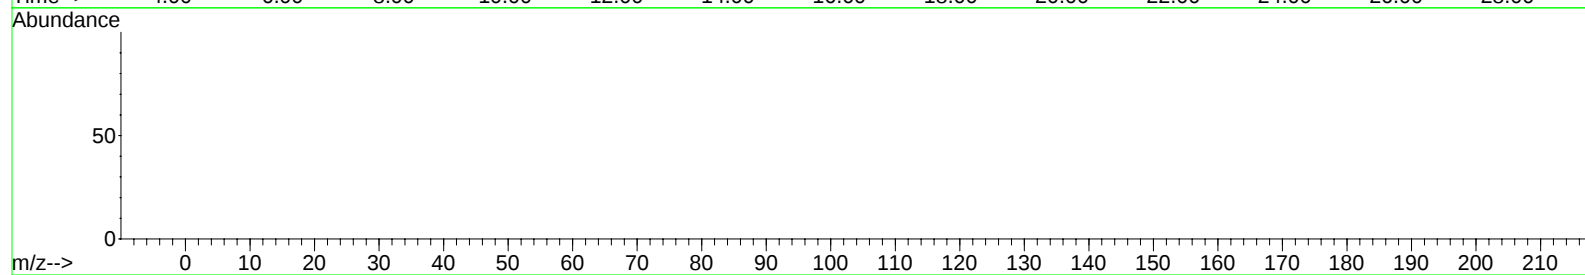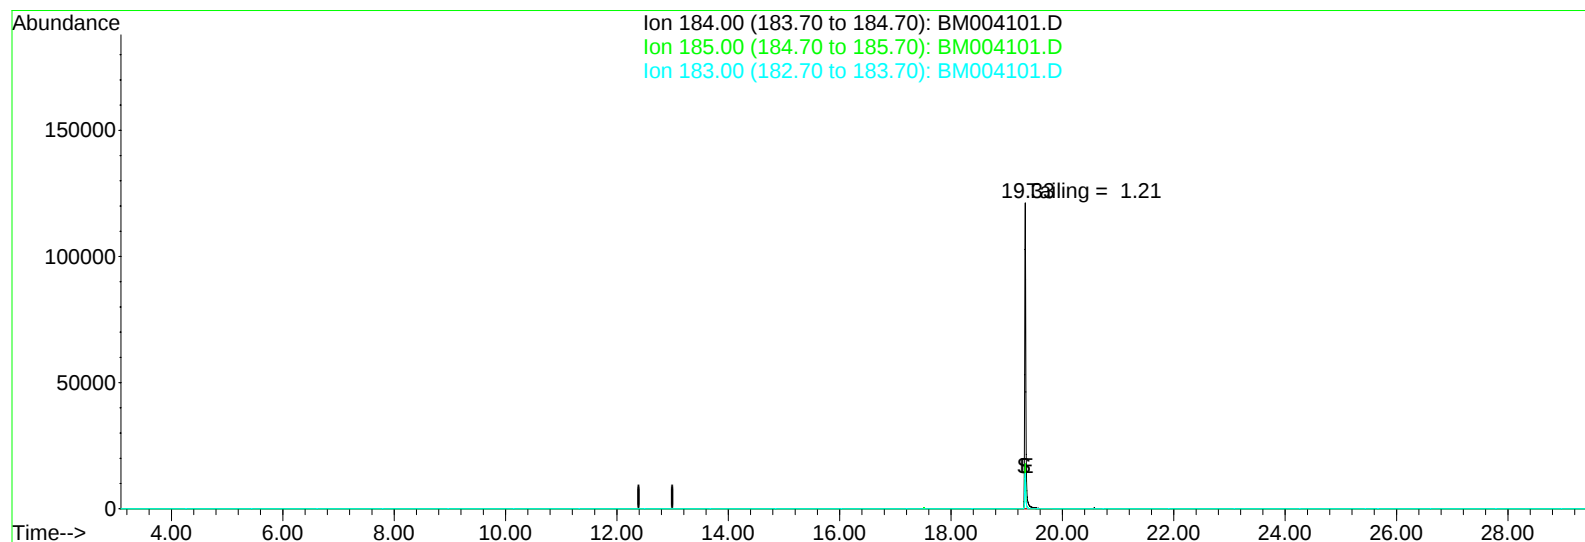

TIC: BM004101.D

(76) Benzidine

12.694min (-12.694) 0.00ng

response 0

Ion	Exp%	Act%
184.00	100	0.00
185.00	15.20	0.00#
183.00	12.30	0.00#
0.00	0.00	0.00