


Data Path : Z:\HPCHEM1\BNA M\DATA\BM012216\
 Data File : BM004101.D
 Acq On : 22 Jan 2016 09:17
 Operator : SJ/UM
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-SIM-BM012216.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 22 14:46:41 2016

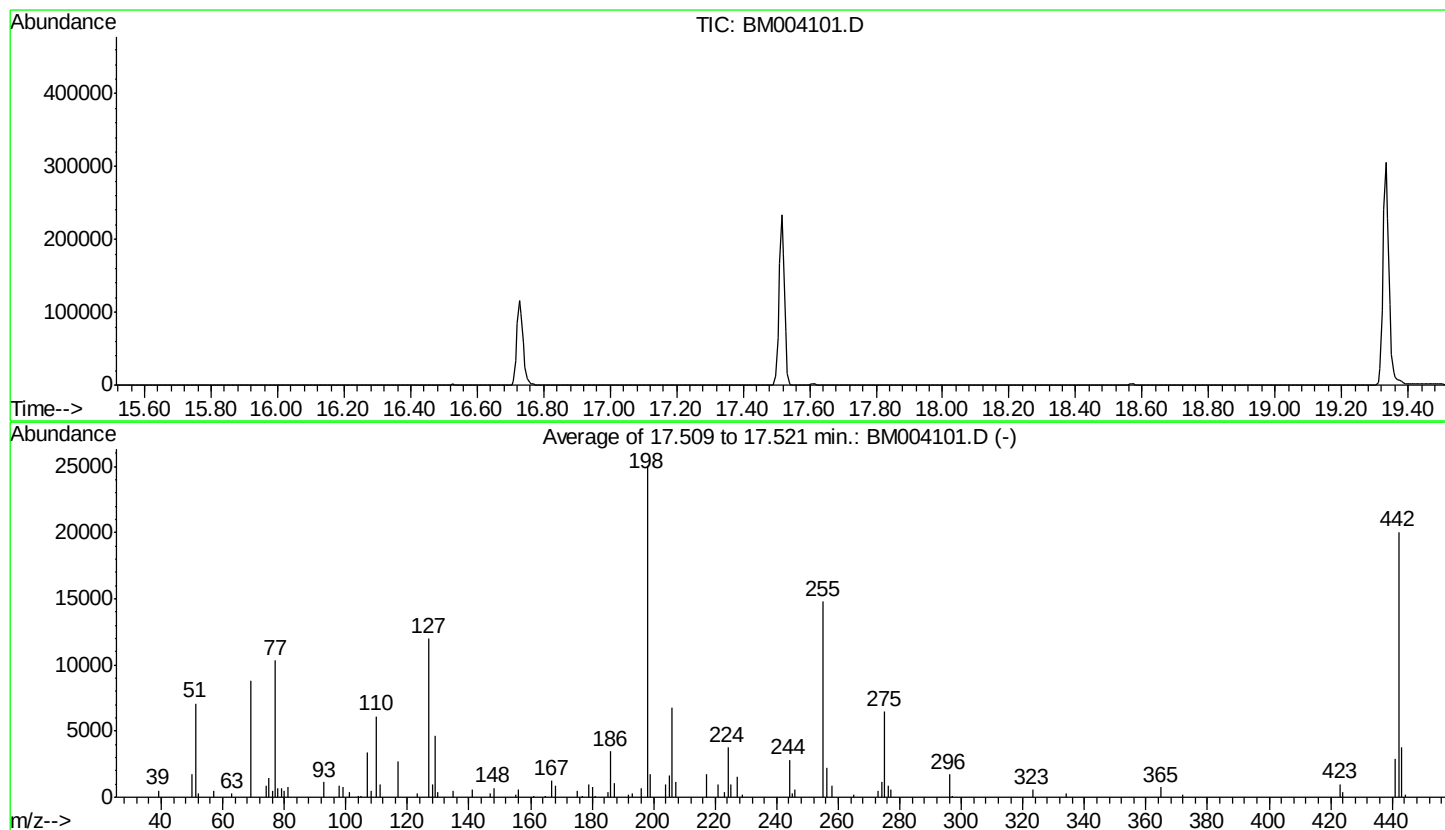

AutoFind: Scans 2452, 2453, 2454; Background Corrected with Scan 2446

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.3	7096	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	35.0	8773	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.7	11952	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	25058	PASS
199	198	5	9	6.9	1725	PASS
275	198	10	60	25.7	6444	PASS
365	198	1	100	3.1	768	PASS
441	442	0.01	24	14.5	2919	PASS
442	198	50	100	80.1	20067	PASS
443	442	15	24	19.0	3817	PASS