

Data Path : U:\HPCHEM1\BNA M\DATA\BM012218\
 Data File : BM013687.D
 Acq On : 22 Jan 2018 11:03
 Operator : SJ/JU
 Sample : PB105818BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Jan 22 14:25:36 2018
 Quant Method : Z:\HPCHEM1\BNA M\Methods\SOM-EPA-BM011018.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jan 22 02:14:14 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.61	152	115047	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	452220	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.26	164	246902	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.02	188	566684	20.00	ng/ul	0.00
75) Chrysene-d12	21.21	240	637892	20.00	ng/ul	0.00
83) Perylene-d12	23.41	264	638883	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.16	96	16163	5.55	ng/uL	0.00
5) Phenol-d5	6.79	99	282559	31.99	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.96	67	173924	32.50	ng/ul	0.00
9) 2-Chlorophenol-d4	7.15	132	230955	32.09	ng/ul	0.00
13) 4-Methylphenol-d8	8.32	113	236810	34.88	ng/ul	0.00
19) Nitrobenzene-d5	8.77	128	120235	34.26	ng/ul	0.00
22) 2-Nitrophenol-d4	9.48	143	128698	34.71	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.02	165	228391	31.88	ng/ul	0.00
29) 4-Chloroaniline-d4	10.54	131	304415	48.98	ng/ul	0.00
43) Dimethylphthalate-d6	13.68	166	740569	36.39	ng/ul	0.00
46) Acenaphthylene-d8	13.95	160	932434	35.93	ng/ul	0.00
51) 4-Nitrophenol-d4	14.49	143	93189	28.18	ng/ul	0.00
57) Fluorene-d10	15.26	176	633038	35.37	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.40	200	95755	28.07	ng/ul	0.00
70) Anthracene-d10	17.12	188	1001295	36.28	ng/ul	0.00
76) Pyrene-d10	19.42	212	1146769	38.61	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.27	264	1160971	39.54	ng/ul	0.00

Target Compounds


				Ovalue	
15) N-Nitroso-di-n-propylamine	8.32	70	6890	1.257	ng/ul# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : U:\HPCHEM1\BNA M\DATA\BM012218\
Data File : BM013687.D
Acq On : 22 Jan 2018 11:03
Operator : SJ/JU
Sample : PB105818BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Jan 22 14:25:36 2018
Quant Method : Z:\HPCHEM1\BNA M\Methods\SOM-EPA-BM011018.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jan 22 02:14:14 2018
Response via : Initial Calibration

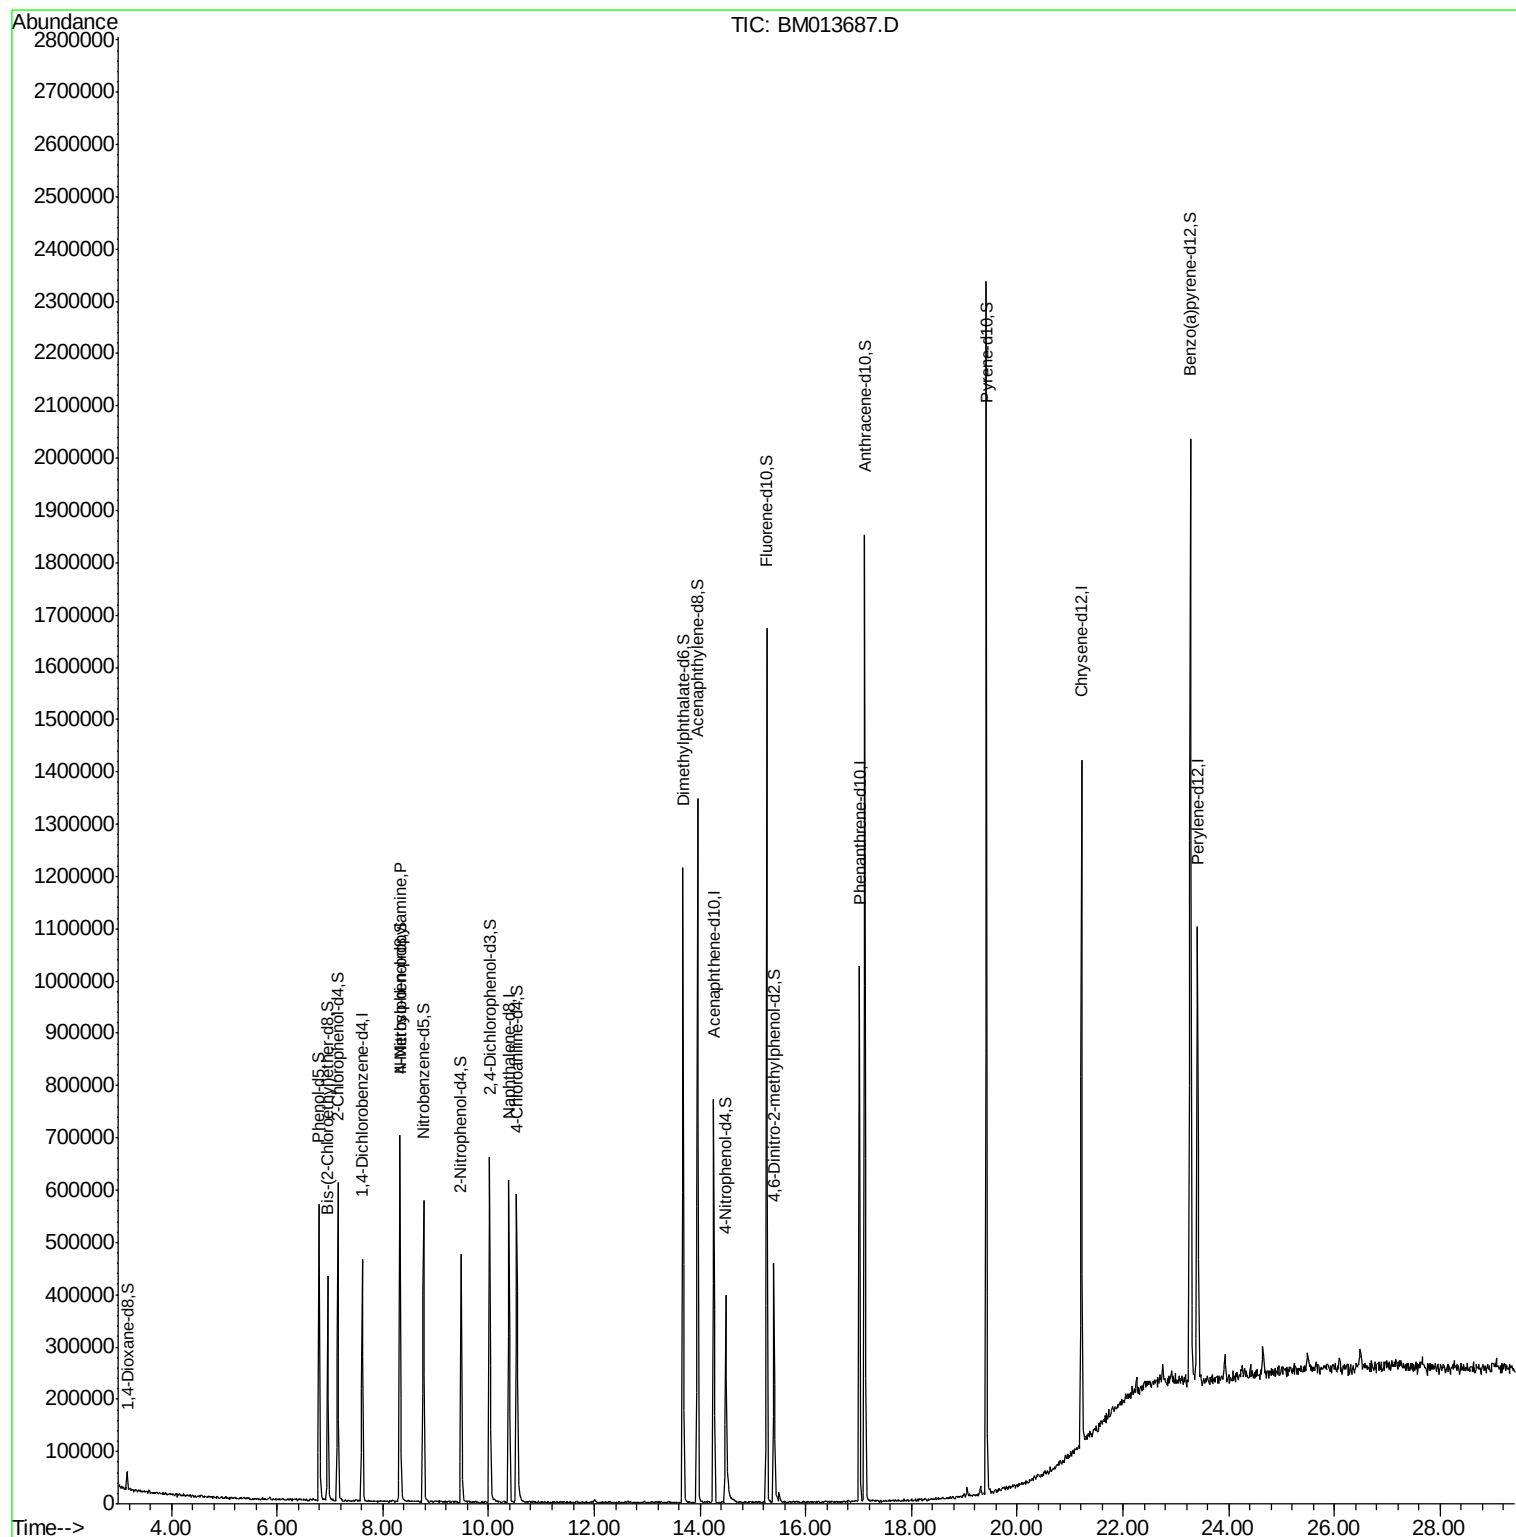

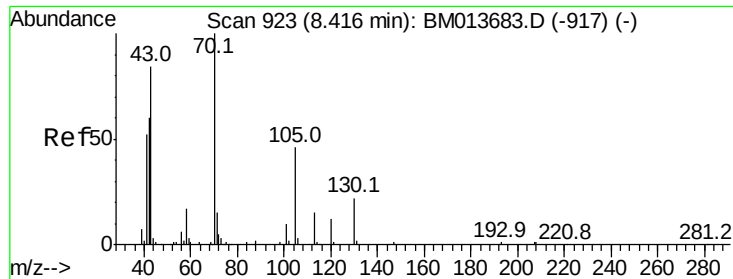

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.257 ng/ul
 RT: 8.32 min Scan# 907
 Delta R.T. -0.10 min
 Lab File: BM013687.D
 Acq: 22 Jan 2018 11:03

Instrument :
 BNA_M
 ClientSampleId :

Tot Ion: 70 Resp: 6890
 Ion Ratio Lower Upper
 70 100
 42 356.5 76.0 114.0#
 101 0.0 6.7 10.1#
 130 0.0 14.6 22.0#

