
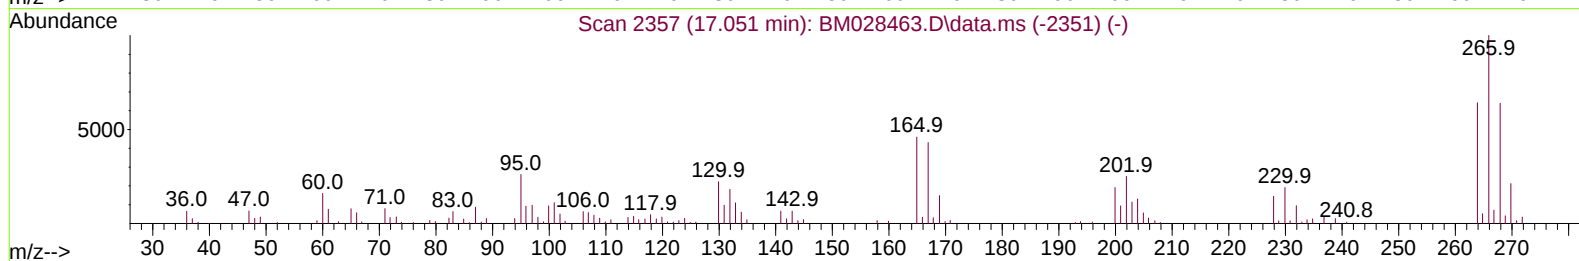
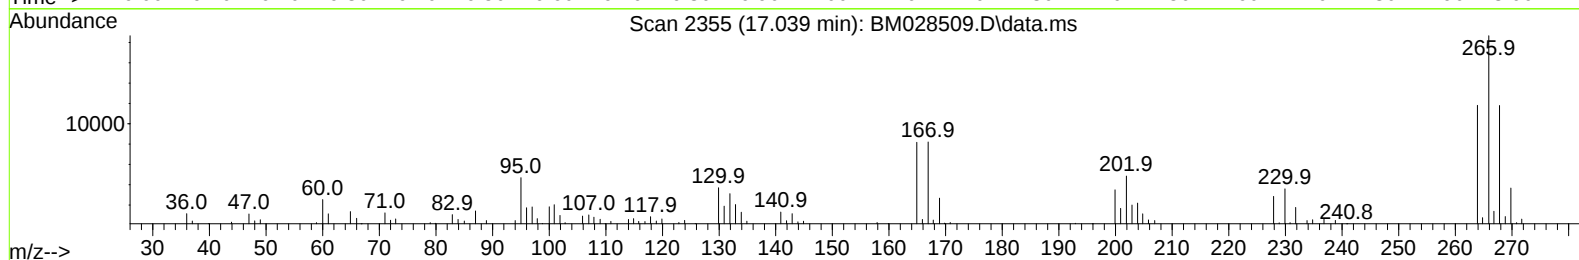


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012221\
Data File : BM028509.D
Acq On : 22 Jan 2021 08:36
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 22 23:27:40 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 22 10:45:04 2021
Response via : Initial Calibration

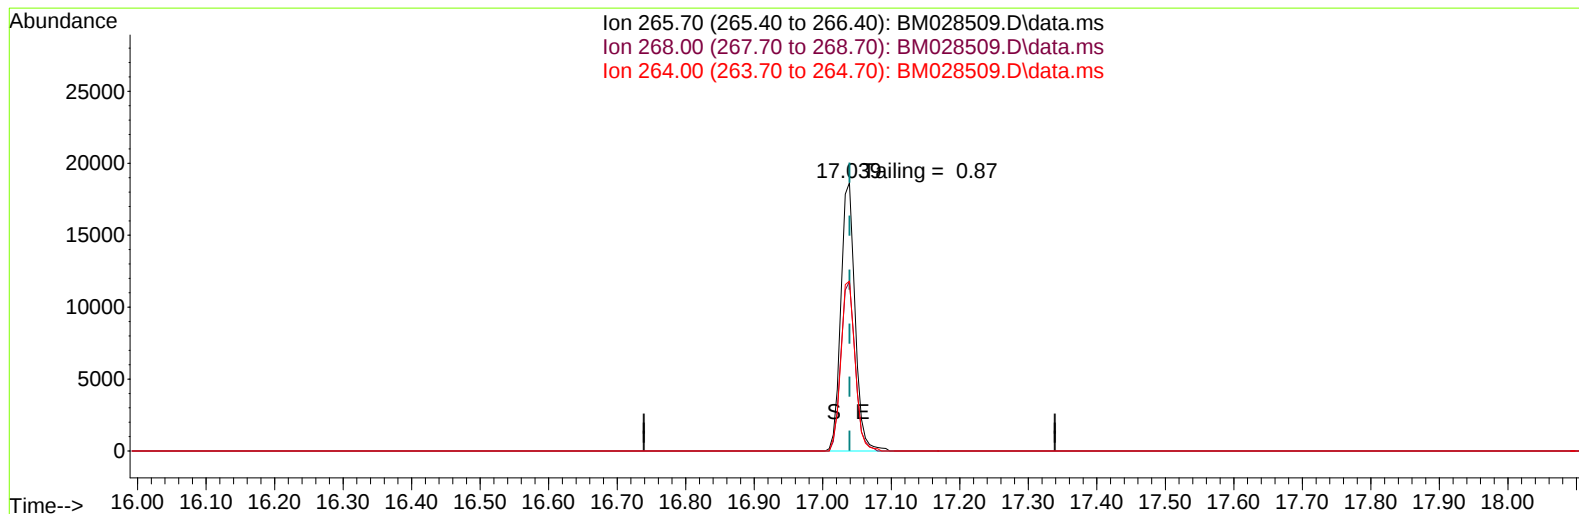

TIC: BM028509.D\data.ms

(70) Pentachlorophenol (C)




17.039min (-0.000) 0.00 ng

response 26852

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	63.21
264.00	63.30	63.32
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012221\
Data File : BM028509.D
Acq On : 22 Jan 2021 08:36
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 22 23:27:40 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 22 10:45:04 2021
Response via : Initial Calibration

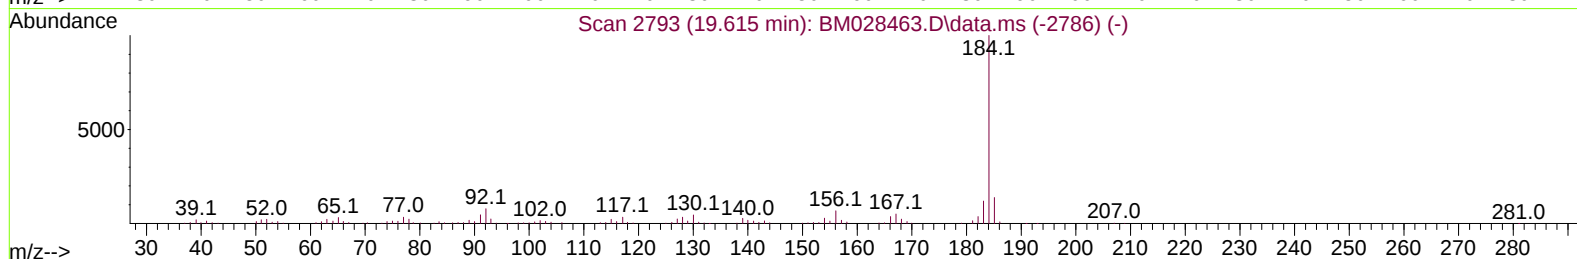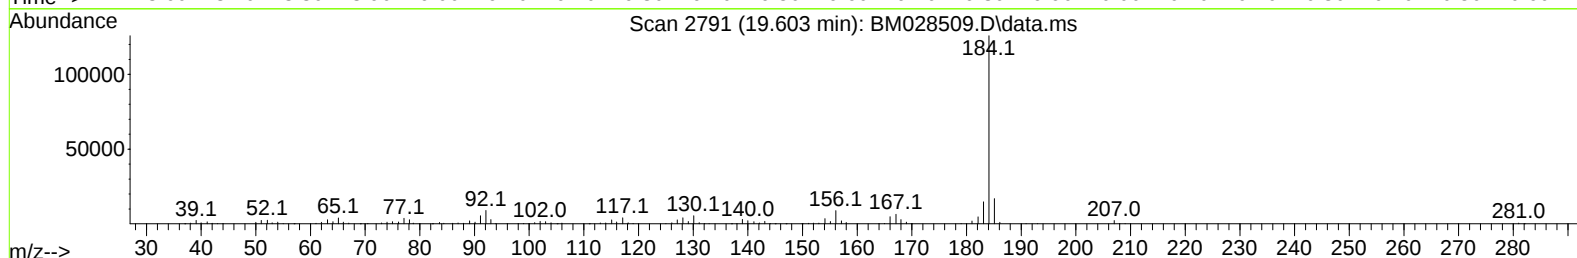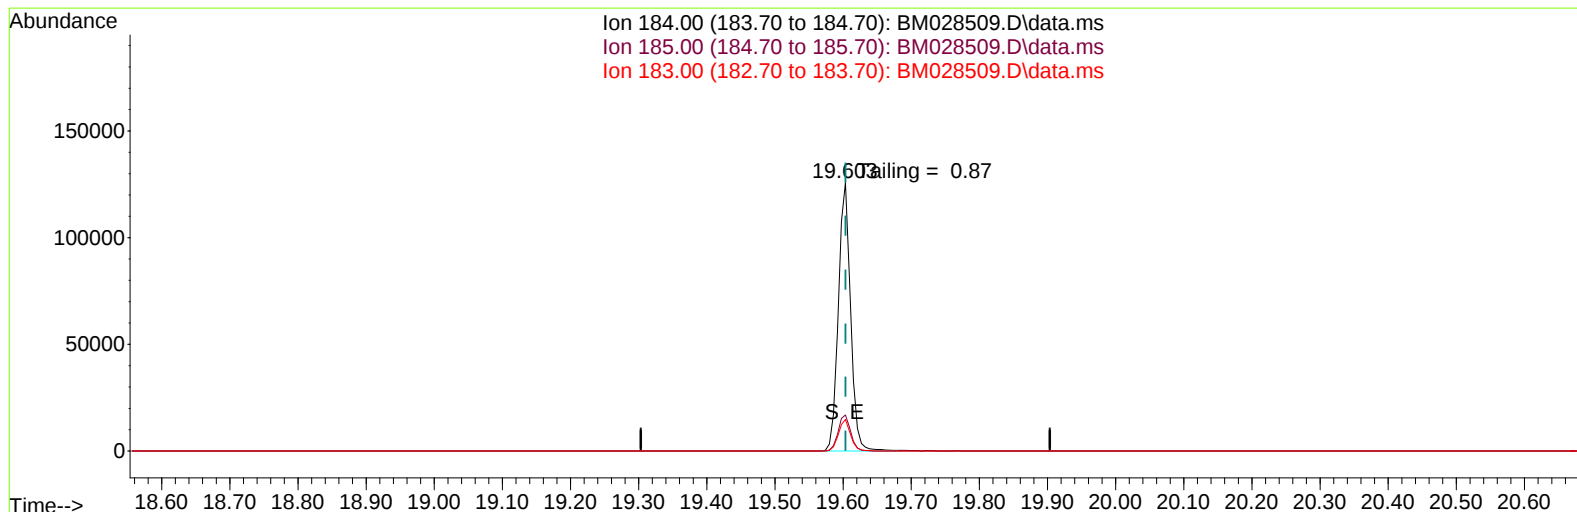

TIC: BM028509.D\data.ms

(77) Benzidine

19.603min (-0.000) 0.00 ng

response 156900

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	13.44
183.00	12.10	11.76
0.00	0.00	0.00