

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012221\
 Data File : BM028511.D
 Acq On : 22 Jan 2021 09:59
 Operator : CG/JU
 Sample : PB134230BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB134230BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM028511.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.540	393	400	410	rVB	432328	629417	29.81%	6.849%
2	7.175	671	678	688	rBV	421016	655562	31.05%	7.134%
3	8.010	814	820	827	rVB	125671	199203	9.43%	2.168%
4	8.340	869	876	884	rBB	579439	911996	43.19%	9.924%
5	9.192	1013	1021	1033	rBV	449025	725298	34.35%	7.893%
6	10.828	1293	1299	1308	rVB	159398	266823	12.64%	2.904%
7	13.286	1710	1717	1728	rBV	1045641	1544159	73.13%	16.804%
8	14.657	1944	1950	1957	rBV	242468	344506	16.32%	3.749%
9	16.139	2196	2202	2213	rBV	449680	637992	30.21%	6.943%
10	17.386	2408	2414	2420	rBV	293187	399189	18.91%	4.344%
11	19.980	2849	2855	2860	rBV	1737037	2111547	100.00%	22.978%
12	21.515	3111	3116	3122	rBV	338004	407310	19.29%	4.432%
13	23.797	3498	3504	3513	rVB2	186205	356340	16.88%	3.878%




Sum of corrected areas: 9189342

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012221\
Data File : BM028511.D
Acq On : 22 Jan 2021 09:59
Operator : CG/JU
Sample : PB134230BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB134230BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

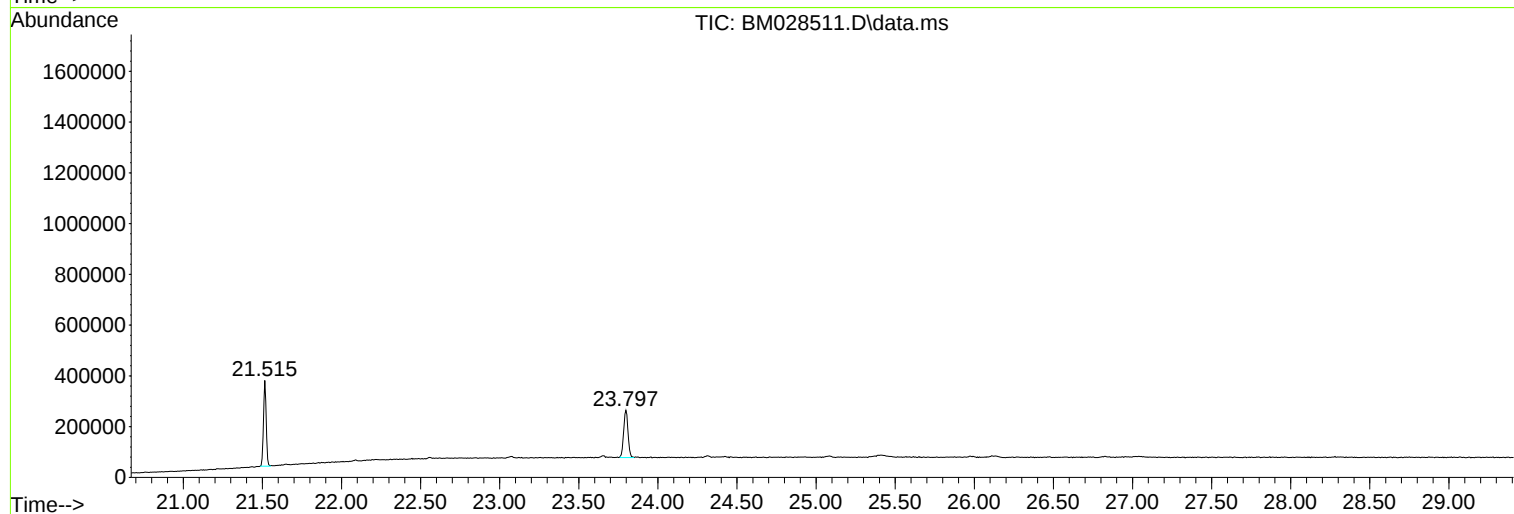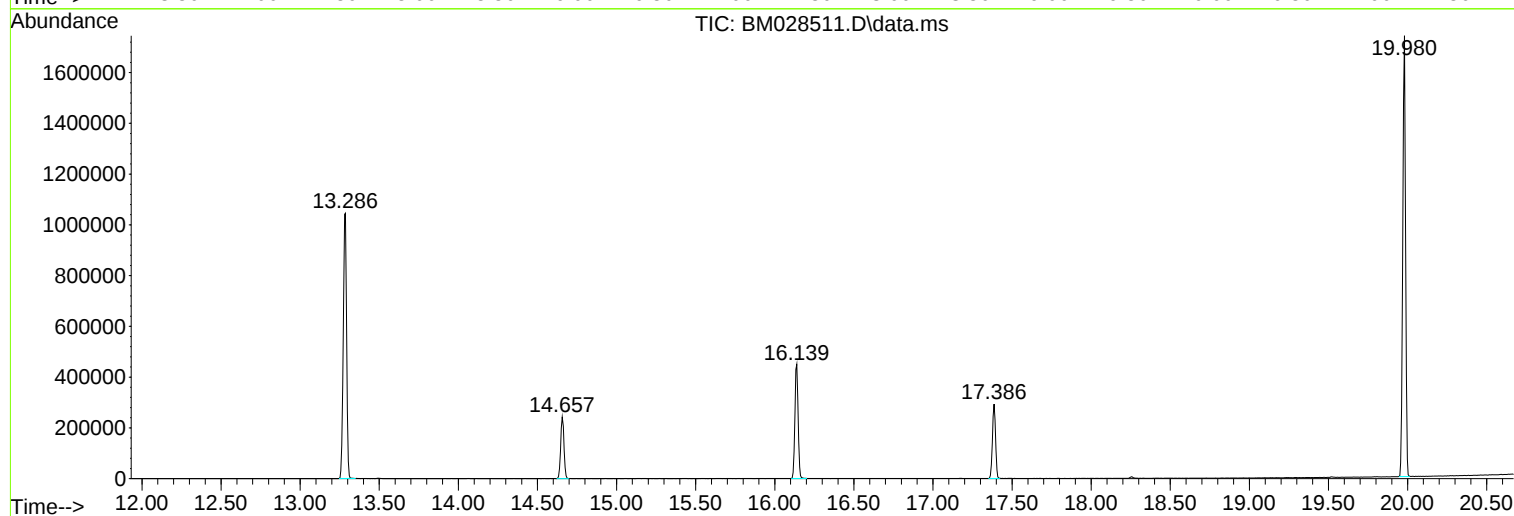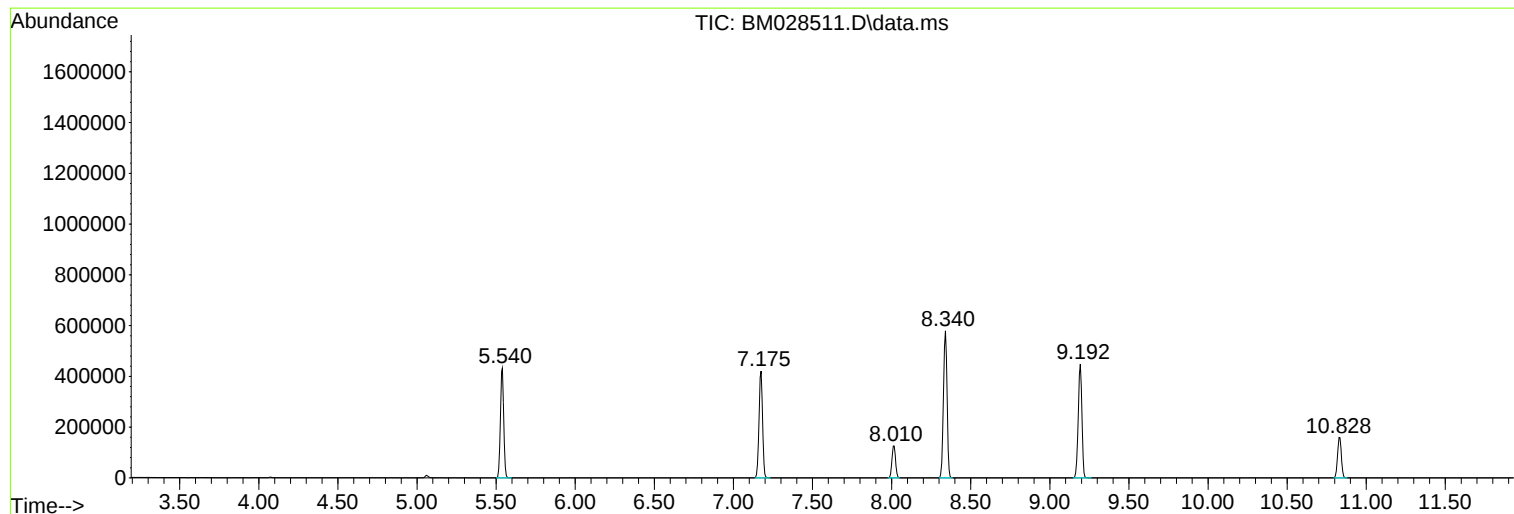

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012221\
Data File : BM028511.D
Acq On : 22 Jan 2021 09:59
Operator : CG/JU
Sample : PB134230BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB134230BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012221\
Data File : BM028511.D
Acq On : 22 Jan 2021 09:59
Operator : CG/JU
Sample : PB134230BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB134230BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------