

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012221\
 Data File : BM028517.D
 Acq On : 22 Jan 2021 14:21
 Operator : CG/JU
 Sample : PB134276BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB134276BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM028517.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.540	393	400	409	rBV	612282	875116	49.08%	10.562%
2	7.175	670	678	689	rBV	588288	915015	51.32%	11.044%
3	8.010	814	820	827	rBB	115898	183678	10.30%	2.217%
4	9.192	1013	1021	1030	rBV	341539	568699	31.90%	6.864%
5	10.828	1292	1299	1306	rBV	154692	255531	14.33%	3.084%
6	13.280	1709	1716	1728	rBV	841904	1198361	67.21%	14.464%
7	14.657	1944	1950	1961	rBV	227850	326881	18.33%	3.945%
8	16.139	2195	2202	2214	rBV	651683	922825	51.76%	11.138%
9	17.386	2408	2414	2420	rBV	271318	385900	21.64%	4.658%
10	19.974	2849	2854	2859	rBV	1407132	1782931	100.00%	21.519%
11	21.515	3111	3116	3123	rBV	364115	445560	24.99%	5.378%
12	23.792	3497	3503	3510	rBV2	228089	424772	23.82%	5.127%




Sum of corrected areas: 8285269

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012221\
Data File : BM028517.D
Acq On : 22 Jan 2021 14:21
Operator : CG/JU
Sample : PB134276BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB134276BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

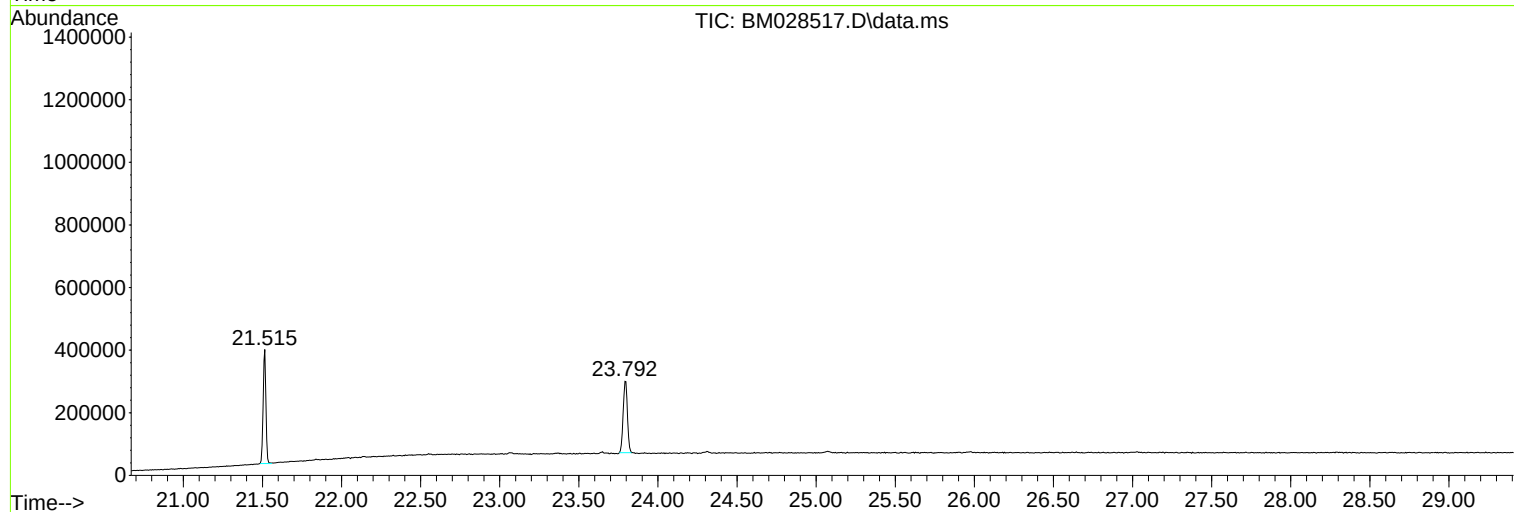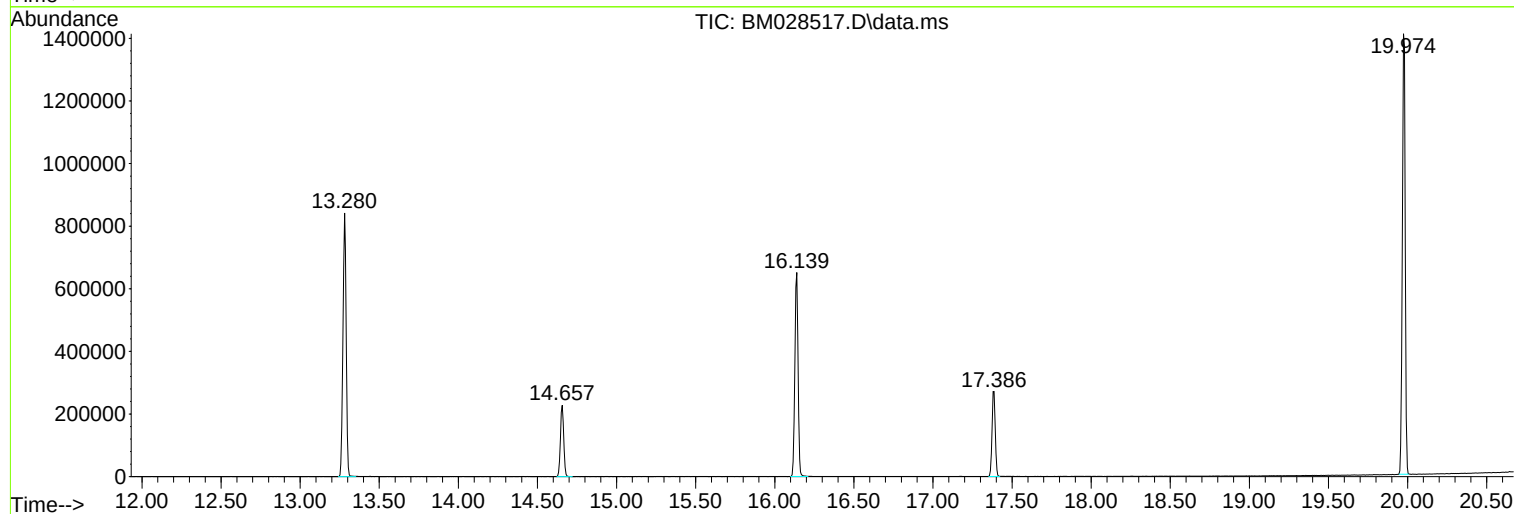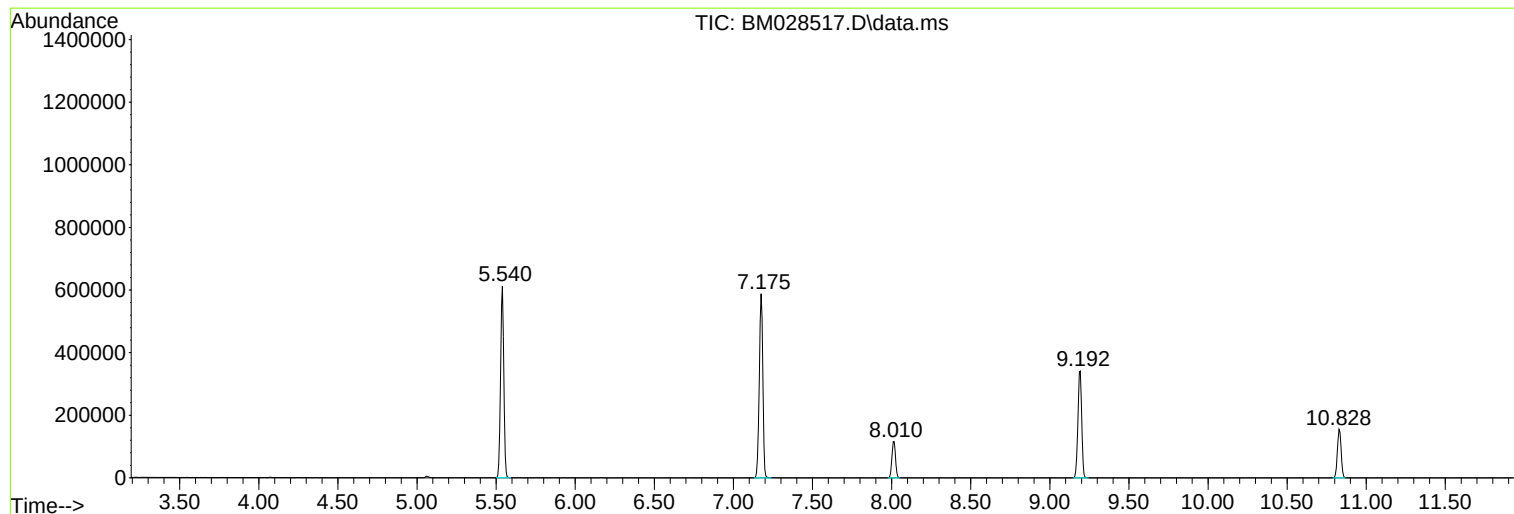

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012221\
Data File : BM028517.D
Acq On : 22 Jan 2021 14:21
Operator : CG/JU
Sample : PB134276BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB134276BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012221\
Data File : BM028517.D
Acq On : 22 Jan 2021 14:21
Operator : CG/JU
Sample : PB134276BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB134276BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------