


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012221\
 Data File : BM028509.D
 Acq On : 22 Jan 2021 08:36
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 22 10:45:04 2021

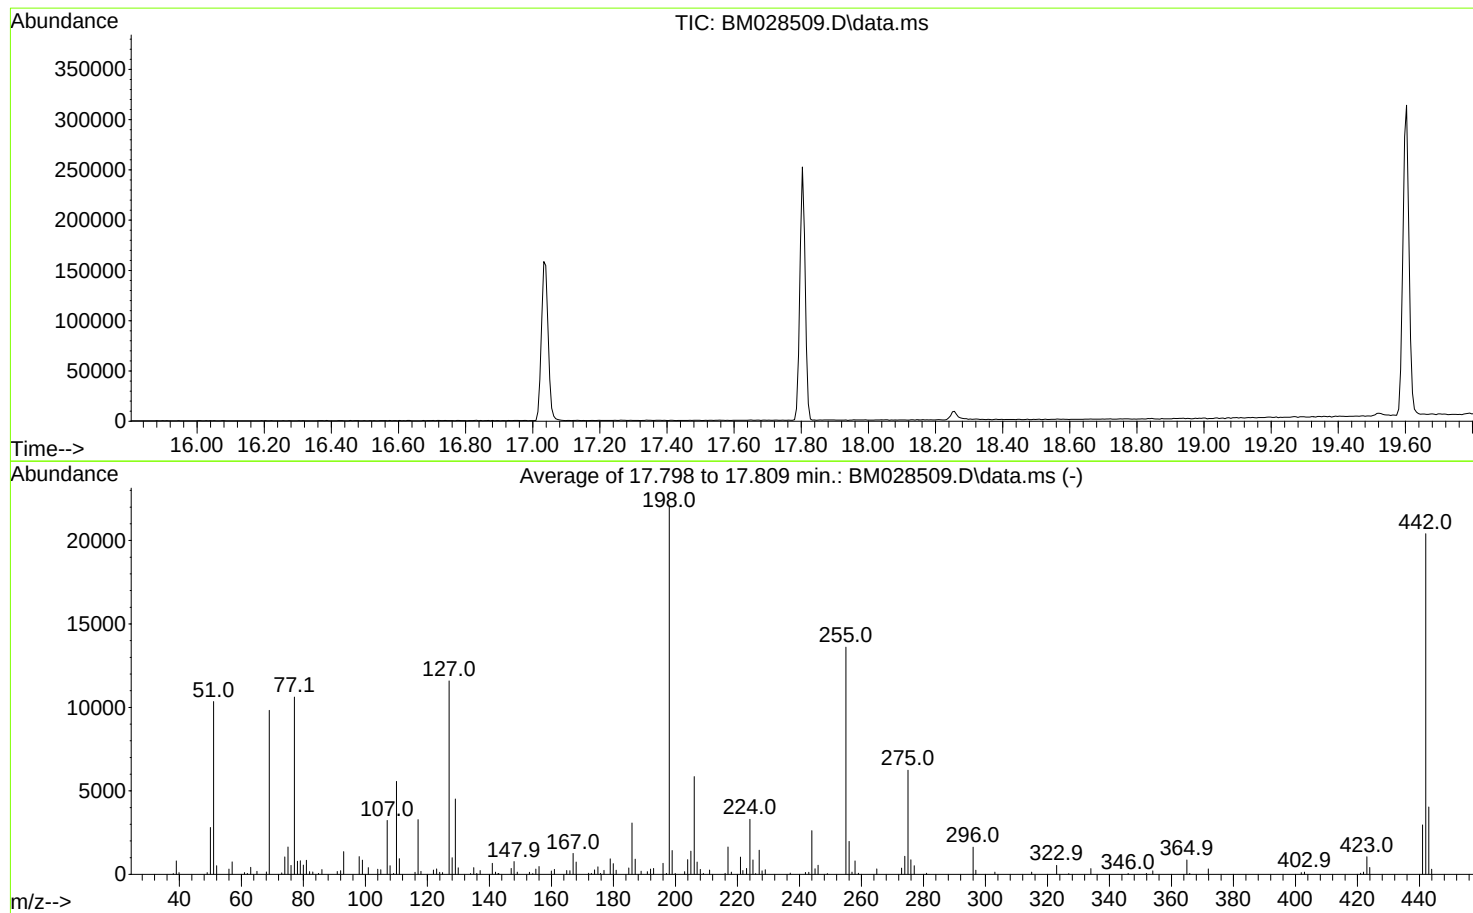

AutoFind: Scans 2484, 2485, 2486; Background Corrected with Scan 2478

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.0	10351	PASS
68	69	0.00	2	1.5	145	PASS
69	198	0.00	100	44.6	9820	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.6	11589	PASS
197	198	0.00	2	0.2	54	PASS
198	198	100	100	100.0	22035	PASS
199	198	5	9	6.5	1432	PASS
275	198	10	60	28.3	6244	PASS
365	198	1	100	3.9	860	PASS
441	198	0.01	100	13.4	2961	PASS
442	198	50	100	92.6	20406	PASS
443	442	15	24	19.8	4037	PASS