

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012224\
 Data File : BM043893.D
 Acq On : 22 Jan 2024 20:19
 Operator : MA/JU
 Sample : PB158503BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK503

Quant Time: Jan 23 00:30:59 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM011924.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 19 22:45:24 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.955	152	3204	0.400	ng/ul	# 0.03
4) Naphthalene-d8	10.837	136	9029	0.400	ng/ul	# 0.07
9) Acenaphthene-d10	0.000	164	0	0.000	ng/ul	-14.58
13) Phenanthrene-d10	17.385	188	8129	0.400	ng/ul	0.03
17) Chrysene-d12	21.550	240	6045	0.400	ng/ul	# 0.01
23) Perylene-d12	23.961	264	7665	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.327	96	3475	0.796	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.448	152	3093	0.270	ng/ul	0.08
18) Fluoranthene-d10	19.387	212	5826	0.292	ng/ul	0.02
Target Compounds						
						Qvalue
5) Naphthalene	10.897	128	650	0.025	ng/ul#	29


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012224\
Data File : BM043893.D
Acq On : 22 Jan 2024 20:19
Operator : MA/JU
Sample : PB158503BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK503

Quant Time: Jan 23 00:30:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM011924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 19 22:45:24 2024
Response via : Initial Calibration

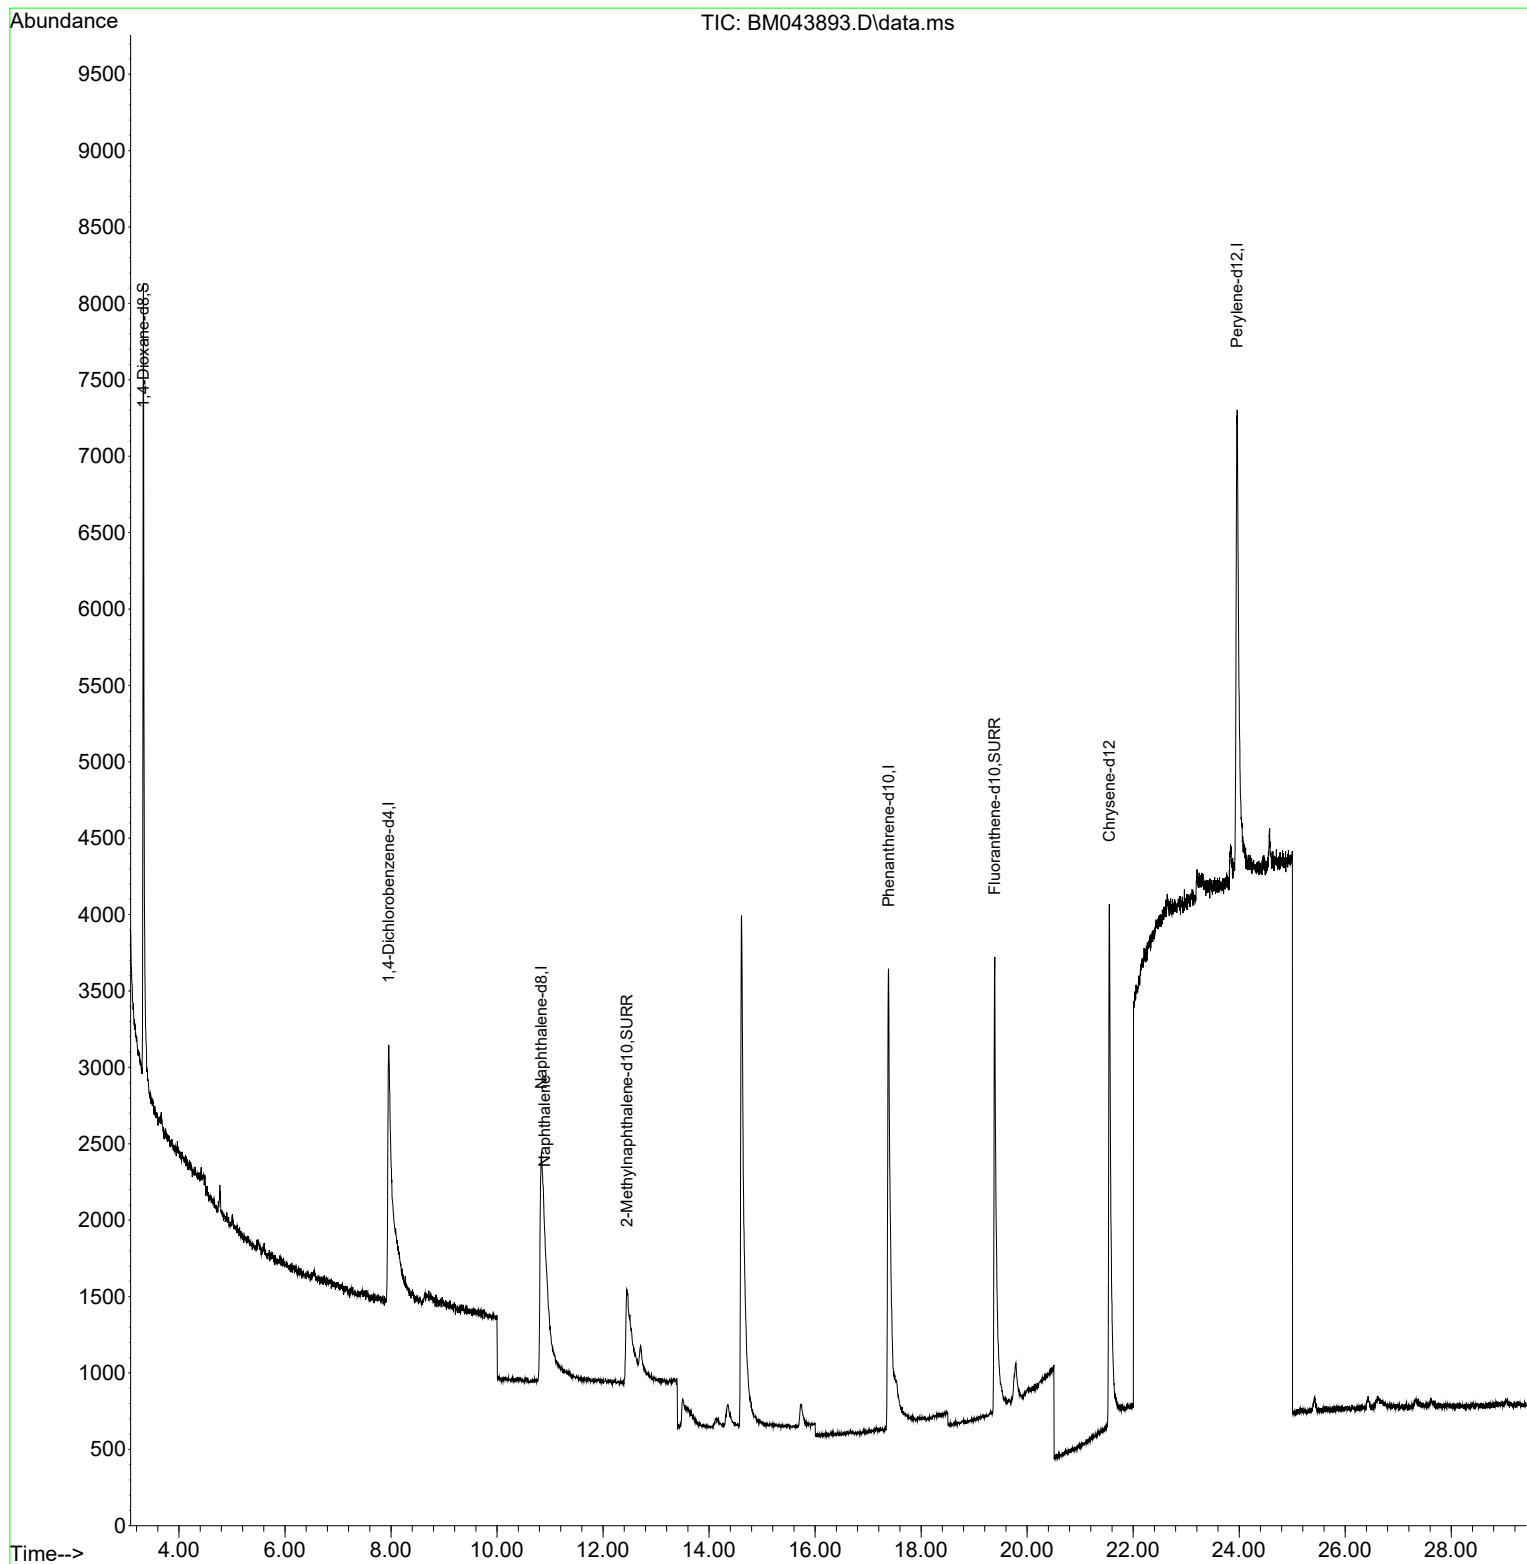

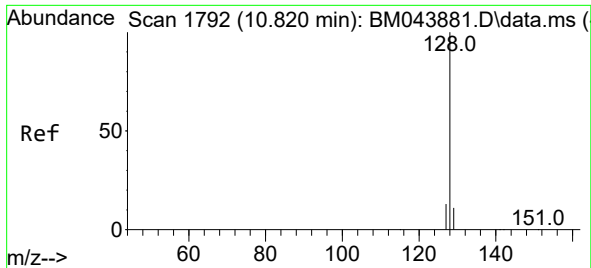

#5
Naphthalene
Concen: 0.025 ng/ul
RT: 10.897 min Scan# 11
Delta R.T. 0.083 min
Lab File: BM043893.D
Acq: 22 Jan 2024 20:19

Instrument :
BNA_M
ClientSampleId :
SBLK503

Tgt Ion:128 Resp: 650
Ion Ratio Lower Upper
128 100
129 44.0 10.0 15.0#
127 40.2 11.4 17.0#

