
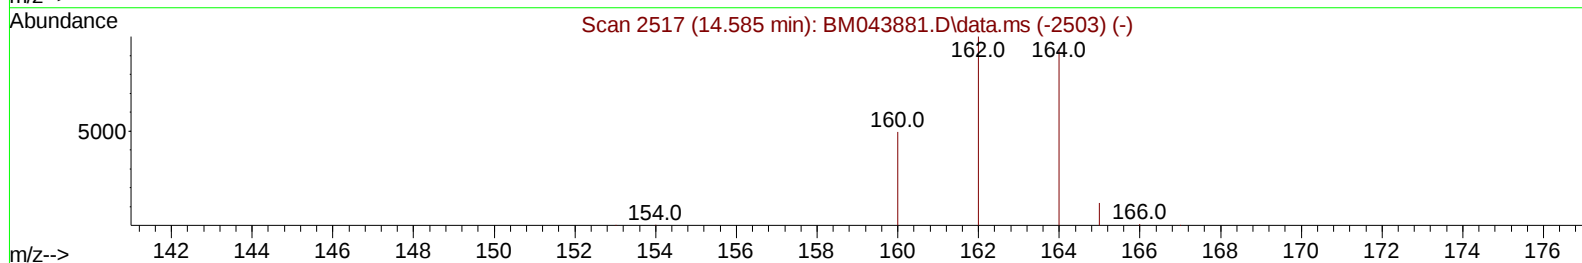
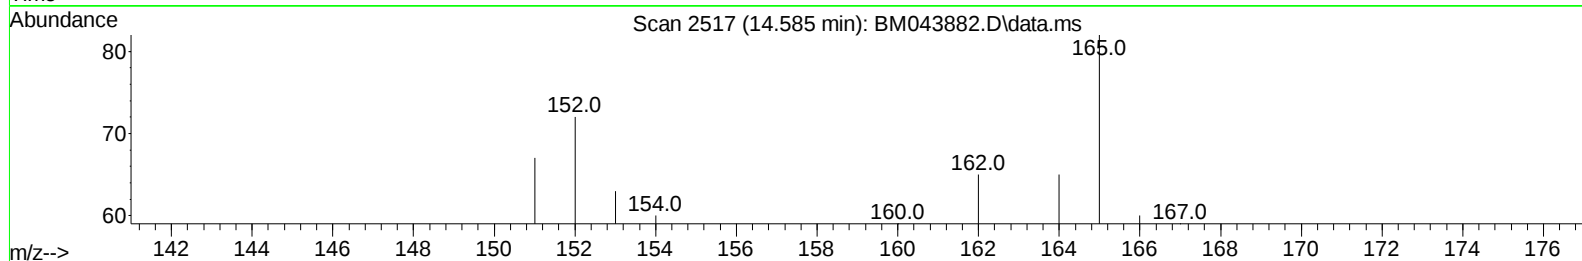


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012224\
Data File : BM043882.D
Acq On : 22 Jan 2024 10:39
Operator : MA/JU
Sample : PB158502BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Jan 23 00:43:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM011924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 19 22:45:24 2024
Response via : Initial Calibration

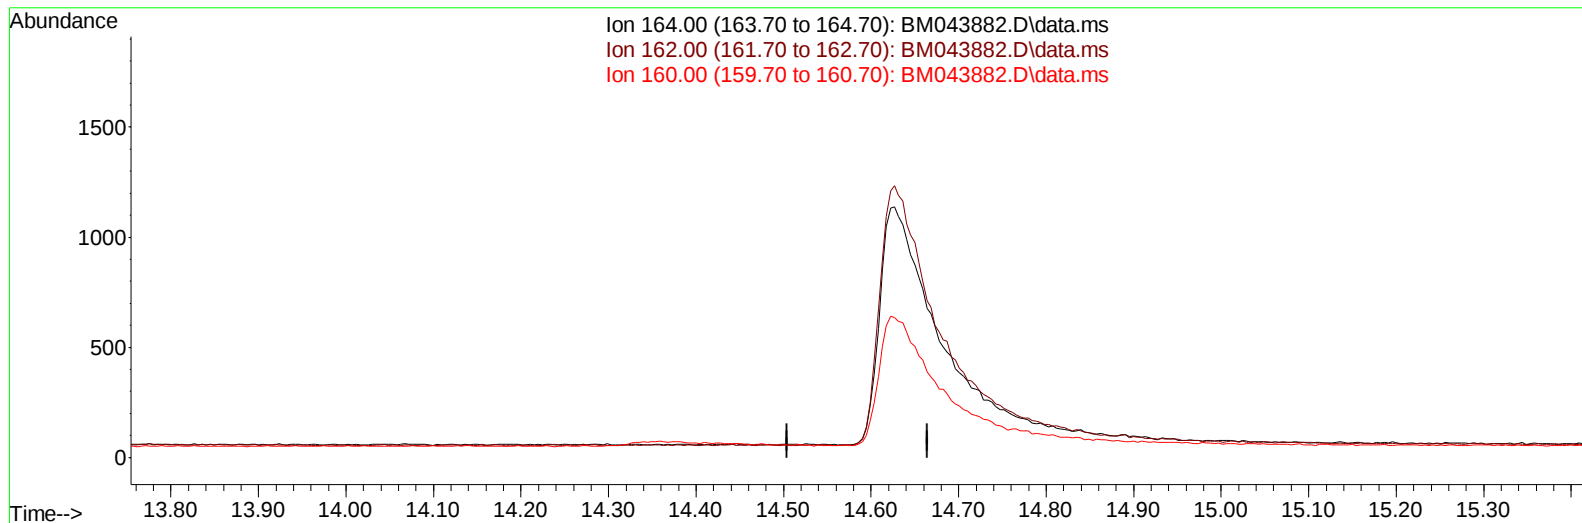

TIC: BM043882.D\data.ms

(9) Acenaphthene-d10 (I)




14.584min (-14.584) 0.00 ng/ul

response 0

Ion	Exp%	Act%
164.00	100.00	0.00
162.00	106.40	0.00#
160.00	52.70	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012224\
Data File : BM043882.D
Acq On : 22 Jan 2024 10:39
Operator : MA/JU
Sample : PB158502BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Jan 23 00:43:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM011924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 19 22:45:24 2024
Response via : Initial Calibration

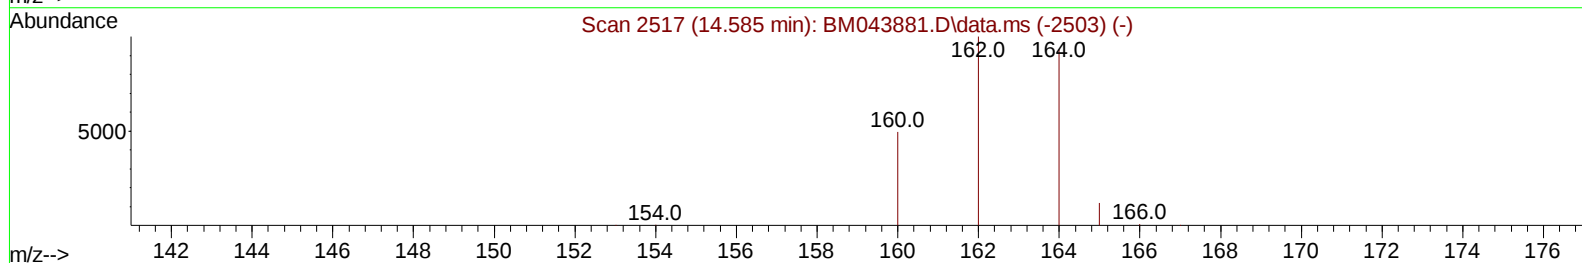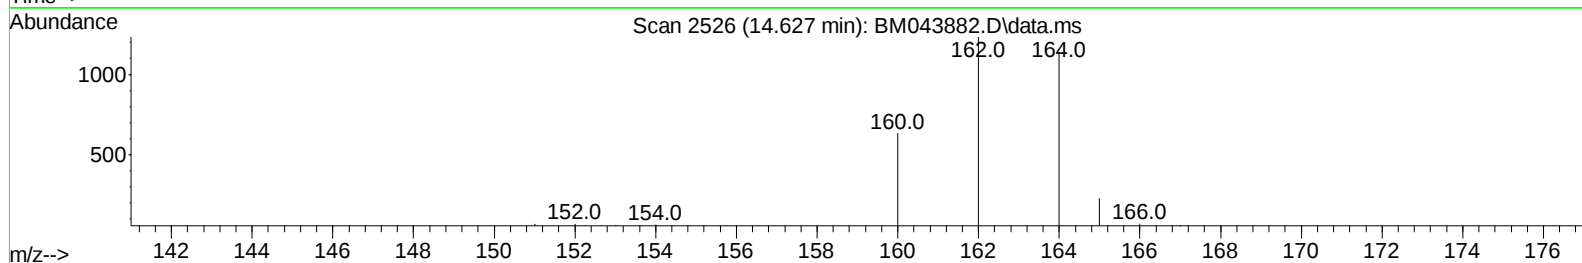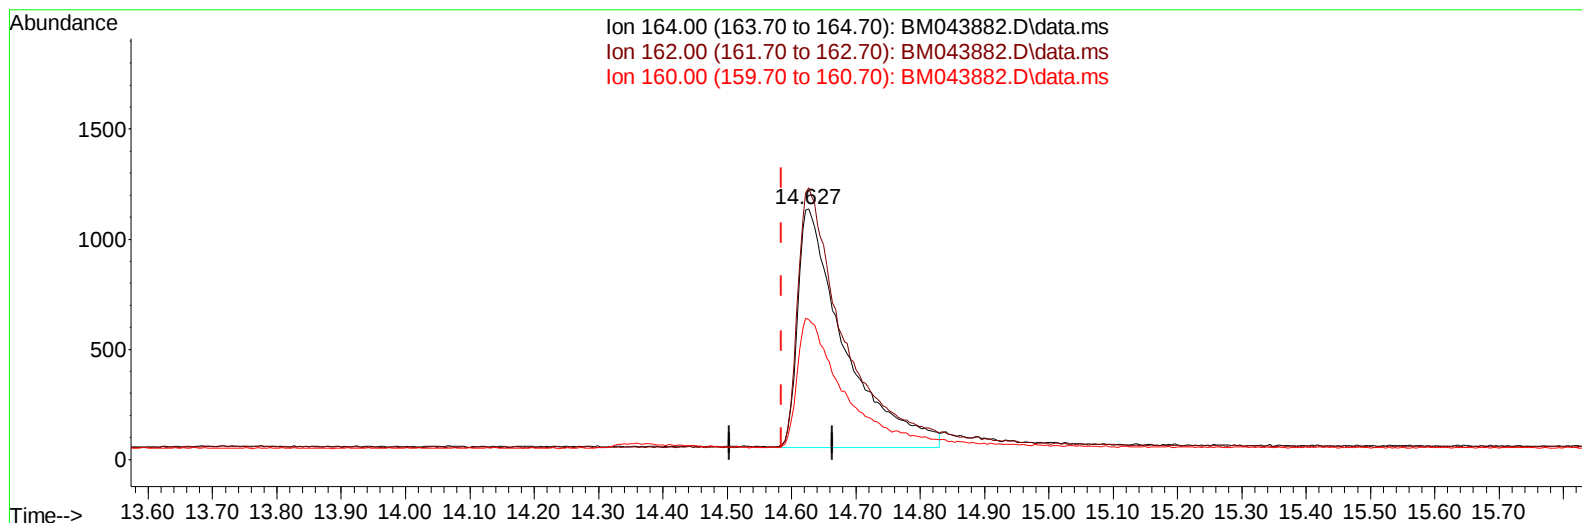

TIC: BM043882.D\data.ms

(9) Acenaphthene-d10 (I)




14.627min (+ 0.042) 0.40 ng/ul m

response 5478

Ion	Exp%	Act%
164.00	100.00	100.00
162.00	106.40	108.44
160.00	52.70	55.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012224\
Data File : BM043882.D
Acq On : 22 Jan 2024 10:39
Operator : MA/JU
Sample : PB158502BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Jan 23 00:43:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM011924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 19 22:45:24 2024
Response via : Initial Calibration

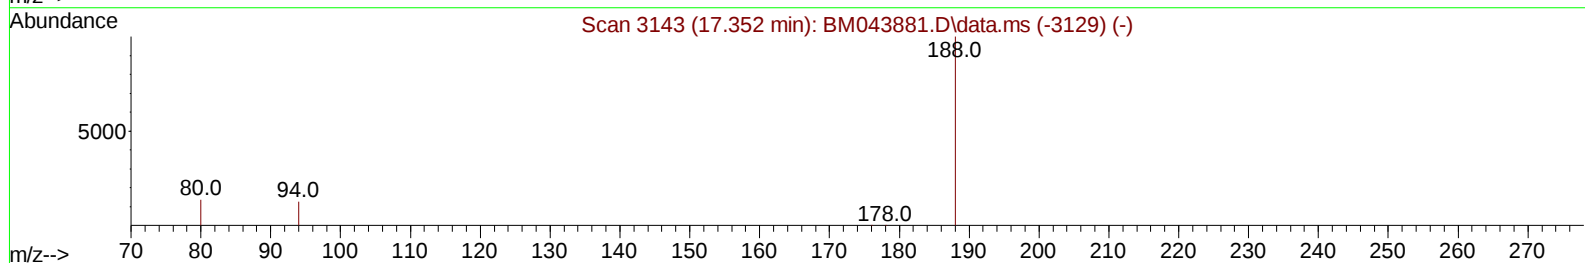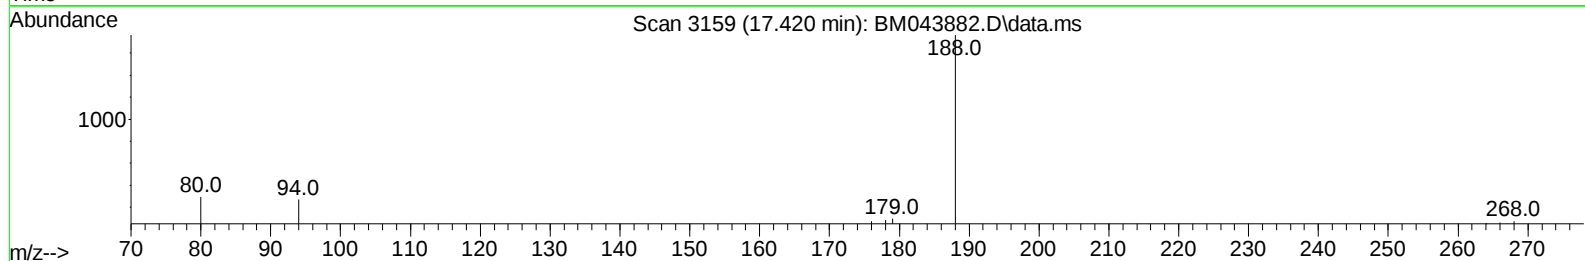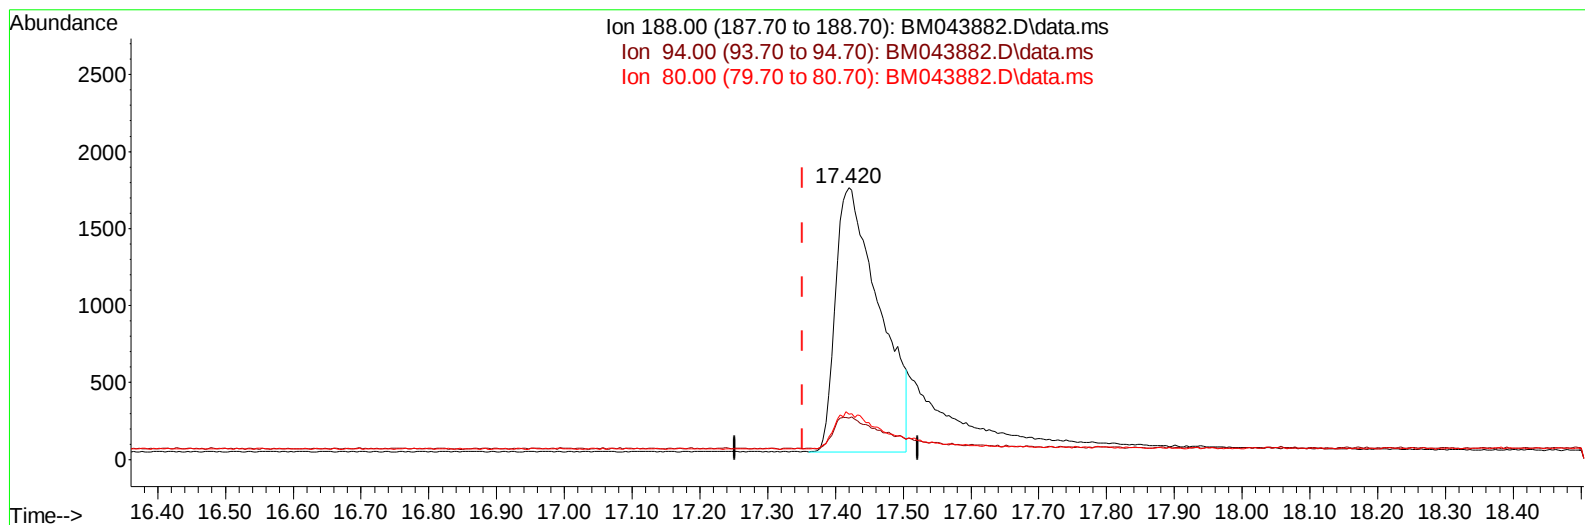

TIC: BM043882.D\data.ms

(13) Phenanthrene-d10 (I)




17.420min (+ 0.068) 0.40 ng/u1

response 7663

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	13.30	15.25
80.00	13.80	16.72#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012224\
Data File : BM043882.D
Acq On : 22 Jan 2024 10:39
Operator : MA/JU
Sample : PB158502BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Jan 23 00:43:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM011924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 19 22:45:24 2024
Response via : Initial Calibration

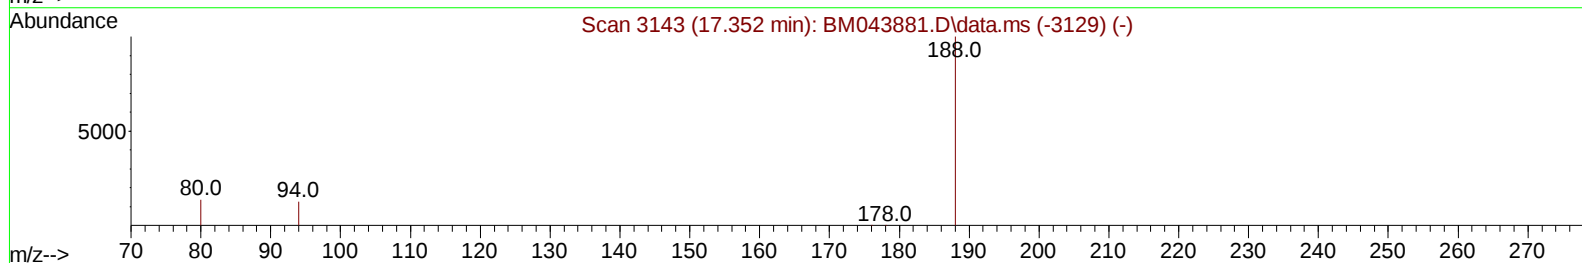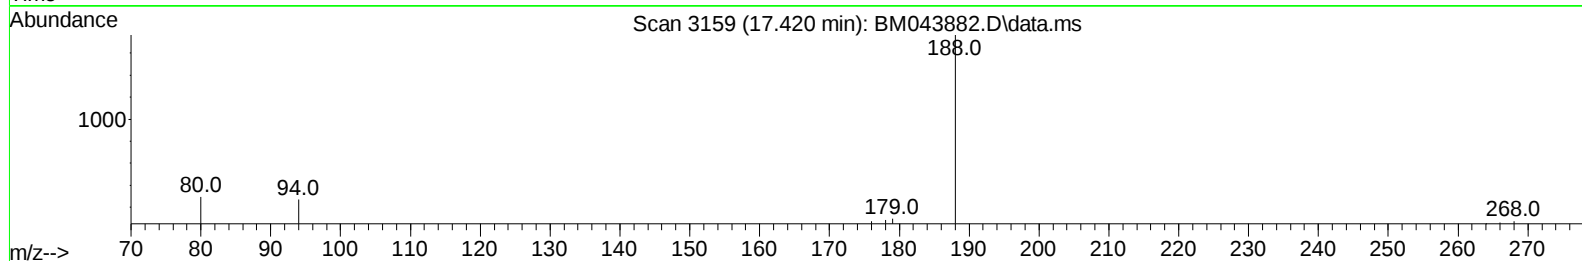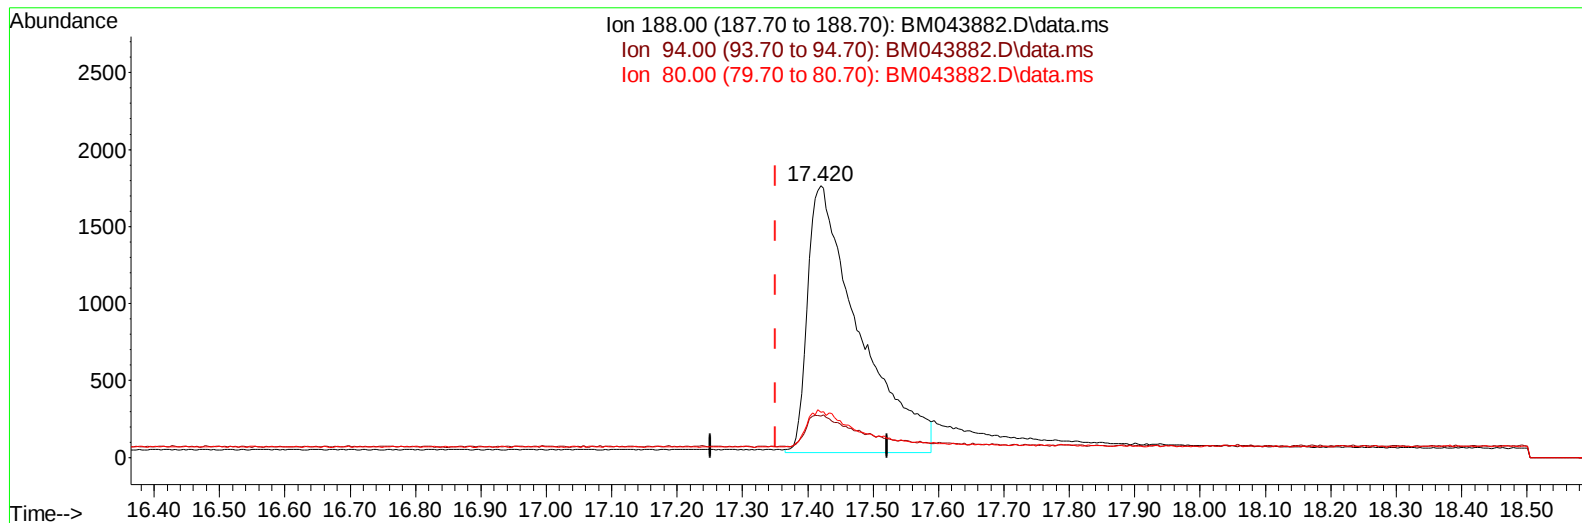

TIC: BM043882.D\data.ms

(13) Phenanthrene-d10 (I)

17.420min (+ 0.068) 0.40 ng/ul m

response 9432

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	13.30	15.25
80.00	13.80	16.72#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012224\
 Data File : BM043882.D
 Acq On : 22 Jan 2024 10:39
 Operator : MA/JU
 Sample : PB158502BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Quant Time: Jan 23 00:43:25 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM011924.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 19 22:45:24 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.976	152	3053	0.400	ng/ul	# 0.05
4) Naphthalene-d8	10.897	136	9572	0.400	ng/ul	# 0.13
9) Acenaphthene-d10	14.627	164	5478m	0.400	ng/ul	0.04
13) Phenanthrene-d10	17.420	188	9432m	0.400	ng/ul	0.07
17) Chrysene-d12	21.560	240	6521	0.400	ng/ul	# 0.03
23) Perylene-d12	23.963	264	8107	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.327	96	4010	0.964	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.492	152	3585	0.295	ng/ul	0.13
18) Fluoranthene-d10	19.411	212	5979	0.278	ng/ul	0.04

Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012224\
Data File : BM043882.D
Acq On : 22 Jan 2024 10:39
Operator : MA/JU
Sample : PB158502BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Jan 23 00:43:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM011924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 19 22:45:24 2024
Response via : Initial Calibration

