
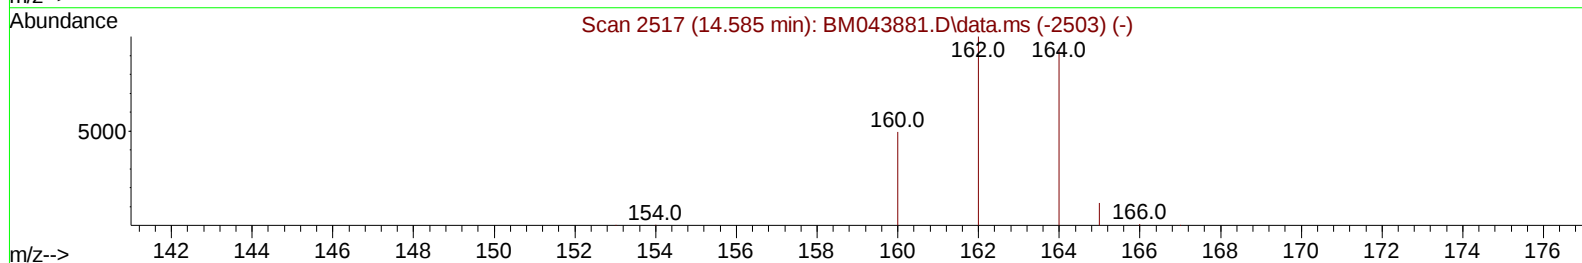
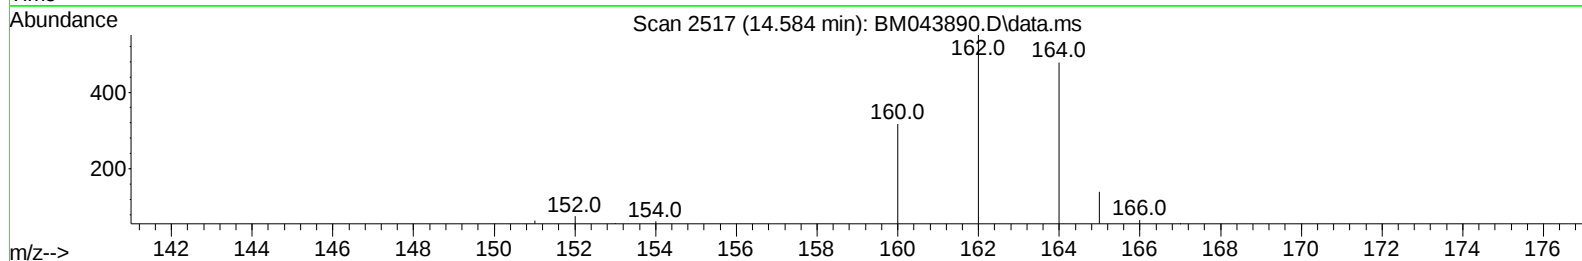


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012224\
Data File : BM043890.D
Acq On : 22 Jan 2024 18:30
Operator : MA/JU
Sample : PB158502BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Quant Time: Jan 23 00:30:28 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM011924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 19 22:45:24 2024
Response via : Initial Calibration

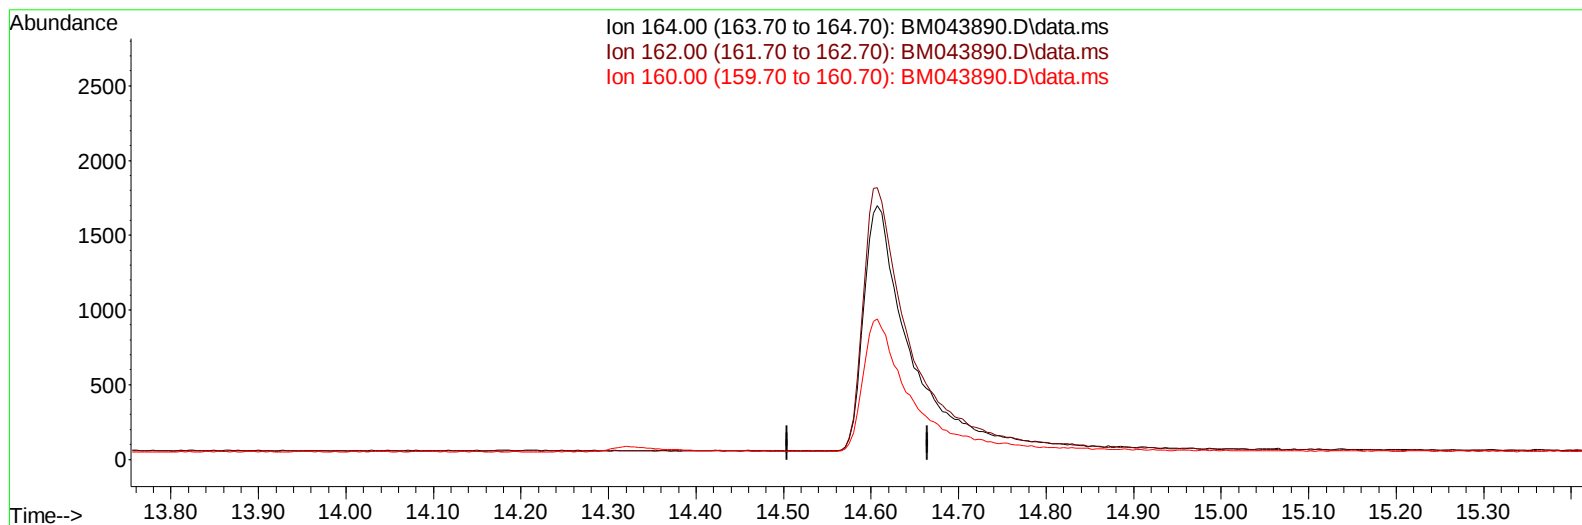

TIC: BM043890.D\data.ms

(9) Acenaphthene-d10 (I)




14.584min (-14.584) 0.00 ng/u1

response 0

Ion	Exp%	Act%
164.00	100.00	0.00
162.00	106.40	0.00#
160.00	52.70	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012224\
Data File : BM043890.D
Acq On : 22 Jan 2024 18:30
Operator : MA/JU
Sample : PB158502BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Quant Time: Jan 23 00:30:28 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM011924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 19 22:45:24 2024
Response via : Initial Calibration

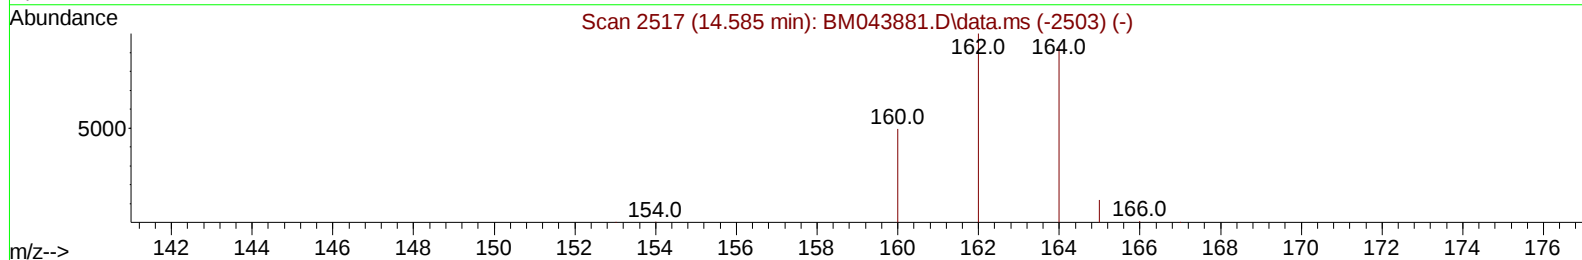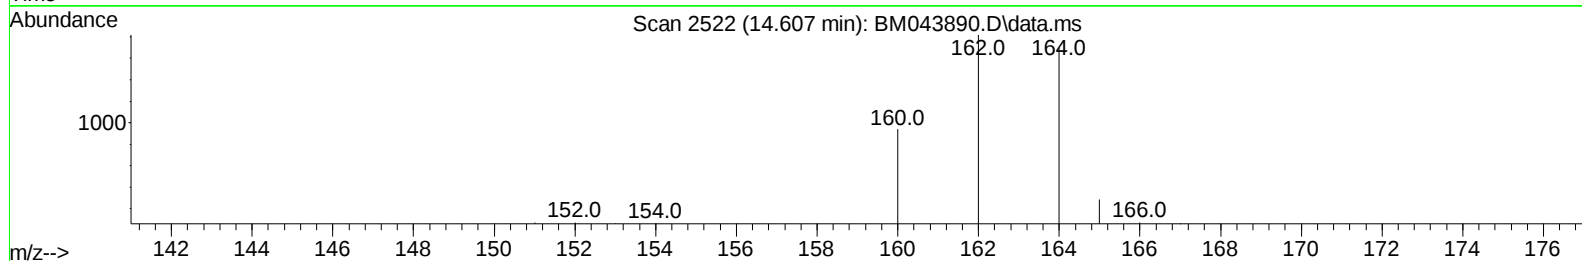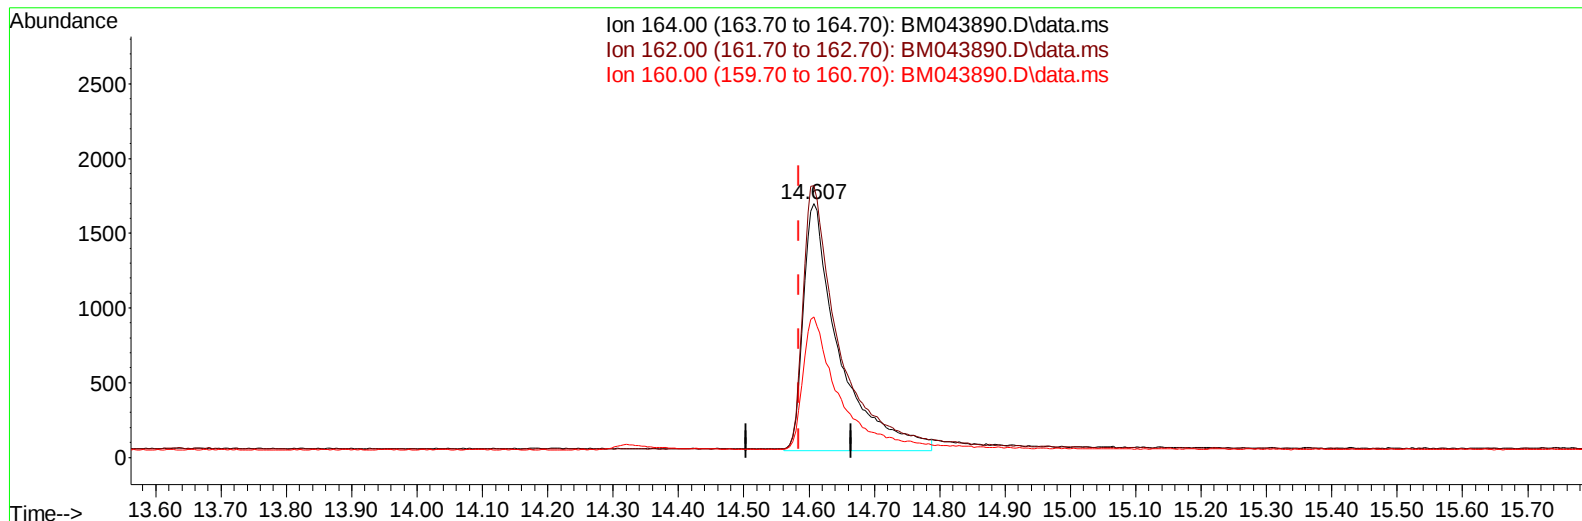

TIC: BM043890.D\data.ms

(9) Acenaphthene-d10 (I)

14.607min (+ 0.023) 0.40 ng/ul m

response 6279

Ion	Exp%	Act%
164.00	100.00	100.00
162.00	106.40	106.95
160.00	52.70	55.33
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012224\
 Data File : BM043890.D
 Acq On : 22 Jan 2024 18:30
 Operator : MA/JU
 Sample : PB158502BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Quant Time: Jan 23 00:30:28 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM011924.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 19 22:45:24 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.951	152	4130	0.400	ng/ul	0.02
4) Naphthalene-d8	10.842	136	11375	0.400	ng/ul #	0.08
9) Acenaphthene-d10	14.607	164	6279m	0.400	ng/ul	0.02
13) Phenanthrene-d10	17.381	188	10151	0.400	ng/ul	0.03
17) Chrysene-d12	21.546	240	7741	0.400	ng/ul	0.01
23) Perylene-d12	23.952	264	10283	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.327	96	3938	0.700	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.442	152	3764	0.260	ng/ul	0.08
18) Fluoranthene-d10	19.391	212	6547	0.257	ng/ul	0.02

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012224\
Data File : BM043890.D
Acq On : 22 Jan 2024 18:30
Operator : MA/JU
Sample : PB158502BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Quant Time: Jan 23 00:30:28 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM011924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 19 22:45:24 2024
Response via : Initial Calibration

